

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW053124\
 Data File : VW028948.D
 Acq On : 31 May 2024 17:13
 Operator : SY/MD
 Sample : P2647-22
 Misc : 3.63g/10mL/MSVOA_W/SOIL/B
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BHBT6

Quant Time: Jun 01 00:36:19 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 01 00:30:04 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	331958	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	270103	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.555	152	81428	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.362	65	102825	16.312	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	65.240%
7) Chloroethane-d5	2.899	69	95481	19.782	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	79.120%
11) 1,1-Dichloroethene-d2	4.021	65	48651	18.473	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.880%
21) 2-Butanone-d5	7.081	46	54291	33.012	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.020%
24) Chloroform-d	7.648	84	244594	23.581	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.320%
26) 1,2-Dichloroethane-d4	8.306	65	141494	23.827	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	95.320%
32) Benzene-d6	8.276	84	433240	24.041	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.160%
36) 1,2-Dichloropropane-d6	9.270	67	155106	28.603	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	114.400%
41) Toluene-d8	10.324	98	344811	21.606	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.440%
43) trans-1,3-Dichloroprop...	10.574	79	38178	17.501	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.000%
47) 2-Hexanone-d5	10.922	63	30688	32.812	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	65.620%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	100042	22.001	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	88.000%
66) 1,2-Dichlorobenzene-d4	13.848	152	65522	21.112	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.440%
Target Compounds						Qvalue
16) Methylene chloride	4.929	84	14188	2.764	ug/L	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW053124\
Data File : VW028948.D
Acq On : 31 May 2024 17:13
Operator : SY/MD
Sample : P2647-22
Misc : 3.63g/10mL/MSVOA_W/SOIL/B
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BHBT6


Quant Time: Jun 01 00:36:19 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM050224SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 01 00:30:04 2024
Response via : Initial Calibration

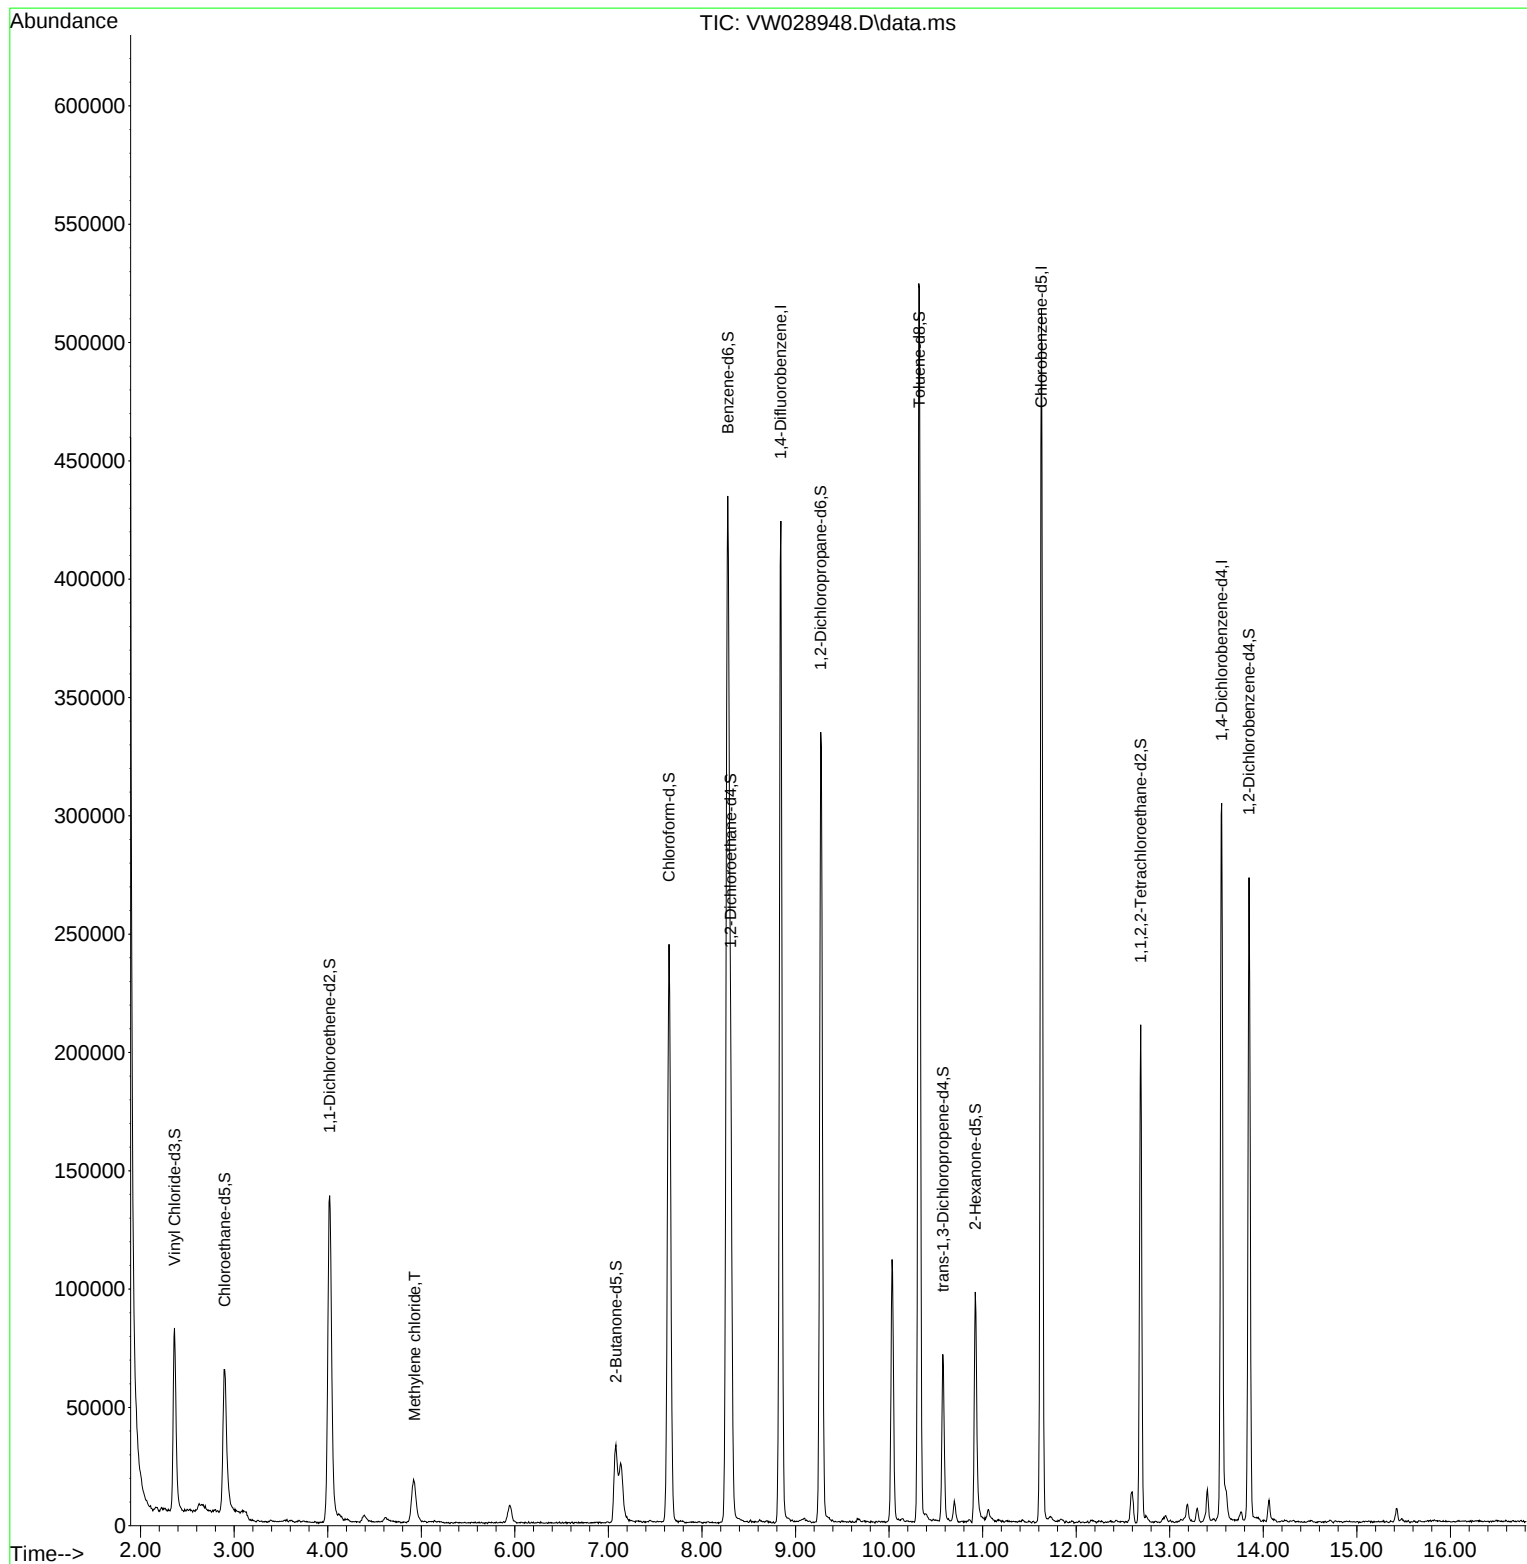

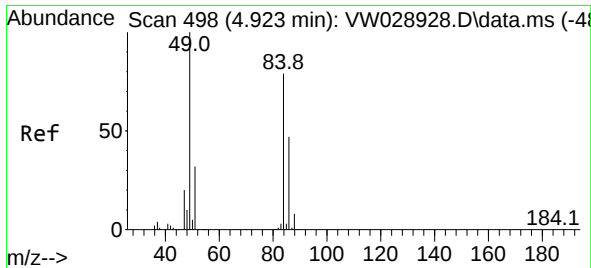

#16
Methylene chloride
Concen: 2.764 ug/L
RT: 4.929 min Scan# 49
Delta R.T. 0.006 min
Lab File: VW028948.D
Acq: 31 May 2024 17:13

Instrument :
MSVOA_W
ClientSampleId :
BHBT6

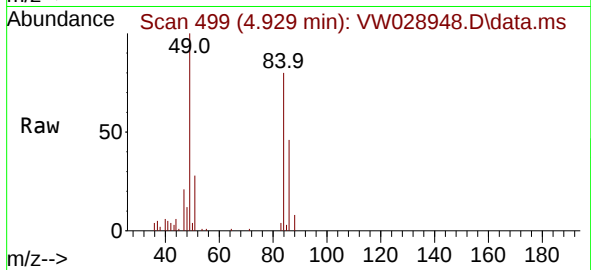

Tgt Ion: 84 Resp: 14188

Ion	Ratio	Lower	Upper
84	100		
86	57.1	44.4	82.4
49	125.3	100.2	186.2

