

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060221\
 Data File : VW019101.D
 Acq On : 02 Jun 2021 15:12
 Operator : SY/VA
 Sample : M2558-06
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 X3552

Manual Integrations
 APPROVED

MMDadoda
 6/4/2021 1:14:14 PM

Quant Time: Jun 03 01:24:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 02 12:40:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	659680	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.633	117	597678	25.00	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	309871	25.00	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	215215	24.67	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.68%
7) Chloroethane-d5	2.891	69	181658	24.45	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.80%
11) 1,1-Dichloroethene-d2	4.025	63	377465	21.78	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	87.12%
21) 2-Butanone-d5	7.073	46	118737	51.96	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.92%
24) Chloroform-d	7.646	84	432889	24.41	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	97.64%
26) 1,2-Dichloroethane-d4	8.305	65	241577m	24.28	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	97.12%
32) Benzene-d6	8.274	84	859933	25.25	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.00%
36) 1,2-Dichloropropane-d6	9.274	67	259054	25.09	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	100.36%
41) Toluene-d8	10.323	98	784540	25.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.36%
43) trans-1,3-Dichloroprop...	10.579	79	111221	24.88	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	99.52%
47) 2-Hexanone-d5	10.926	63	95885	54.77	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.54%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	216816	25.46	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.84%
66) 1,2-Dichlorobenzene-d4	13.853	152	264099	24.42	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	97.68%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	2.013	85	79677	9.32	ug/L	98
3) Chloromethane	2.214	50	86931	11.00	ug/L	99
5) Vinyl chloride	2.367	62	272955	22.63	ug/L	99
6) Bromomethane	2.781	94	107131	11.94	ug/L	100
8) Chloroethane	2.928	64	60872	8.49	ug/L	99
9) Trichlorofluoromethane	3.257	101	63363	9.57	ug/L	100
10) 1,1,2-Trichloro-1,2,2-...	4.068	101	190243	20.09	ug/L	97
12) 1,1-Dichloroethene	4.049	96	136551	14.60	ug/L	92
15) Methyl Acetate	4.665	43	104372	25.63	ug/L	97
16) Methylene chloride	4.921	84	215353	17.59	ug/L	95
18) Methyl tert-butyl Ether	5.421	73	536730	41.20	ug/L	98
22) 2-Butanone	7.171	43	221928	81.98	ug/L	98
25) Chloroform	7.677	83	351530	19.27	ug/L	100
29) Cyclohexane	7.957	56	320300	20.59	ug/L	98
33) Benzene	8.323	78	1611310	40.99	ug/L	100
34) Trichloroethene	9.091	95	533858	52.09	ug/L	91
42) Toluene	10.390	91	2136965	50.53	ug/L	99
45) 1,1,2-Trichloroethane	10.786	97	147078	20.23	ug/L	96
46) Tetrachloroethene	10.859	164	79575	10.16	ug/L	96

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060221\
 Data File : VW019101.D
 Acq On : 02 Jun 2021 15:12
 Operator : SY/VA
 Sample : M2558-06
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 X3552

Manual Integrations
 APPROVED

MMDadoda
 6/4/2021 1:14:14 PM

Quant Time: Jun 03 01:24:23 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 02 12:40:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

51) Chlorobenzene	11.658	112	326310	12.50	ug/L	99
52) Ethylbenzene	11.731	91	1153194	24.79	ug/L	100
53) m,p-Xylene	11.847	106	530802	30.94	ug/L	97
54) o-Xylene	12.164	106	409183	25.04	ug/L	93
55) Styrene	12.182	104	281320	10.01	ug/L	96
57) 1,1,2,2-Tetrachloroethane	12.713	83	108793	12.14	ug/L	99
59) Bromoform	12.353	173	50508	10.58	ug/L	96
60) Isopropylbenzene	12.463	105	908574	19.58	ug/L	99
63) 1,2,4-Trimethylbenzene	13.249	105	920864	24.21	ug/L	99
64) 1,3-Dichlorobenzene	13.499	146	389453	19.24	ug/L	92
65) 1,4-Dichlorobenzene	13.578	146	199186	9.62	ug/L	97
70) 1,2,4-trichlorobenzene	15.133	180	231250	19.26	ug/L	100
72) 1,2,3-Trichlorobenzene	15.554	180	316714	29.77	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060221\
Data File : VW019101.D
Acq On : 02 Jun 2021 15:12
Operator : SY/VA
Sample : M2558-06
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 13 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampled :
X3552

Quant Time: Jun 03 01:24:23 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 02 12:40:32 2021
Response via : Initial Calibration

Manual Integrations
APPROVED

MMDadoda
6/4/2021 1:14:14 PM

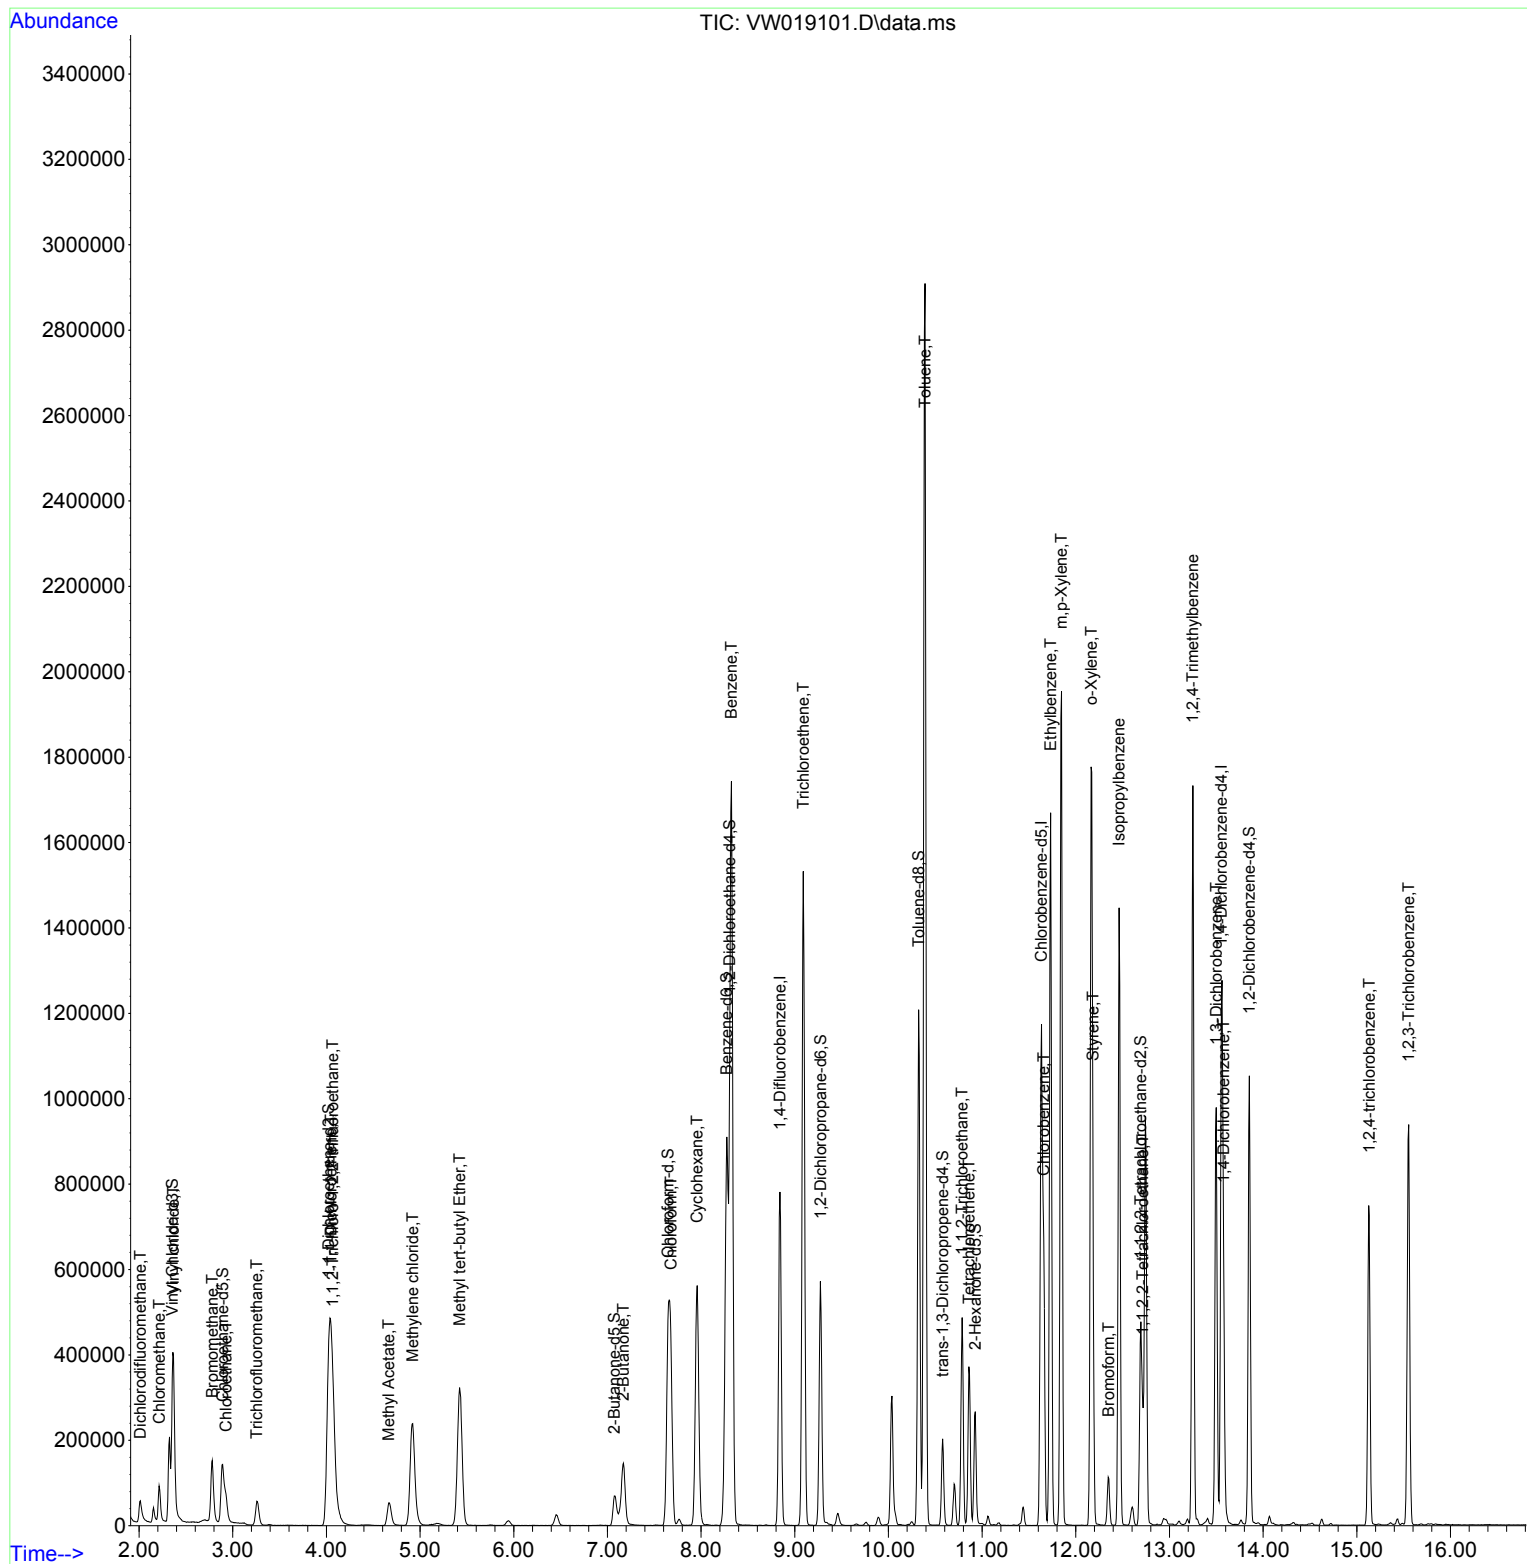







#2
Dichlorodifluoromethane
Concen: 9.32 ug/L
RT: 2.013 min Scan# 18
Delta R.T. 0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12

Tgt Ion: 85 Resp: 79677
Ion Ratio Lower Upper
85 100
87 28.1 23.3 34.9

Instrument :
MSVOA_W
ClientSampleId :
X3552




Manual Integrations
APPROVED


MMDadoda
6/4/2021 1:14:14 PM



#3
Chloromethane
Concen: 11.00 ug/L
RT: 2.214 min Scan# 51
Delta R.T. 0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12

Tgt Ion: 50 Resp: 86931
Ion Ratio Lower Upper
50 100
52 32.6 22.5 41.9

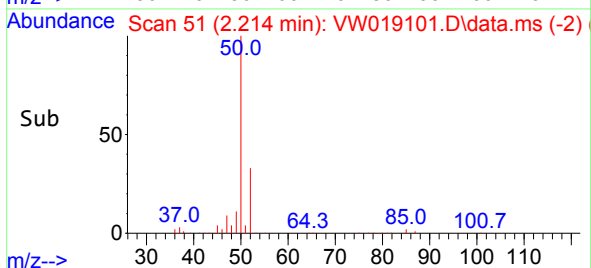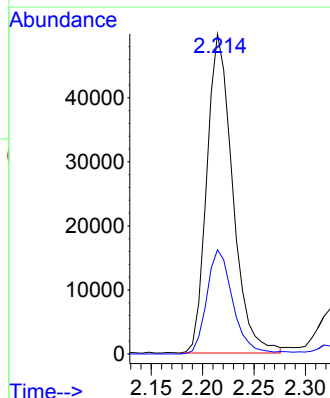

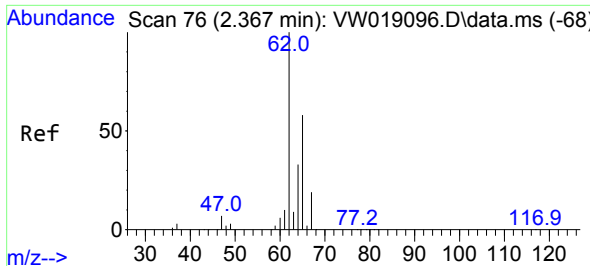





#5
 Vinyl chloride
 Concen: 22.63 ug/L
 RT: 2.367 min Scan# 76
 Delta R.T. 0.000 min
 Lab File: VW019101.D
 Acq: 02 Jun 2021 15:12

Tgt Ion: 62 Resp: 272955
 Ion Ratio Lower Upper
 62 100
 64 34.0 24.2 45.0

Instrument :
 MSVOA_W
 ClientSampleId :
 X3552




Manual Integrations
 APPROVED


MMDadoda
 6/4/2021 1:14:14 PM

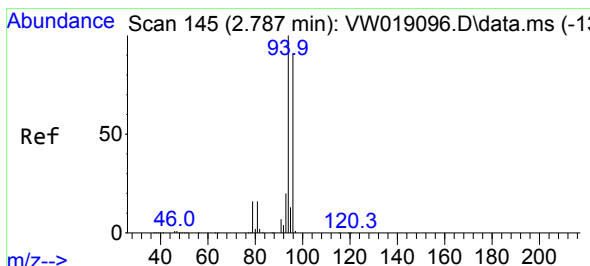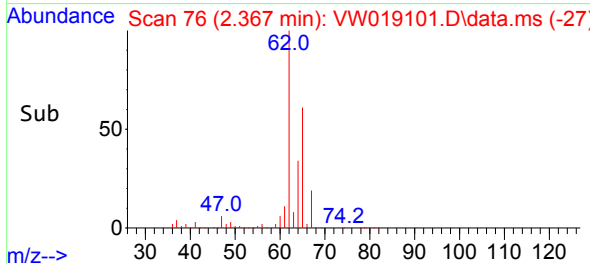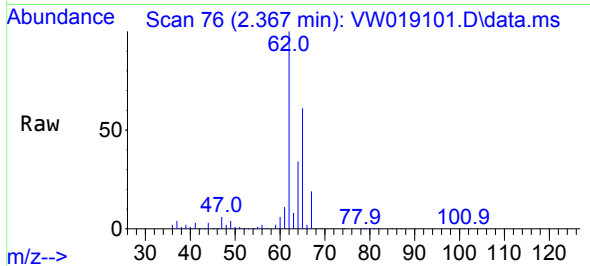

#6
 Bromomethane
 Concen: 11.94 ug/L
 RT: 2.781 min Scan# 144
 Delta R.T. -0.006 min
 Lab File: VW019101.D
 Acq: 02 Jun 2021 15:12


Tgt Ion: 94 Resp: 107131
 Ion Ratio Lower Upper
 94 100
 96 93.2 65.3 121.3

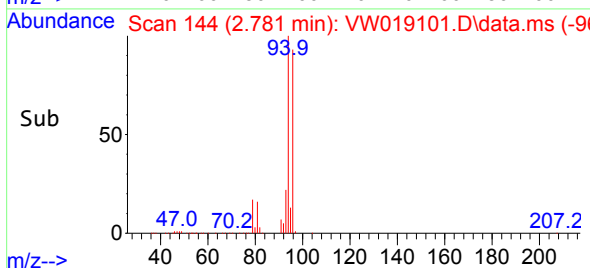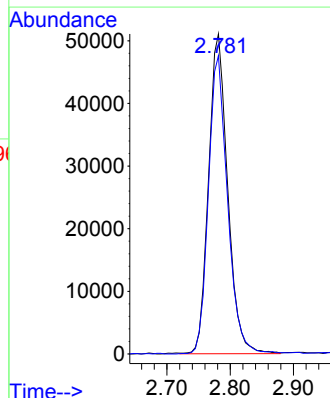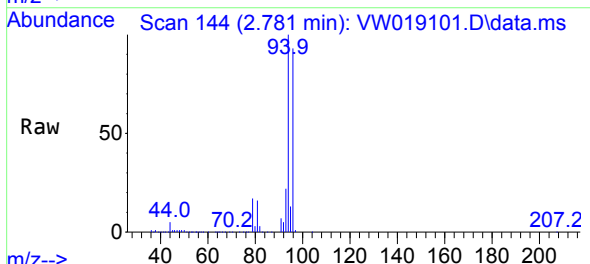



#8
Chloroethane
Concen: 8.49 ug/L
RT: 2.928 min Scan# 168
Delta R.T. 0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12



Instrument :
MSVOA_W
ClientSampleId :
X3552




Tgt Ion: 64 Resp: 60872
Ion Ratio Lower Upper
64 100
66 32.7 23.4 43.6

Manual Integrations
APPROVED



MMDadoda
6/4/2021 1:14:14 PM

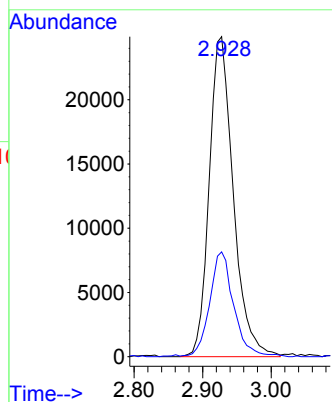


#9
Trichlorofluoromethane
Concen: 9.57 ug/L
RT: 3.257 min Scan# 222
Delta R.T. -0.006 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12




Tgt Ion: 101 Resp: 63363
Ion Ratio Lower Upper
101 100
103 63.3 51.0 76.4

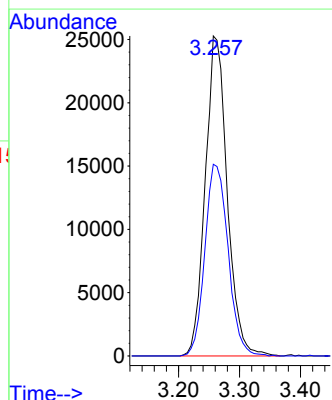

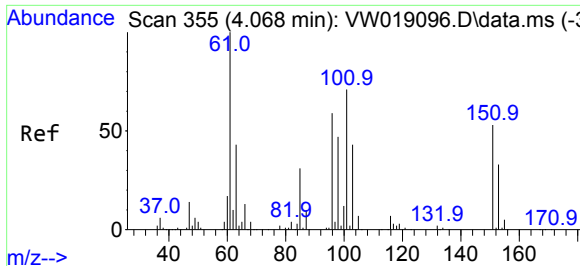

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 20.09 ug/L
 RT: 4.068 min Scan# 355
 Delta R.T. 0.000 min
 Lab File: VW019101.D
 Acq: 02 Jun 2021 15:12




Instrument :
 MSVOA_W
 ClientSampleId :
 X3552

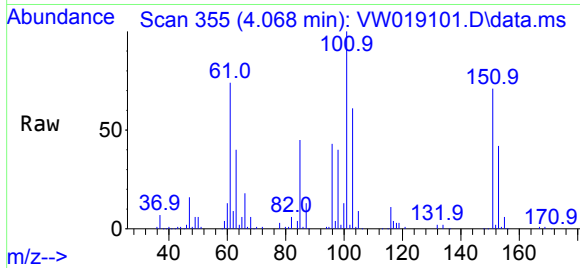


Tgt Ion:101 Resp: 190243
 Ion Ratio Lower Upper
 101 100
 85 44.2 38.2 57.2
 151 71.7 56.6 85.0

Manual Integrations
 APPROVED



MMDadoda
 6/4/2021 1:14:14 PM

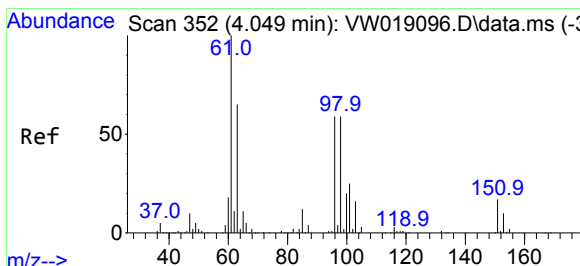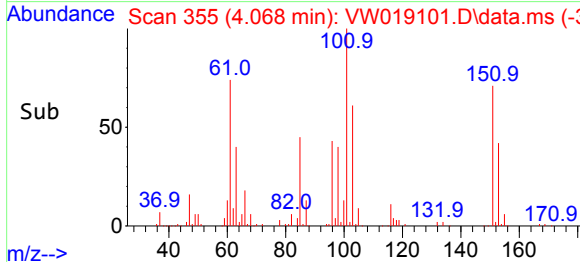


#12
 1,1-Dichloroethene
 Concen: 14.60 ug/L
 RT: 4.049 min Scan# 352
 Delta R.T. 0.000 min
 Lab File: VW019101.D
 Acq: 02 Jun 2021 15:12

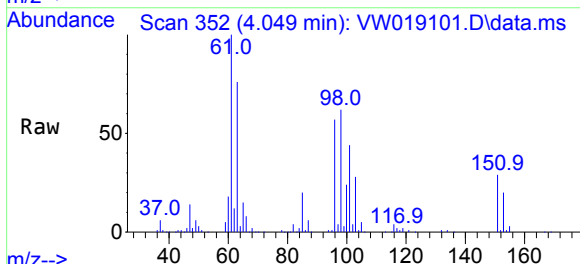

Tgt Ion: 96 Resp: 136551
 Ion Ratio Lower Upper
 96 100
 61 175.4 118.1 219.3
 63 134.1 83.7 155.5

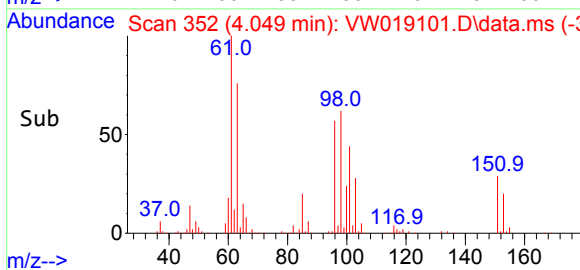







#15
Methyl Acetate
Concen: 25.63 ug/L
RT: 4.665 min Scan# 453
Delta R.T. -0.012 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12

Tgt Ion: 43 Resp: 104372
Ion Ratio Lower Upper
43 100
74 26.7 20.0 30.0

Instrument :
MSVOA_W
ClientSampleId :
X3552




Manual Integrations
APPROVED


MMDadoda
6/4/2021 1:14:14 PM

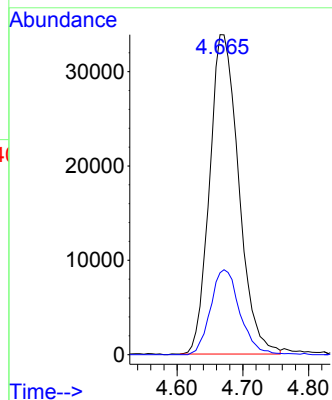


#16
Methylene chloride
Concen: 17.59 ug/L
RT: 4.921 min Scan# 495
Delta R.T. 0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12

Tgt Ion: 84 Resp: 215353
Ion Ratio Lower Upper
84 100
86 62.4 45.3 84.1
49 117.3 86.6 160.8

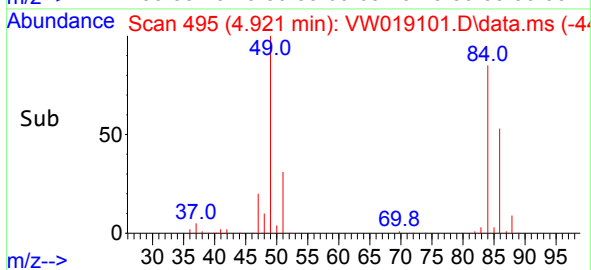
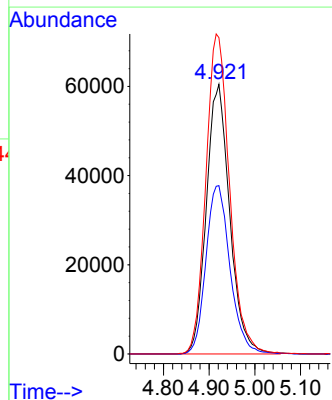






#18
Methyl tert-butyl Ether
Concen: 41.20 ug/L
RT: 5.421 min Scan# 577
Delta R.T. -0.006 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12

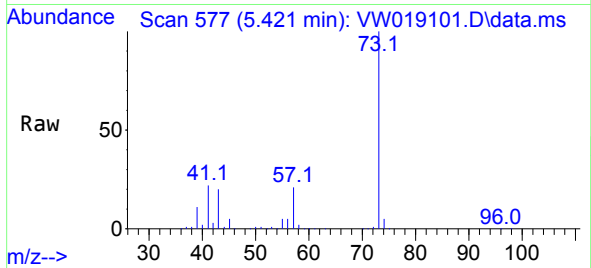



Tgt Ion: 73 Resp: 536730
Ion Ratio Lower Upper
73 100
43 20.5 17.7 26.5
57 21.5 17.0 25.4



#22
2-Butanone
Concen: 81.98 ug/L
RT: 7.171 min Scan# 864
Delta R.T. -0.006 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12




Tgt Ion: 43 Resp: 221928
Ion Ratio Lower Upper
43 100
72 28.9 14.9 44.7

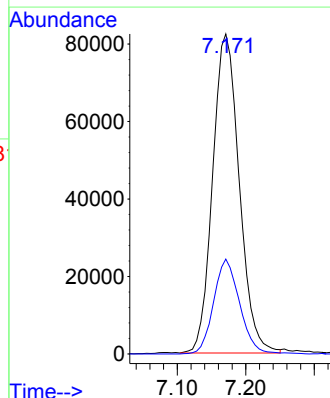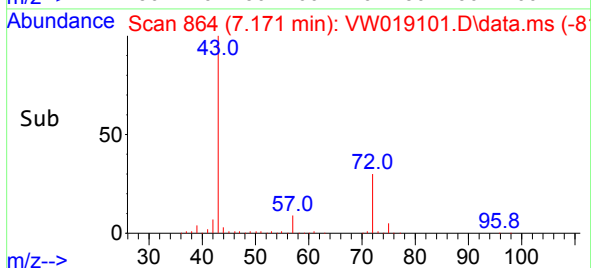

Instrument :
MSVOA_W
ClientSampleId :
X3552

Manual Integrations
APPROVED

MMDadoda
6/4/2021 1:14:14 PM







#25
Chloroform
Concen: 19.27 ug/L
RT: 7.677 min Scan# 947
Delta R.T. -0.006 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12

Tgt Ion: 83 Resp: 351530
Ion Ratio Lower Upper
83 100
85 63.5 44.6 82.8

Instrument :
MSVOA_W
ClientSampleId :
X3552




Manual Integrations
APPROVED


MMDadoda
6/4/2021 1:14:14 PM



#29
Cyclohexane
Concen: 20.59 ug/L
RT: 7.957 min Scan# 993
Delta R.T. -0.006 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12

Tgt Ion: 56 Resp: 320300
Ion Ratio Lower Upper
56 100
69 31.8 24.5 36.7
84 91.4 75.0 112.4

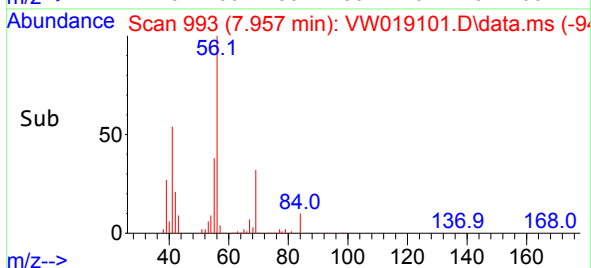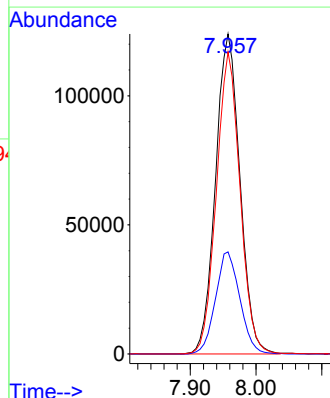

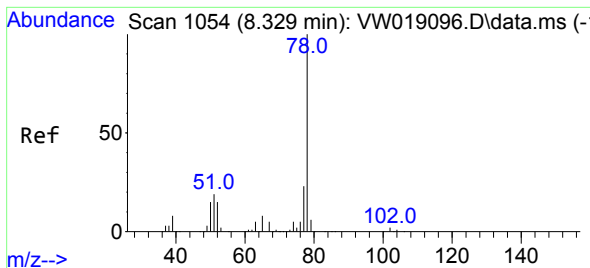





#33
Benzene
Concen: 40.99 ug/L
RT: 8.323 min Scan# 1053
Delta R.T. -0.006 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12

Tgt Ion: 78 Resp: 1611310

Instrument :
MSVOA_W
ClientSampled :
X3552

Manual Integrations
APPROVED




MMDadoda
6/4/2021 1:14:14 PM

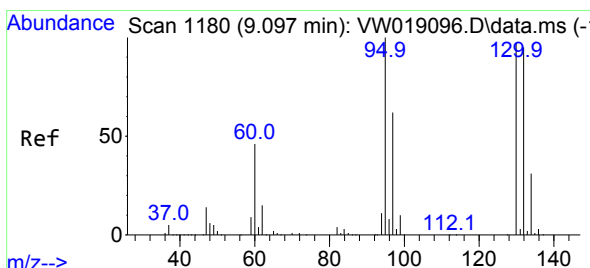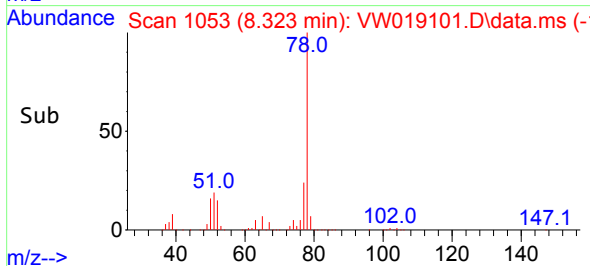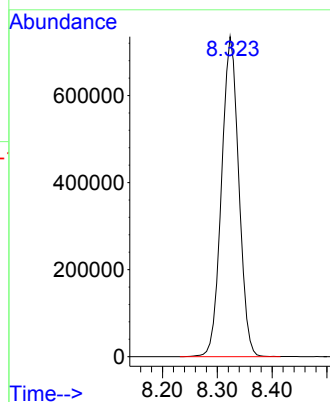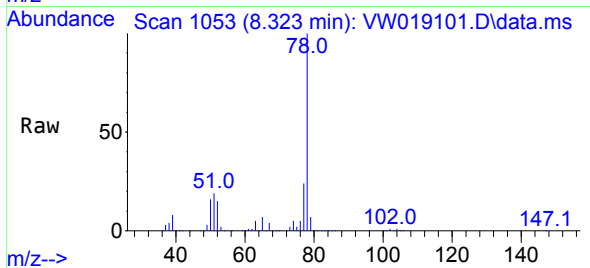


#34
Trichloroethene
Concen: 52.09 ug/L
RT: 9.091 min Scan# 1179
Delta R.T. -0.006 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12

Tgt Ion: 95 Resp: 533858

Ion	Ratio	Lower	Upper
95	100		
97	61.8	47.3	87.8
132	85.2	71.0	131.8
130	94.6	65.1	120.9

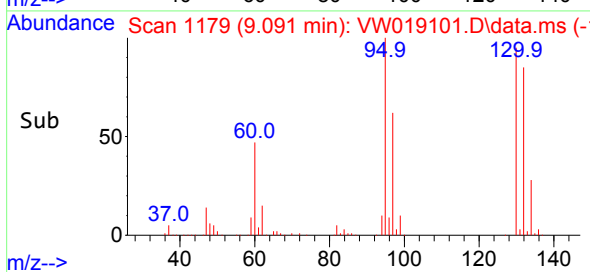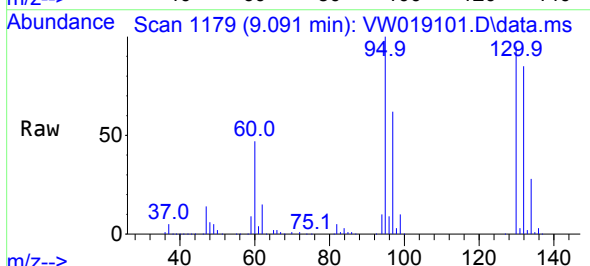

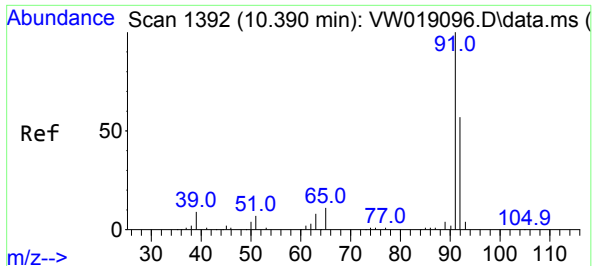


#42
Toluene
Concen: 50.53 ug/L
RT: 10.390 min Scan# 1392
Delta R.T. -0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12




Instrument :
MSVOA_W
ClientSampleId :
X3552

Manual Integrations
APPROVED

MMDadoda
6/4/2021 1:14:14 PM



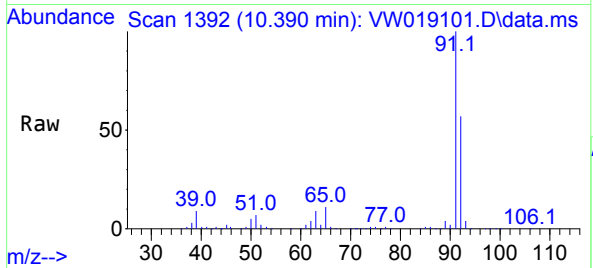



Tgt Ion: 91 Resp: 2136965
Ion Ratio Lower Upper
91 100
92 56.9 39.5 73.3

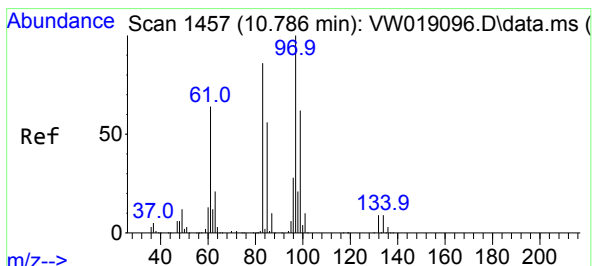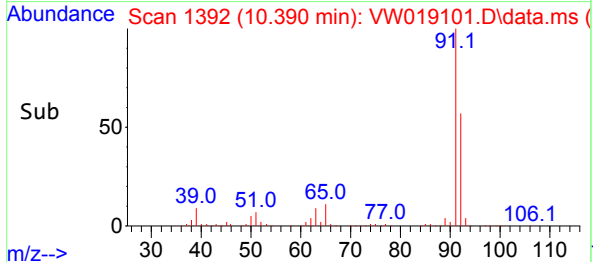

#45
1,1,2-Trichloroethane
Concen: 20.23 ug/L
RT: 10.786 min Scan# 1457
Delta R.T. 0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12


Tgt Ion: 97 Resp: 147078
Ion Ratio Lower Upper
97 100
99 60.2 45.1 83.7
83 84.8 58.1 107.9
85 56.2 37.3 69.3

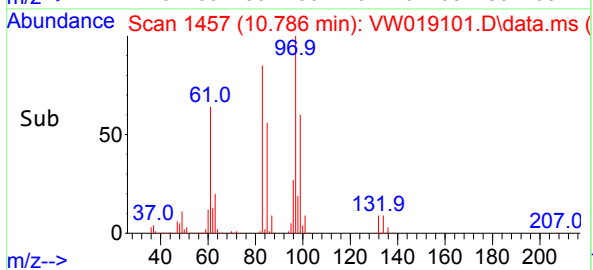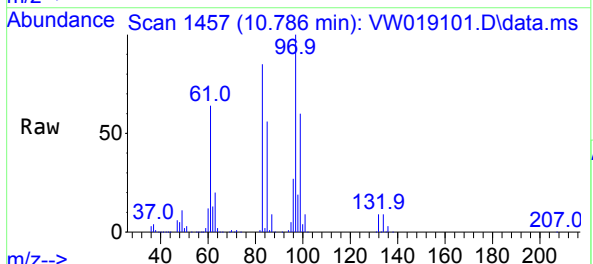



#46
Tetrachloroethene
Concen: 10.16 ug/L
RT: 10.859 min Scan# 1469
Delta R.T. -0.006 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12




Instrument :
MSVOA_W
ClientSampled :
X3552

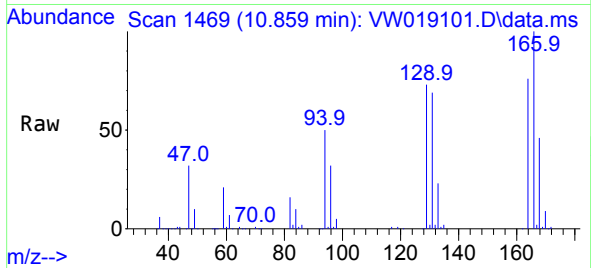


Tgt Ion:164 Resp: 79575
Ion Ratio Lower Upper
164 100
129 96.1 66.7 123.9
131 91.1 61.1 113.5
166 131.2 87.0 161.6

Manual Integrations
APPROVED



MMDadoda
6/4/2021 1:14:14 PM

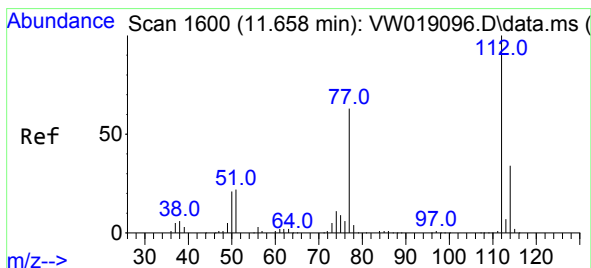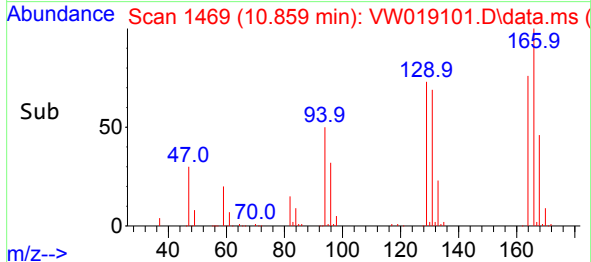


#51
Chlorobenzene
Concen: 12.50 ug/L
RT: 11.658 min Scan# 1600
Delta R.T. 0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12

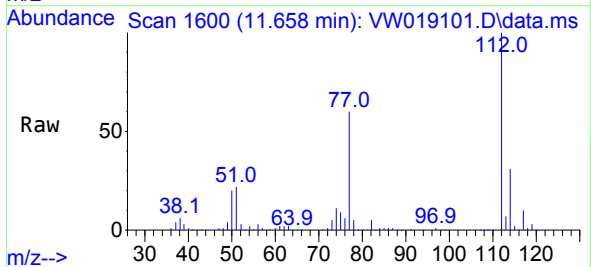


Tgt Ion:112 Resp: 326310
Ion Ratio Lower Upper
112 100
114 31.5 23.4 43.6
77 59.6 47.6 71.4

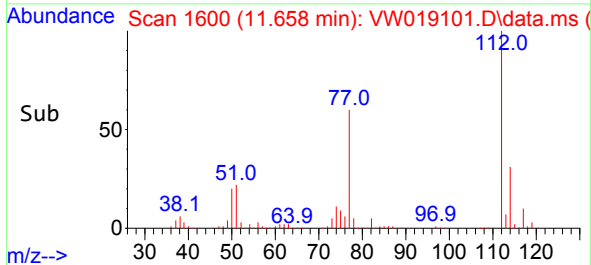



#52
Ethylbenzene
Concen: 24.79 ug/L
RT: 11.731 min Scan# 1612
Delta R.T. 0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12




Instrument :
MSVOA_W
ClientSampleId :
X3552



Tgt Ion: 91 Resp: 1153194
Ion Ratio Lower Upper
91 100
106 32.0 22.5 41.7




Manual Integrations
APPROVED


MMDadoda
6/4/2021 1:14:14 PM

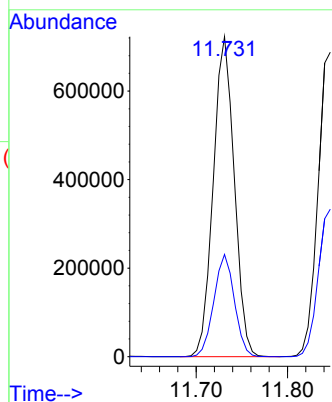

#53
m,p-Xylene
Concen: 30.94 ug/L
RT: 11.847 min Scan# 1631
Delta R.T. 0.006 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12


Tgt Ion: 106 Resp: 530802
Ion Ratio Lower Upper
106 100
91 206.4 141.3 262.3

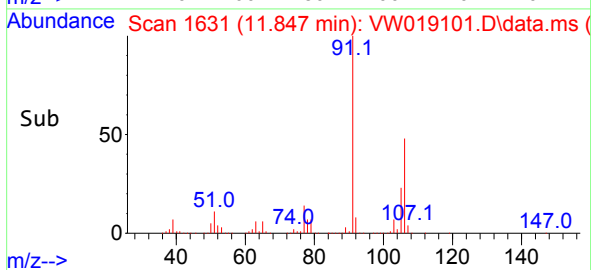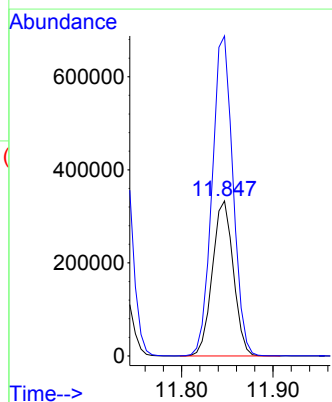



#54
o-Xylene
Concen: 25.04 ug/L
RT: 12.164 min Scan# 1683
Delta R.T. 0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12



Instrument :
MSVOA_W
ClientSampleId :
X3552




Tgt Ion:106 Resp: 409183
Ion Ratio Lower Upper
106 100
91 224.9 150.0 278.6

Manual Integrations
APPROVED



MMDadoda
6/4/2021 1:14:14 PM

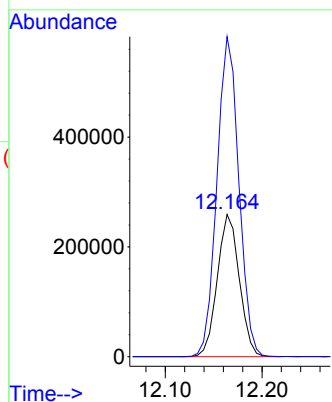


#55
Styrene
Concen: 10.01 ug/L
RT: 12.182 min Scan# 1686
Delta R.T. 0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12




Tgt Ion:104 Resp: 281320
Ion Ratio Lower Upper
104 100
78 48.8 32.5 60.3


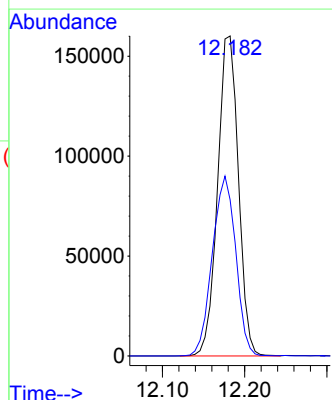
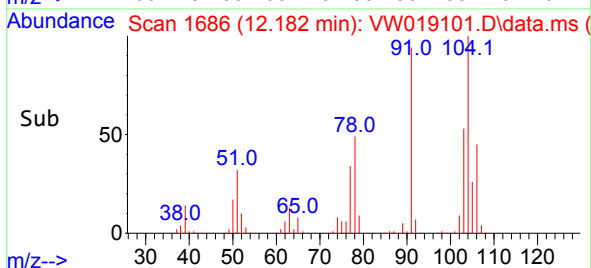





#57
1,1,2,2-Tetrachloroethane
Concen: 12.14 ug/L
RT: 12.713 min Scan# 1773
Delta R.T. 0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12

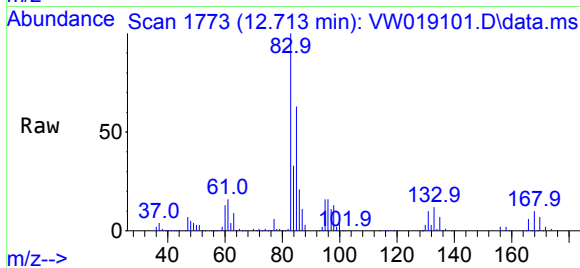



Tgt Ion: 83 Resp: 108793
Ion Ratio Lower Upper
83 100
85 62.7 44.4 82.4
131 9.5 8.2 12.4

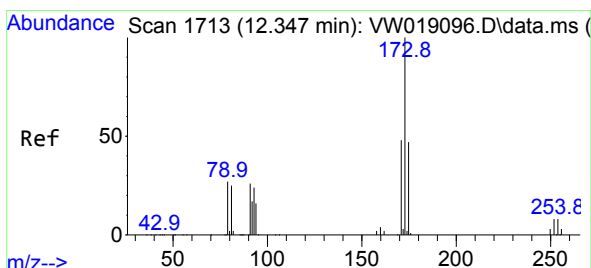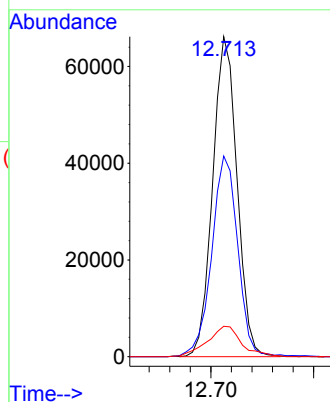

#59
Bromoform
Concen: 10.58 ug/L
RT: 12.353 min Scan# 1714
Delta R.T. 0.006 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12

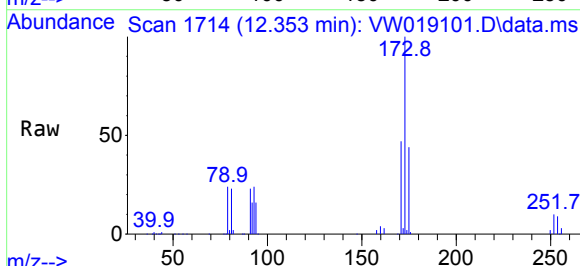


Tgt Ion: 173 Resp: 50508
Ion Ratio Lower Upper
173 100
175 49.6 37.5 56.3
254 9.3 7.0 10.4

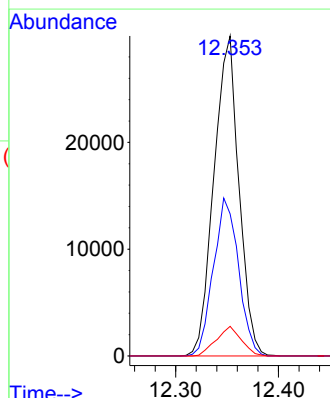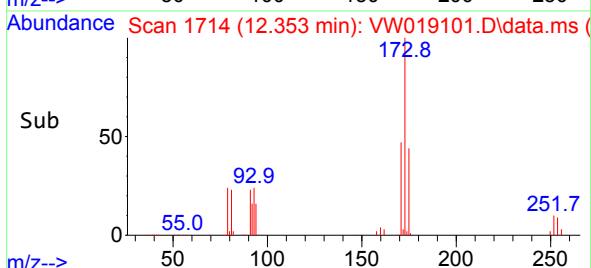

Instrument :
MSVOA_W
ClientSampleId :
X3552


Manual Integrations
APPROVED

MMDadoda
6/4/2021 1:14:14 PM

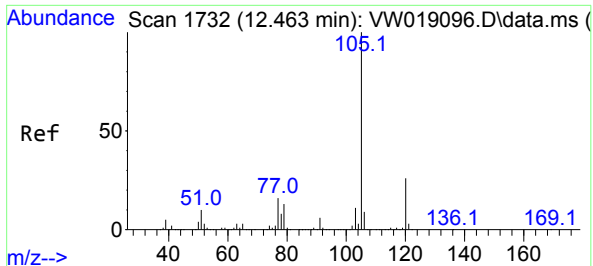

#60
Isopropylbenzene
Concen: 19.58 ug/L
RT: 12.463 min Scan# 1732
Delta R.T. 0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12




Instrument :
MSVOA_W
ClientSampleId :
X3552

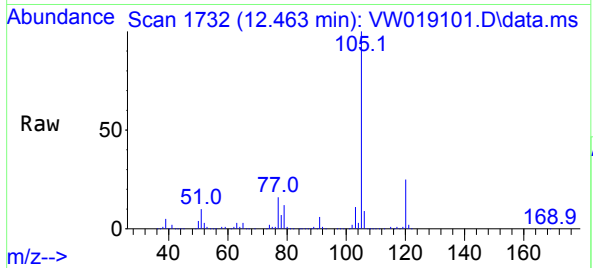

Tgt Ion:105 Resp: 908574
Ion Ratio Lower Upper
105 100
120 25.9 21.1 31.7
77 16.4 13.2 19.8




Manual Integrations
APPROVED


MMDadoda
6/4/2021 1:14:14 PM

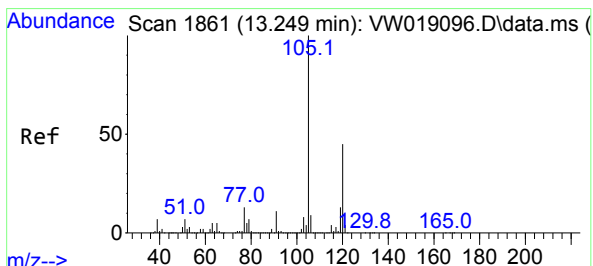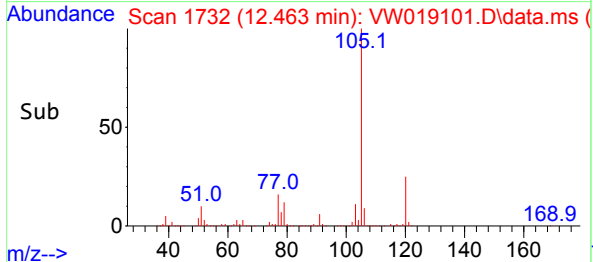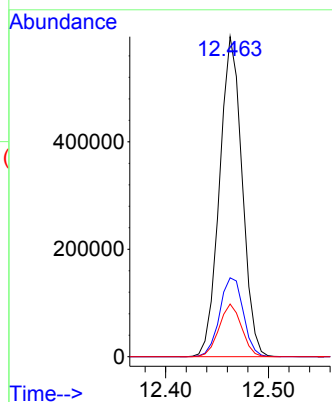

#63
1,2,4-Trimethylbenzene
Concen: 24.21 ug/L
RT: 13.249 min Scan# 1861
Delta R.T. 0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12


Tgt Ion:105 Resp: 920864
Ion Ratio Lower Upper
105 100
120 43.7 35.6 53.4

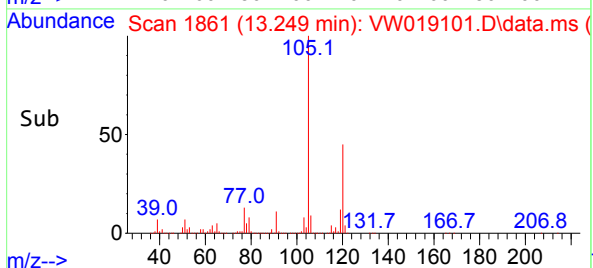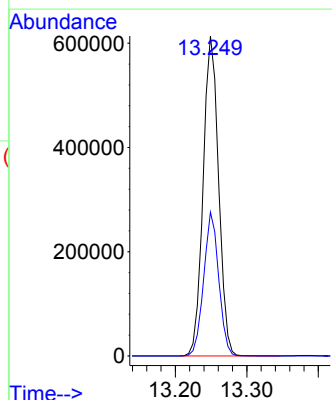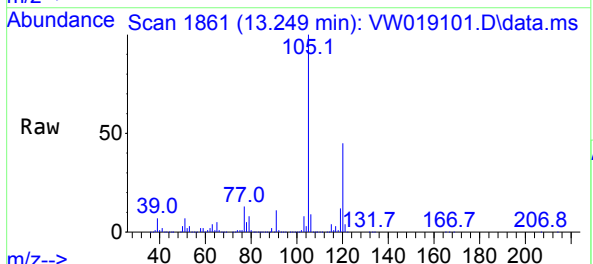



#64
1,3-Dichlorobenzene
Concen: 19.24 ug/L
RT: 13.499 min Scan# 1902
Delta R.T. 0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12




Instrument :
MSVOA_W
ClientSampled :
X3552




Tgt Ion:146 Resp: 389453
Ion Ratio Lower Upper
146 100
111 42.9 26.7 49.7
148 64.3 41.1 76.3

Manual Integrations
APPROVED



MMDadoda
6/4/2021 1:14:14 PM

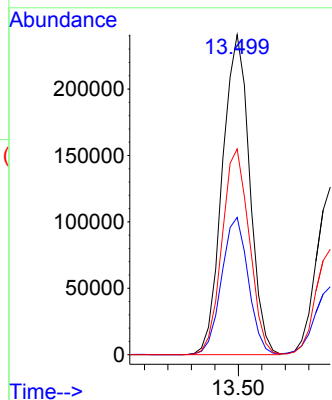


#65
1,4-Dichlorobenzene
Concen: 9.62 ug/L
RT: 13.578 min Scan# 1915
Delta R.T. 0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12




Tgt Ion:146 Resp: 199186
Ion Ratio Lower Upper
146 100
111 40.6 28.8 53.4
148 62.9 46.8 87.0

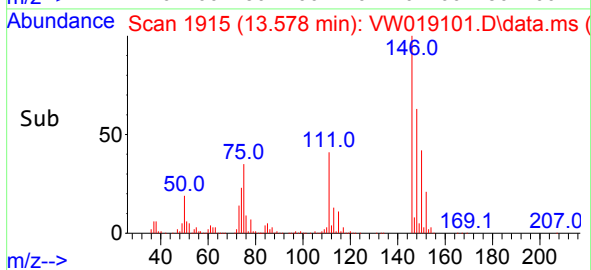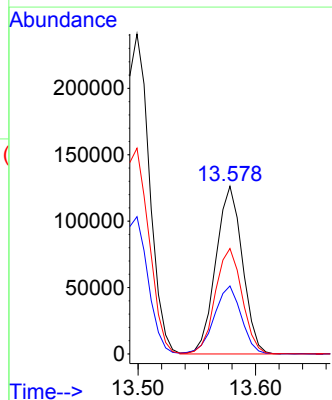



#70
1,2,4-trichlorobenzene
Concen: 19.26 ug/L
RT: 15.133 min Scan# 2170
Delta R.T. 0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12




Instrument :
MSVOA_W
ClientSampled :
X3552




Tgt Ion:180 Resp: 231250
Ion Ratio Lower Upper
180 100
182 92.8 74.7 112.1
145 31.2 25.0 37.4

Manual Integrations
APPROVED

MMDadoda
6/4/2021 1:14:14 PM

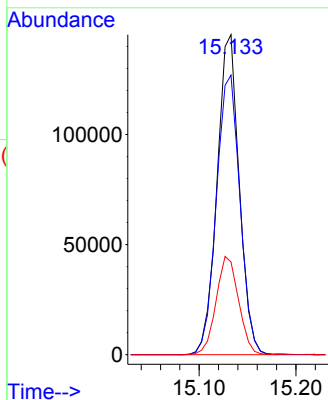

#72
1,2,3-Trichlorobenzene
Concen: 29.77 ug/L
RT: 15.554 min Scan# 2239
Delta R.T. 0.000 min
Lab File: VW019101.D
Acq: 02 Jun 2021 15:12



Tgt Ion:180 Resp: 316714
Ion Ratio Lower Upper
180 100
182 93.6 76.7 115.1
145 32.7 28.9 43.3

