
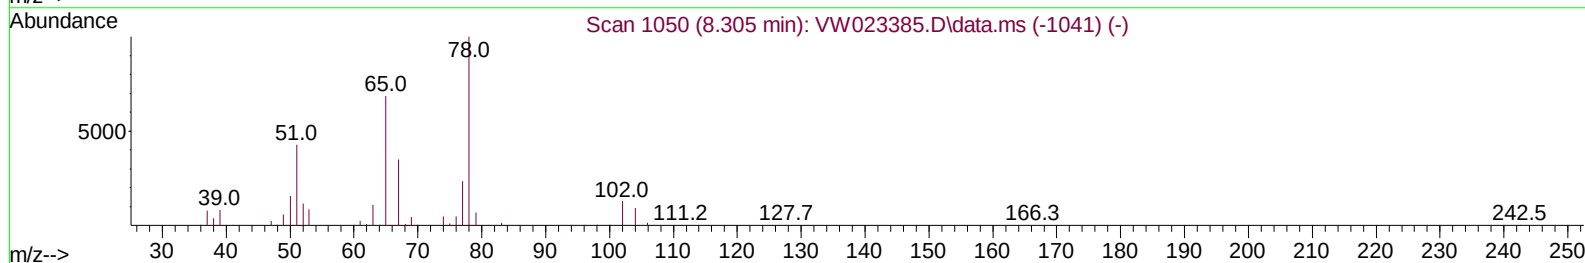
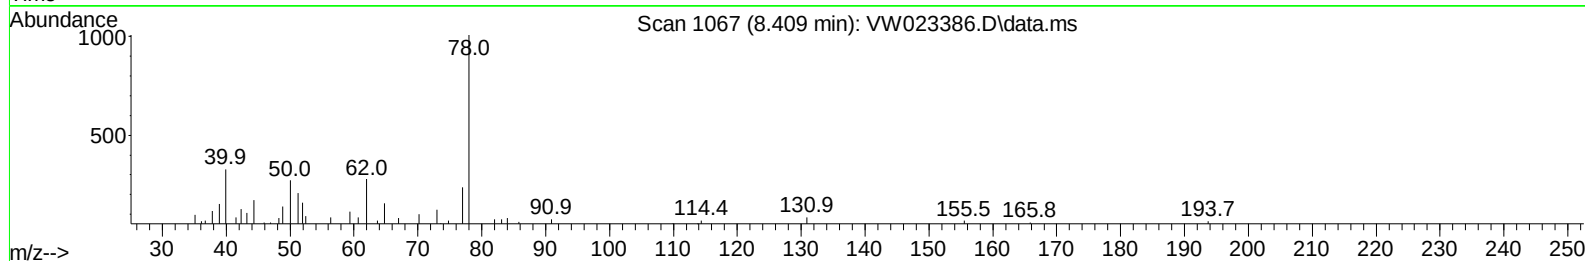


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060322\
 Data File : VW023386.D
 Acq On : 03 Jun 2022 09:31
 Operator : SY/VA
 Sample : VW0603SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 23:33:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 03 23:33:12 2022
 Response via : Initial Calibration

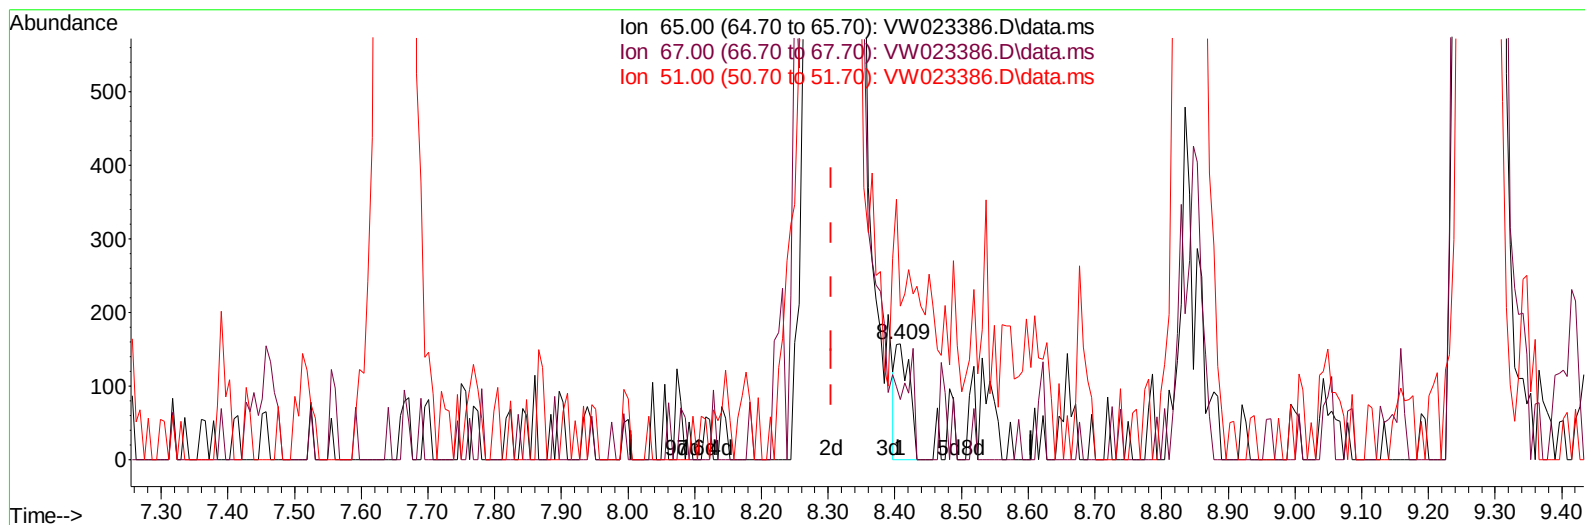

TIC: VW023386.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)




8.409min (+ 0.104) 0.04 ug/L

response 227

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	47.58
51.00	92.30	101.32
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060322\
 Data File : VW023386.D
 Acq On : 03 Jun 2022 09:31
 Operator : SY/VA
 Sample : VW0603SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 23:33:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 03 23:33:12 2022
 Response via : Initial Calibration

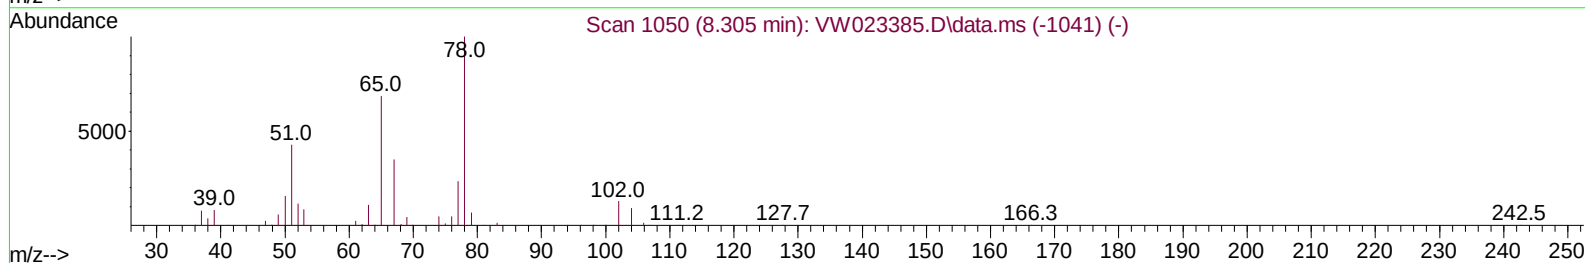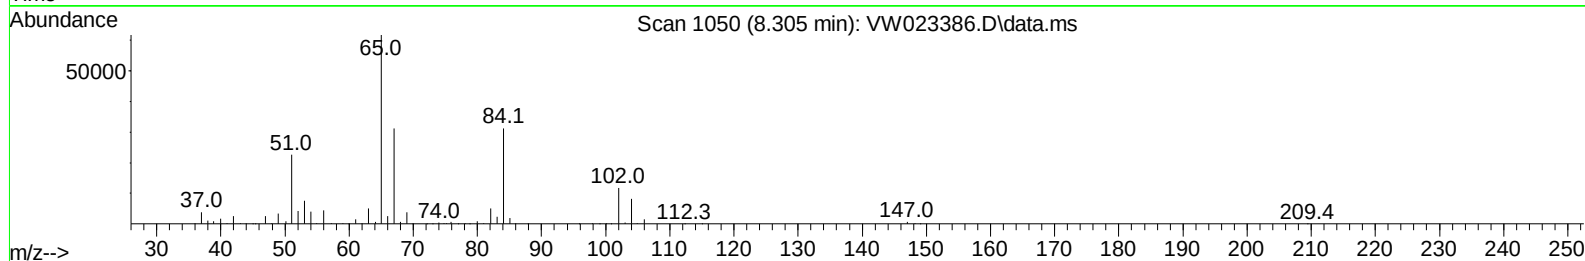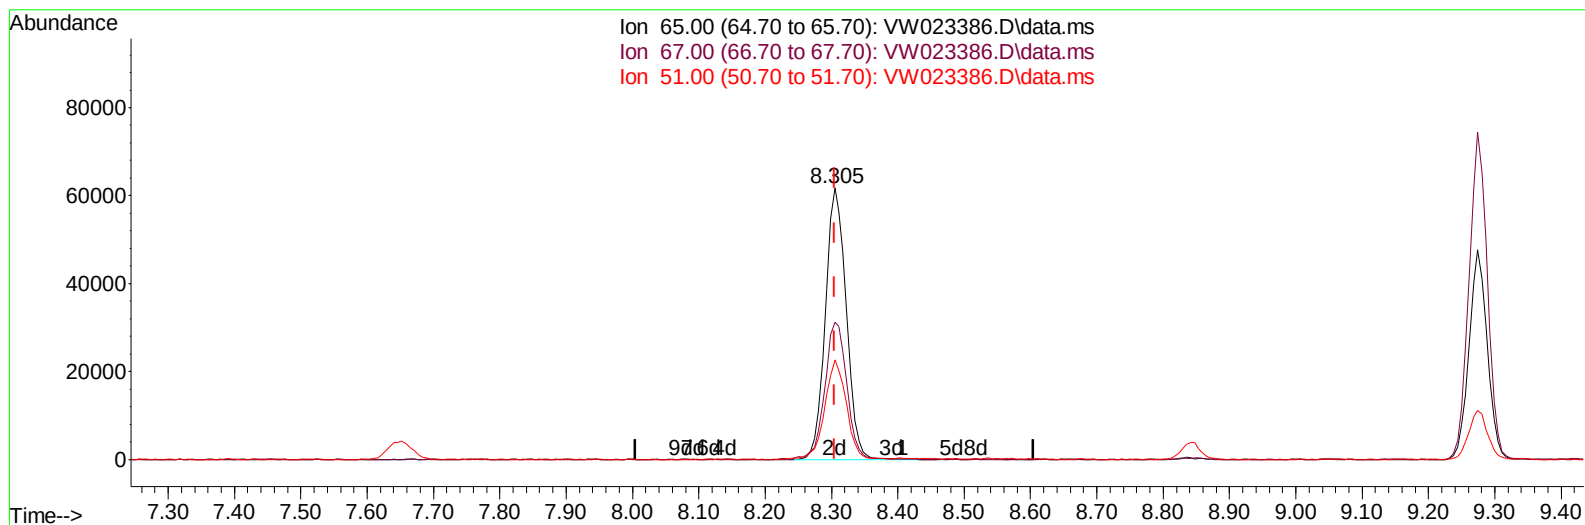

TIC: VW023386.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)**8.305min (+ 0.000) 24.81 ug/L m****response 134447**

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.10	0.08#
51.00	92.30	0.17#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060322\
 Data File : VW023386.D
 Acq On : 03 Jun 2022 09:31
 Operator : SY/VA
 Sample : VW0603SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 23:33:44 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060222SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 03 23:33:12 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	392862	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.628	117	361605	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	162834	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	143116	24.634	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	98.520%		
7) Chloroethane-d5	2.885	69	101986	25.321	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	101.280%		
11) 1,1-Dichloroethene-d2	4.019	63	159969	17.914	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	71.640%		
21) 2-Butanone-d5	7.080	46	56996	47.804	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	95.600%		
24) Chloroform-d	7.653	84	249625	24.130	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	96.520%		
26) 1,2-Dichloroethane-d4	8.305	65	134447m	24.813	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	99.240%		
32) Benzene-d6	8.281	84	483931	24.907	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	99.640%		
36) 1,2-Dichloropropane-d6	9.274	67	142970	25.721	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	102.880%		
41) Toluene-d8	10.323	98	464468	25.072	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	100.280%		
43) trans-1,3-Dichloroprop...	10.579	79	56570	22.797	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	91.200%		
47) 2-Hexanone-d5	10.926	63	41789	46.797	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	93.600%		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	114042	23.261	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	93.040%		
66) 1,2-Dichlorobenzene-d4	13.853	152	151553	26.330	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	105.320%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060322\
Data File : VW023386.D
Acq On : 03 Jun 2022 09:31
Operator : SY/VA
Sample : VW0603SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 03 23:33:44 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060222SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 03 23:33:12 2022
Response via : Initial Calibration

