


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060322\
Data File : VW023384.D
Acq On : 03 Jun 2022 07:46
Operator : SY/VA
Sample : BFB566
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB566

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060222SMA.M
Title : SFAM01.0
Last Update : Fri Jun 03 23:33:12 2022

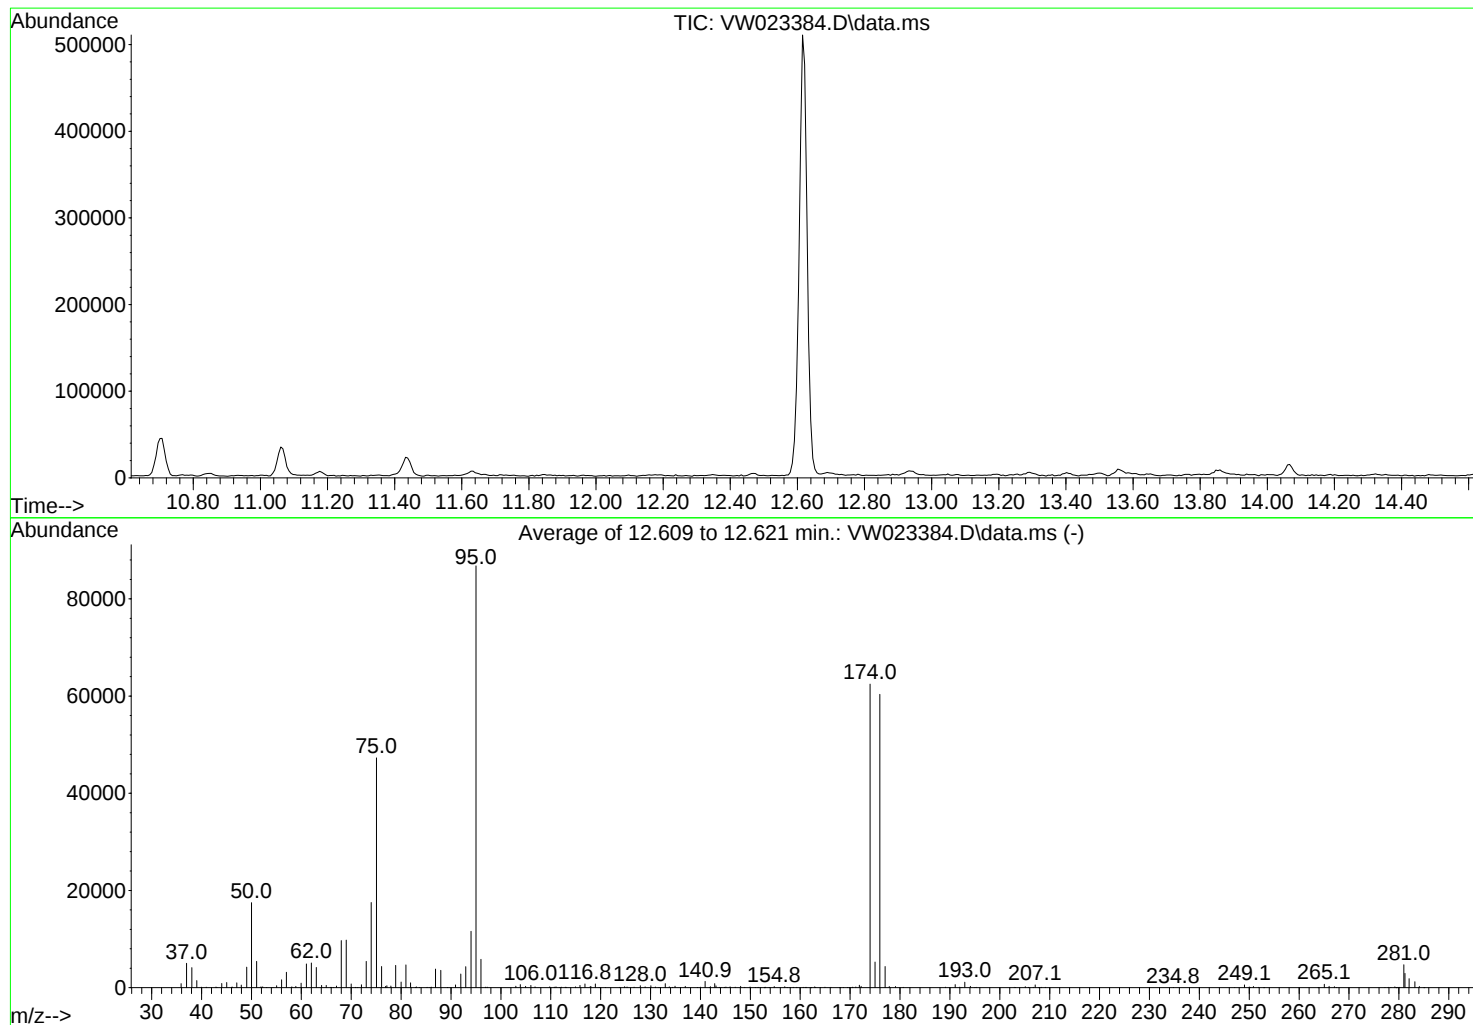

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	17502	PASS
75	95	30	80	54.5	47299	PASS
95	95	100	100	100.0	86797	PASS
96	95	5	9	6.7	5839	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.0	62461	PASS
175	174	5	9	8.5	5280	PASS
176	174	95	105	96.6	60336	PASS
177	176	5	10	7.2	4351	PASS

m/z	Abundance
35.10	92.0
35.80	171.0
36.70	78.0
37.10	70.0
38.20	86.0
39.10	156.0
39.90	443.0
41.20	94.0
42.00	85.0
42.40	73.0
43.50	138.0
44.10	190.0
46.80	100.0
47.80	107.0
48.80	55.0
53.20	51.0
53.80	64.0
56.20	72.0
61.00	57.0
63.80	72.0
72.70	60.0
78.50	77.0
88.60	79.0
221.00	115.0
261.10	72.0

Instrument :
MSVOA_W
ClientSampleId :
BFB566

m/z	Abundance
35.10	120.0
36.00	1061.0
37.00	4576.0
38.10	3781.0
39.00	1535.0
40.00	660.0
40.90	112.0
43.00	214.0
44.00	1022.0
45.10	925.0
46.00	232.0
47.10	942.0
48.10	530.0
49.00	3788.0
50.00	15089.0
51.00	4818.0
51.90	212.0
53.10	54.0
54.00	53.0
55.10	337.0
56.10	1549.0
57.00	2853.0
58.20	179.0
59.00	364.0
59.90	1037.0
61.00	4581.0
62.00	4118.0
63.00	3220.0
64.00	544.0
65.10	343.0
65.90	206.0
66.40	104.0
67.00	220.0
68.00	8496.0
69.00	8252.0
69.90	600.0
71.30	120.0
72.10	368.0
73.00	4676.0
74.00	15729.0
75.00	40712.0
76.10	3648.0
77.20	585.0
78.00	307.0
78.90	3881.0
80.00	942.0
80.90	4079.0
81.90	687.0
82.90	126.0
85.20	79.0
85.80	244.0
86.90	2782.0
88.00	3122.0
89.30	108.0
90.90	442.0
92.00	2279.0
93.00	3873.0
94.00	10327.0
95.00	70728.0
96.00	4990.0
97.00	137.0
97.30	145.0
103.00	400.0
103.90	555.0
105.00	271.0
106.00	383.0
106.90	92.0
109.80	250.0
110.70	149.0
111.20	129.0
111.80	123.0
112.90	78.0
115.00	223.0
115.80	358.0
116.80	703.0
117.90	605.0
119.00	715.0
120.90	76.0
124.80	293.0
125.30	217.0
126.70	151.0
128.00	273.0
128.90	110.0
130.10	327.0
130.90	113.0
131.70	76.0
133.00	1112.0
133.80	348.0
134.40	162.0
134.90	336.0
137.00	307.0
139.40	90.0

Instrument :
MSVOA_W
ClientSampleId :
BFB566

140.00	65.0
140.90	1116.0
141.80	99.0
142.90	1092.0
144.80	205.0
146.00	146.0
146.90	160.0
148.10	167.0
148.90	123.0
150.00	96.0
151.60	86.0
152.10	78.0
152.80	57.0
154.80	205.0
156.90	118.0
159.40	107.0
160.60	178.0
162.90	477.0
164.10	63.0
165.00	191.0
166.20	106.0
169.80	51.0
170.40	108.0
171.10	221.0
172.20	766.0
174.00	48256.0
175.10	3993.0
176.00	44080.0
177.00	3460.0
177.90	340.0
179.20	381.0
180.60	117.0
189.10	158.0
191.00	882.0
192.00	352.0
193.00	1649.0
194.20	380.0
195.00	142.0
202.90	164.0
205.10	382.0
205.80	93.0
207.00	727.0
208.30	165.0
209.10	83.0
221.00	71.0
234.80	88.0
247.10	61.0
249.10	745.0
250.00	349.0
250.80	340.0
251.90	121.0
252.90	53.0
263.80	57.0
265.10	832.0
265.90	279.0
267.00	199.0
267.50	87.0
277.20	97.0
278.40	83.0
279.30	260.0
281.00	9730.0
282.00	2835.0
283.30	1318.0
284.10	281.0

Instrument :
MSVOA_W
ClientSampleId :
BFB566

m/z	Abundance
36.00	1004.0
37.00	5743.0
38.00	4926.0
39.00	1814.0
40.00	447.0
40.90	71.0
42.80	157.0
44.10	1082.0
45.00	1399.0
46.20	210.0
47.00	1090.0
47.90	829.0
49.10	4295.0
50.00	19656.0
51.10	6042.0
51.90	249.0
52.30	317.0
53.10	91.0
54.30	73.0
55.00	404.0
56.00	1791.0
57.00	3632.0
58.00	183.0
58.90	323.0
60.00	839.0
61.00	5064.0
62.00	5633.0
63.00	4890.0
64.00	419.0
64.90	742.0
66.10	99.0
67.10	300.0
68.00	10629.0
69.00	10755.0
70.00	744.0
70.90	56.0
72.00	865.0
73.00	5971.0
74.00	19104.0
75.00	53320.0
76.10	4971.0
76.90	762.0
77.90	681.0
78.90	5178.0
80.00	1208.0
80.90	5216.0
81.90	1185.0
83.10	255.0
85.20	85.0
86.90	4779.0
87.90	3572.0
91.00	615.0
92.00	3415.0
93.00	4719.0
94.00	12517.0
95.00	95576.0
96.00	5851.0
96.90	199.0
103.00	278.0
103.90	773.0
104.90	259.0
105.90	600.0
106.90	179.0
109.80	121.0
110.70	198.0
111.00	213.0
112.10	75.0
113.10	165.0
114.90	169.0
115.90	505.0
116.90	719.0
118.10	361.0
118.90	775.0
119.70	73.0
121.00	63.0
123.80	100.0
124.80	297.0
126.70	196.0
128.00	434.0
128.80	215.0
130.00	317.0
131.00	159.0
132.00	71.0
132.90	827.0
134.80	262.0
136.90	300.0
139.40	50.0
140.00	74.0
140.90	1453.0
142.00	315.0
142.80	1361.0
143.80	187.0

Instrument :
MSVOA_W
ClientSampleId :
BFB566

145.10	237.0
146.00	199.0
147.00	168.0
148.10	317.0
149.90	198.0
151.00	59.0
151.50	72.0
153.00	185.0
154.80	246.0
156.90	286.0
161.00	199.0
162.10	57.0
163.10	238.0
164.90	88.0
166.10	108.0
168.70	73.0
170.60	119.0
171.80	909.0
174.00	70008.0
175.00	5757.0
175.90	68784.0
177.00	4782.0
177.80	170.0
179.00	245.0
180.70	107.0
189.10	107.0
191.10	763.0
193.00	950.0
194.00	238.0
195.30	97.0
203.10	86.0
205.00	105.0
205.70	93.0
207.10	585.0
209.10	131.0
248.90	498.0
250.20	153.0
250.90	254.0
251.90	100.0
265.00	767.0
266.00	319.0
267.10	248.0
277.90	110.0
279.10	220.0
279.80	210.0
281.20	8824.0
282.10	2707.0
283.10	1484.0
284.00	231.0

Instrument :
MSVOA_W
ClientSampleId :
BFB566

m/z	Abundance
35.90	880.0
37.00	4902.0
38.10	3952.0
39.10	1474.0
40.00	528.0
41.00	123.0
43.10	146.0
44.10	1089.0
45.00	799.0
46.10	185.0
47.00	946.0
48.00	499.0
49.00	4600.0
50.00	17760.0
51.10	5332.0
52.10	159.0
52.90	91.0
55.00	498.0
56.00	1718.0
57.00	2997.0
58.10	144.0
58.80	158.0
60.00	864.0
61.10	5192.0
62.00	5440.0
63.00	4319.0
64.10	474.0
65.10	339.0
66.00	81.0
67.00	460.0
68.00	9908.0
69.00	10389.0
70.10	974.0
70.90	102.0
72.10	506.0
73.00	5592.0
74.00	17696.0
75.10	47864.0
76.10	4406.0
77.10	623.0
78.90	4711.0
80.00	1310.0
81.00	4732.0
81.90	1095.0
83.00	233.0
83.70	79.0
86.10	308.0
86.90	3945.0
88.00	4022.0
90.80	588.0
91.90	2731.0
92.90	4319.0
94.00	11959.0
95.00	94088.0
96.00	6676.0
97.20	158.0
103.00	218.0
103.90	537.0
104.90	264.0
106.10	441.0
106.80	209.0
109.80	108.0
110.90	195.0
112.10	184.0
112.90	223.0
114.90	158.0
115.80	500.0
116.90	869.0
118.00	323.0
119.00	803.0
123.90	131.0
125.30	143.0
127.90	442.0
129.00	157.0
130.00	498.0
131.00	142.0
131.70	55.0
133.00	588.0
133.60	183.0
135.00	334.0
136.00	75.0
137.00	210.0
140.00	126.0
141.00	1291.0
142.00	291.0
143.10	1088.0
144.10	79.0
145.10	171.0
145.90	140.0
147.90	261.0
148.90	121.0
149.90	88.0

Instrument :
MSVOA_W
ClientSampleId :
BFB566

152.90	82.0
153.80	80.0
154.80	199.0
156.90	180.0
157.40	67.0
158.00	61.0
158.60	211.0
159.20	105.0
161.20	217.0
165.00	58.0
167.90	53.0
168.60	72.0
169.50	69.0
170.50	181.0
171.20	139.0
171.90	575.0
174.00	69120.0
174.90	6090.0
176.00	68144.0
177.00	4812.0
177.90	205.0
179.00	62.0
191.10	242.0
192.40	106.0
193.00	773.0
194.20	130.0
195.20	101.0
203.20	60.0
205.00	114.0
206.70	188.0
207.20	384.0
207.80	53.0
249.10	441.0
250.00	89.0
251.00	113.0
265.10	444.0
266.10	225.0
267.10	189.0
277.80	69.0
279.40	56.0
280.10	228.0
281.00	4440.0
283.10	843.0
284.20	150.0
285.00	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB566