

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060421\
Data File : VW019123.D
Acq On : 04 Jun 2021 10:57
Operator : SY/VA
Sample : VW0604SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
VBLK130

Manual Integrations
APPROVED

MMDadoda
6/7/2021 7:15:13 PM

Quant Time: Jun 05 00:38:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 05 00:35:45 2021
Response via : Initial Calibration

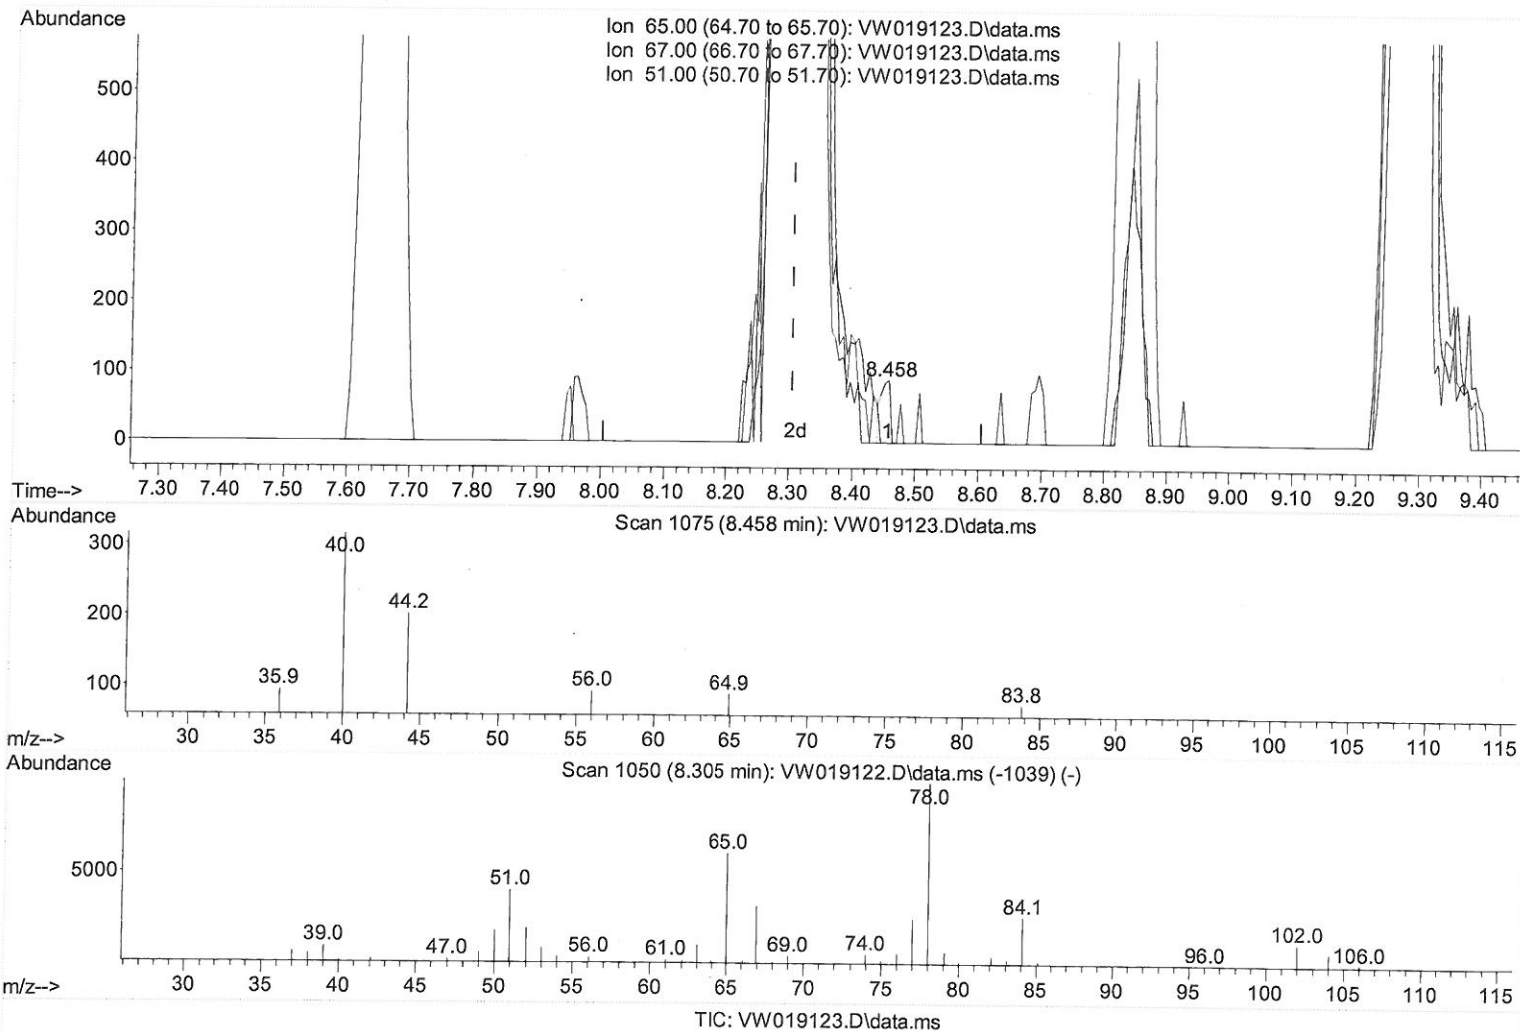

(26) 1,2-Dichloroethane-d4 (S)

8.458min (+ 0.152) 0.01 ug/L

response 89

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.70	51.69
51.00	98.00	83.15
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060421\
 Data File : VW019123.D
 Acq On : 04 Jun 2021 10:57
 Operator : SY/VA
 Sample : VW0604SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK130

Manual Integrations
 APPROVED

MMDadoda
 6/7/2021 7:15:13 PM

Quant Time: Jun 05 00:38:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 05 00:35:45 2021
 Response via : Initial Calibration

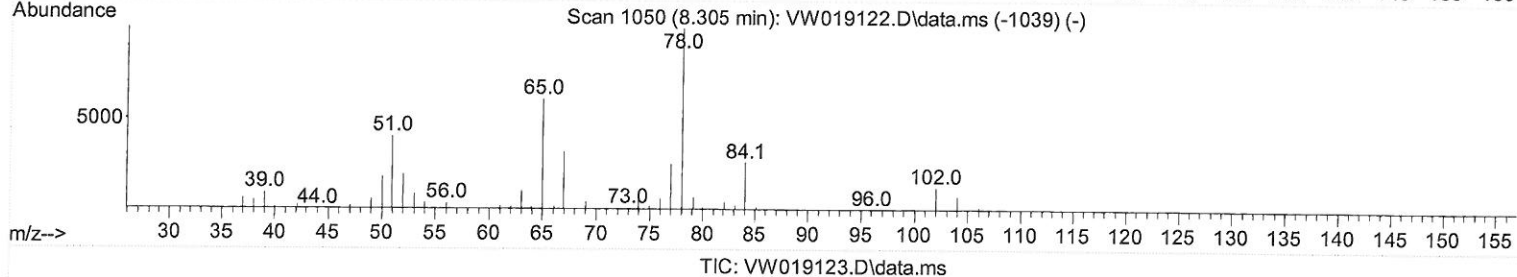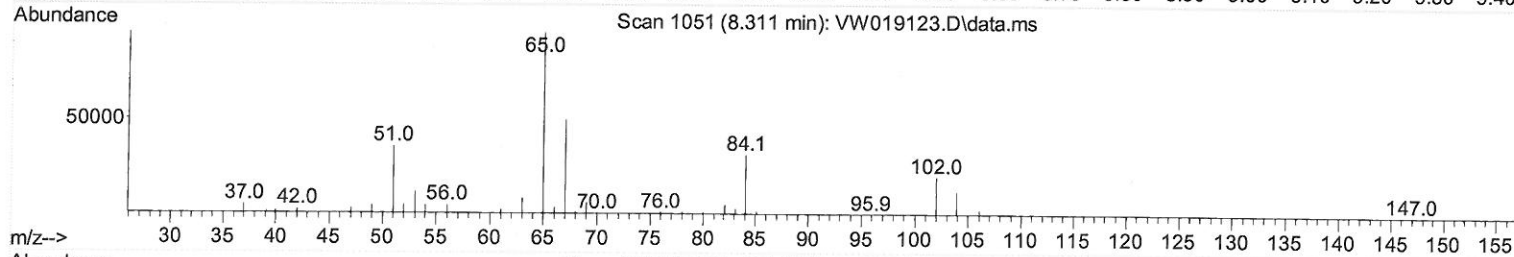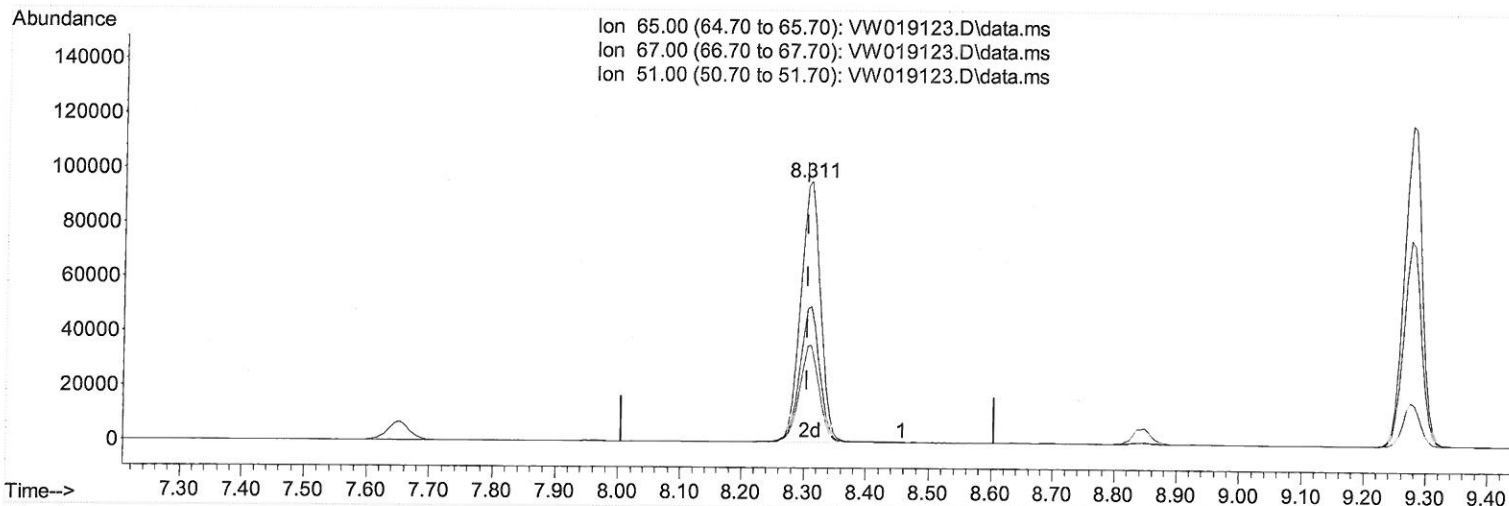

(26) 1,2-Dichloroethane-d4 (S)

8.311min (+ 0.006) 24.38 ug/L m

response 213222

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.70	0.02#
51.00	98.00	0.03#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060421\
 Data File : VW019123.D
 Acq On : 04 Jun 2021 10:57
 Operator : SY/VA
 Sample : VW0604SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK130

Manual Integrations
 APPROVED

MMDadoda
 6/7/2021 7:15:13 PM

Quant Time: Jun 05 00:38:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 05 00:35:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	579973	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	528326	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	244274	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	193837	25.275	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 101.080%			
7) Chloroethane-d5	2.898	69	159137	24.363	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 97.440%			
11) 1,1-Dichloroethene-d2	4.025	63	280436	18.404	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 73.600%			
21) 2-Butanone-d5	7.086	46	85360	42.491	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 84.980%			
24) Chloroform-d	7.653	84	389033	24.950	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 99.800%			
26) 1,2-Dichloroethane-d4	8.311	65	213222m	24.379	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 97.520%			
32) Benzene-d6	8.275	84	794314	26.388	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 105.560%			
36) 1,2-Dichloropropane-d6	9.274	67	236576	25.925	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 103.720%			
41) Toluene-d8	10.323	98	730392	26.421	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 105.680%			
43) trans-1,3-Dichloroprop...	10.579	79	92272	23.347	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 93.400%			
47) 2-Hexanone-d5	10.927	63	69700	45.042	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 90.080%			
56) 1,1,2,2-Tetrachloroeth...	12.695	84	174674	23.205	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 92.800%			
66) 1,2-Dichlorobenzene-d4	13.853	152	236978	27.795	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 111.160%			
Target Compounds						
16) Methylene chloride	4.928	84	17315	1.609	ug/L	89
42) Toluene	10.390	91	13697	0.366	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

06/14/21 sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060421\
Data File : VW019123.D
Acq On : 04 Jun 2021 10:57
Operator : SY/VA
Sample : VW0604SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK130

Manual Integrations
APPROVED

MMDadoda
6/7/2021 7:15:13 PM

Quant Time: Jun 05 00:38:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 05 00:35:45 2021
Response via : Initial Calibration

