

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060421\
 Data File : VW019127.D
 Acq On : 04 Jun 2021 12:53
 Operator : SY/VA
 Sample : VIBLK123
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK123

Quant Time: Jun 05 00:39:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 05 00:35:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	715774	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	642667	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	311239	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	230084	24.309	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	97.240%		
7) Chloroethane-d5	2.897	69	168854	20.946	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	83.800%		
11) 1,1-Dichloroethene-d2	4.031	63	316019	16.805	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	67.200%		
21) 2-Butanone-d5	7.086	46	95748	38.619	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	77.240%		
24) Chloroform-d	7.653	84	411760	21.397	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	85.600%		
26) 1,2-Dichloroethane-d4	8.311	65	230037	21.311	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	85.240%		
32) Benzene-d6	8.275	84	849783	23.208	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	92.840%		
36) 1,2-Dichloropropane-d6	9.274	67	244767	22.050	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	88.200%		
41) Toluene-d8	10.323	98	786017	23.375	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	93.480%		
43) trans-1,3-Dichloroprop...	10.579	79	106211	22.093	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	88.360%		
47) 2-Hexanone-d5	10.926	63	81252	43.166	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	86.340%		
56) 1,1,2,2-Tetrachloroeth...	12.694	84	185289	20.235	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	80.960%		
66) 1,2-Dichlorobenzene-d4	13.853	152	260984	24.024	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	96.080%		
Target Compounds						Qvalue
16) Methylene chloride	4.921	84	23748	1.788	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060421\
Data File : VW019127.D
Acq On : 04 Jun 2021 12:53
Operator : SY/VA
Sample : VIBLK123
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK123

Quant Time: Jun 05 00:39:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 05 00:35:45 2021
Response via : Initial Calibration

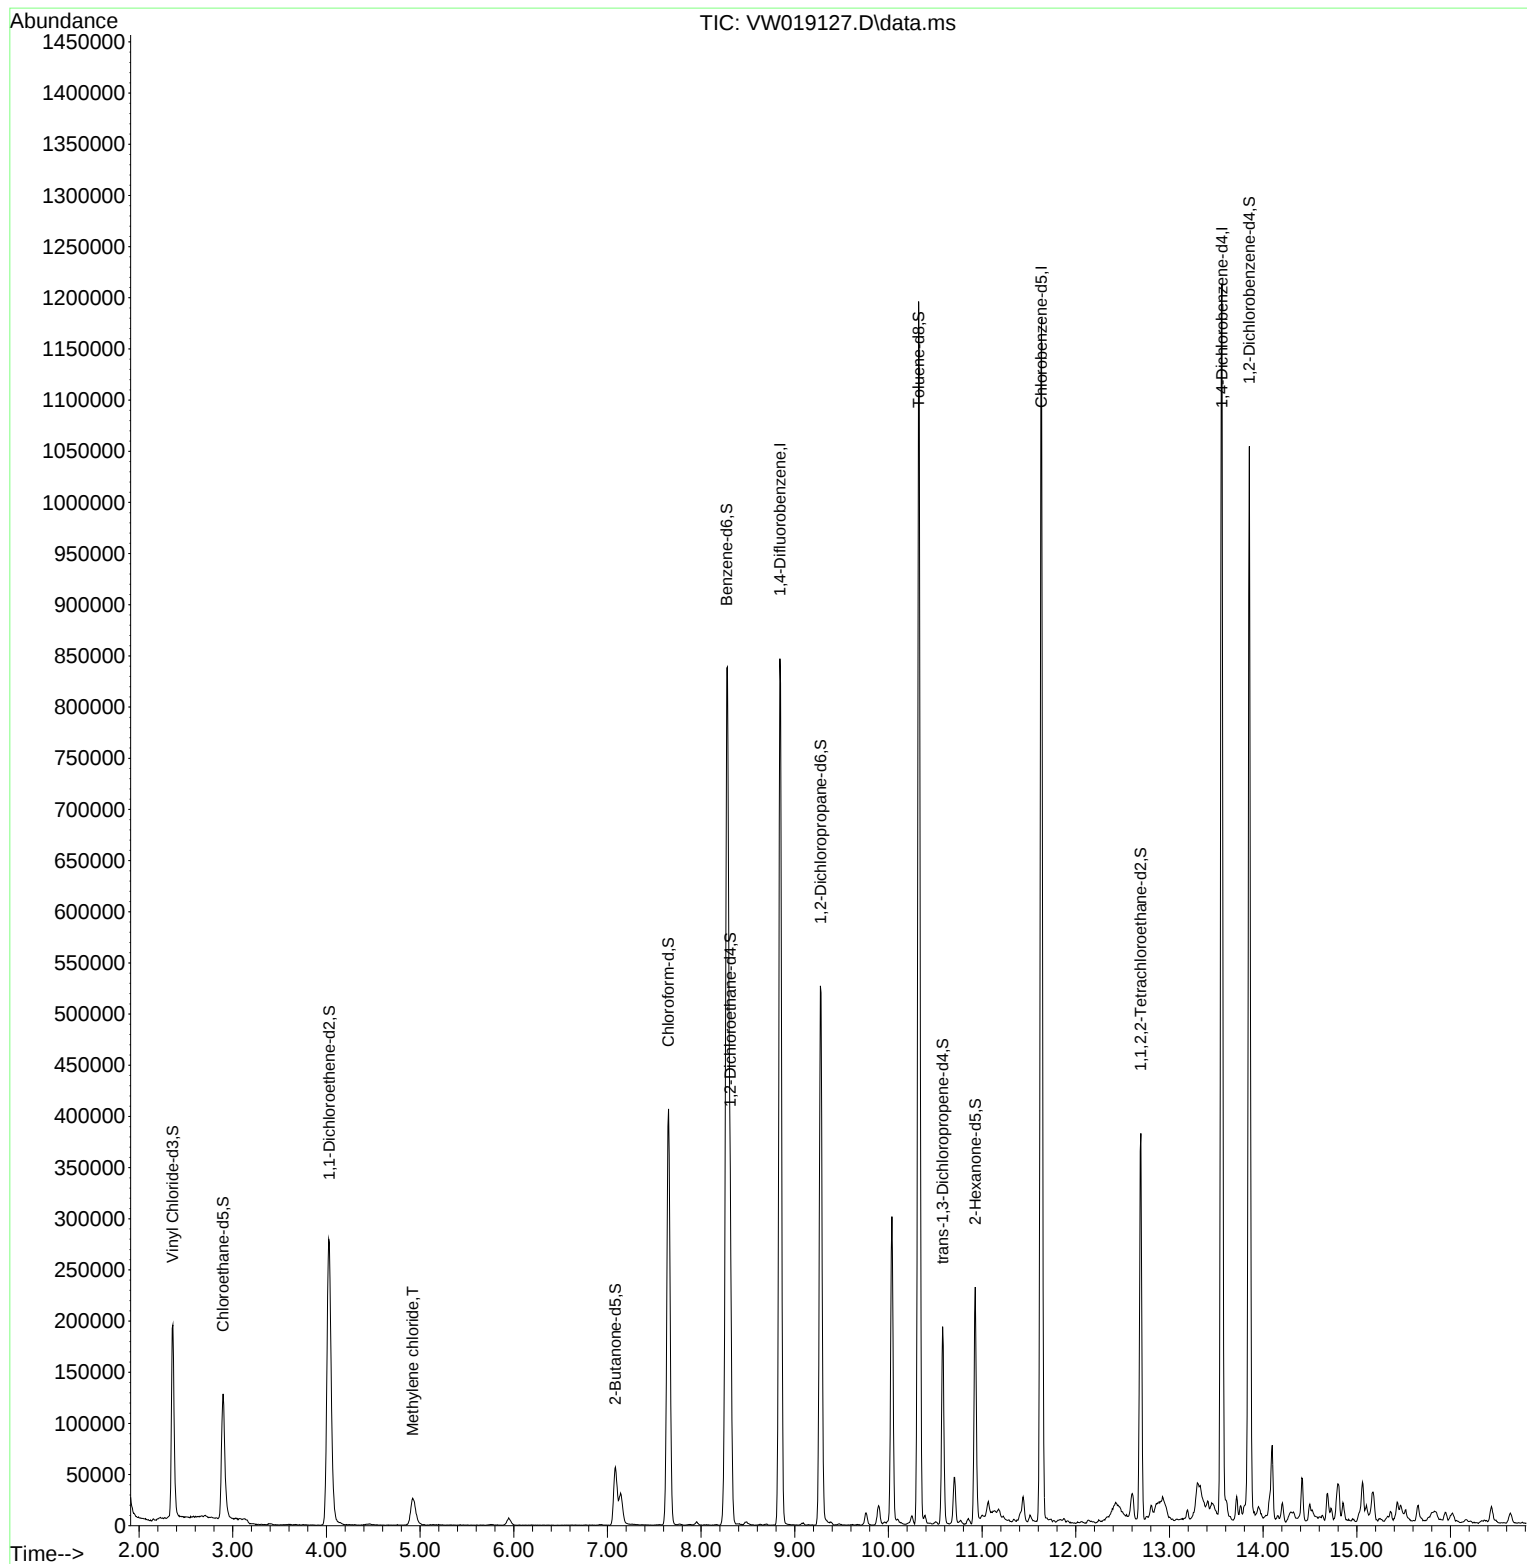

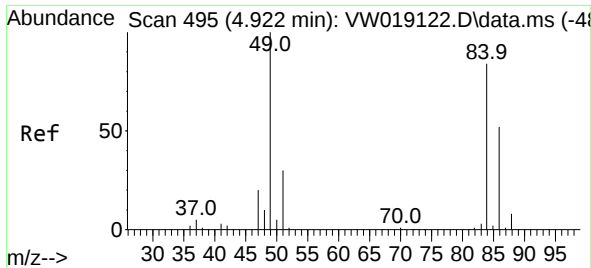

#16
Methylene chloride
Concen: 1.788 ug/L
RT: 4.921 min Scan# 495
Delta R.T. -0.000 min
Lab File: VW019127.D
Acq: 04 Jun 2021 12:53

Instrument :
MSVOA_W
ClientSampleId :
VIBLK123

Tgt Ion:	84	Resp:	23748
Ion	Ratio	Lower	Upper
84	100		
86	68.4	45.3	84.1
49	128.9	86.6	160.8

