

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW060619\
 Data File : VW010709.D
 Acq On : 06 Jun 2019 14:54
 Operator : SY/VA
 Sample : K3211-05
 Misc : 6.43G/5ML/MSVOA W/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 RT-5124

Quant Time: Jun 07 08:26:24 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W060419S.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 05 03:21:19 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	145907	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	237293	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	201005	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	88497	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.30	65	90757	52.77	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.54%	
35) Dibromofluoromethane	7.88	113	65674	50.99	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.98%	
50) Toluene-d8	10.32	98	305050	54.01	ug/l	0.00
Spiked Amount 50.000			Recovery	=	108.02%	
62) 4-Bromofluorobenzene	12.62	95	104437	50.82	ug/l	0.00
Spiked Amount 50.000			Recovery	=	101.64%	
Target Compounds						
16) Acetone	4.13	43	12673	27.502	ug/l	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW060619\
Data File : VW010709.D
Acq On : 06 Jun 2019 14:54
Operator : SY/VA
Sample : K3211-05
Misc : 6.43G/5ML/MSVOA W/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
RT-5124

Quant Time: Jun 07 08:26:24 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W060419S.M
Quant Title : SW846 8260
QLast Update : Wed Jun 05 03:21:19 2019
Response via : Initial Calibration

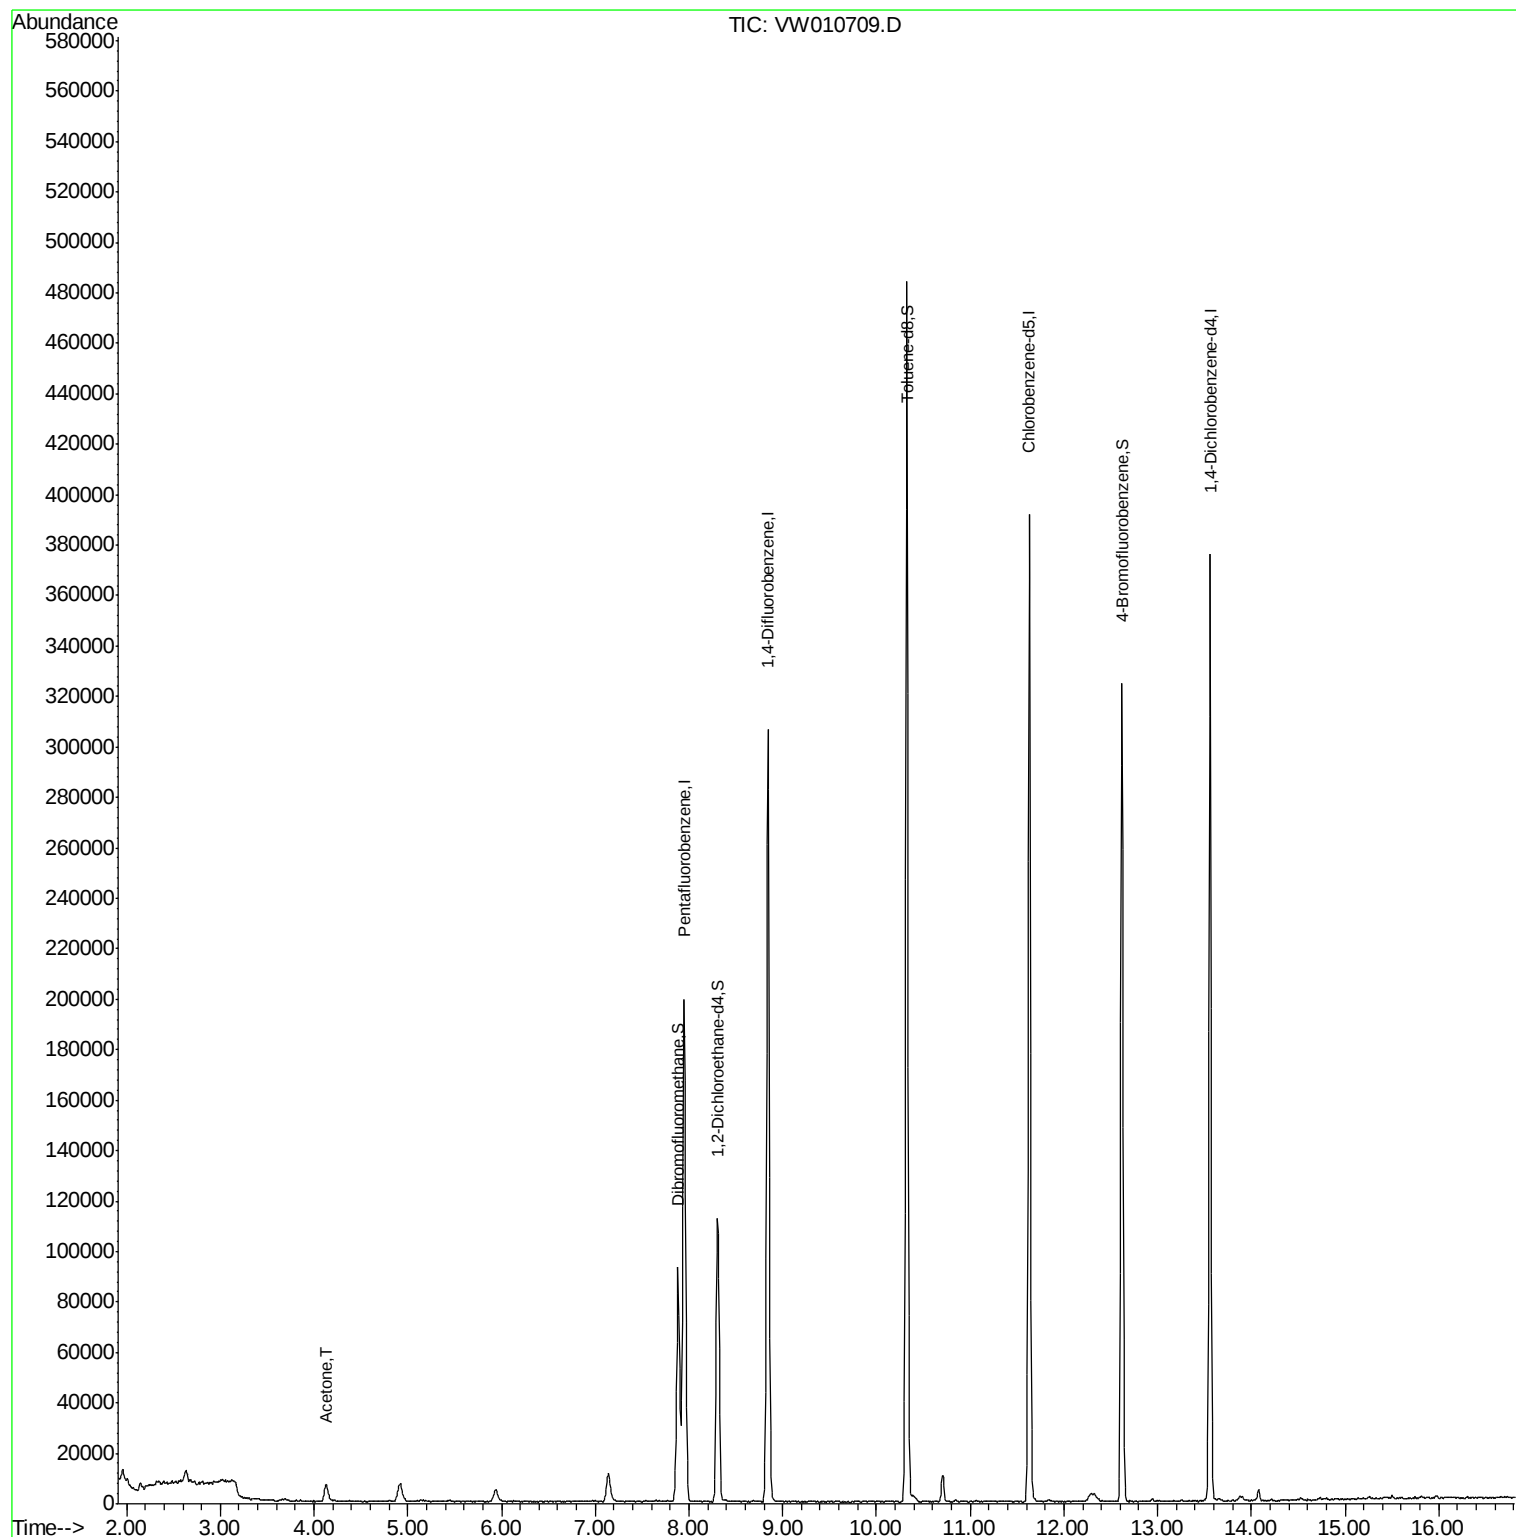

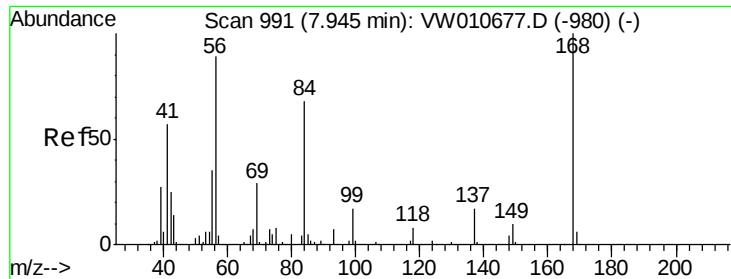

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. 0.01 min

Lab File: VW010709.D

Acq: 06 Jun 2019 14:54

Instrument :

MSVOA_W

ClientSampleId :


RT-5124

Tot Ion:168 Resp: 145907

Ion Ratio Lower Upper




168 100

99 60.4 47.7 71.5

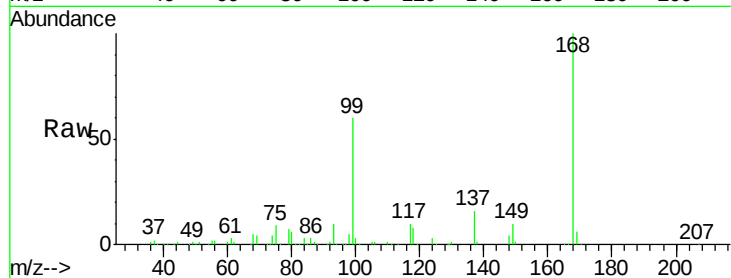

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

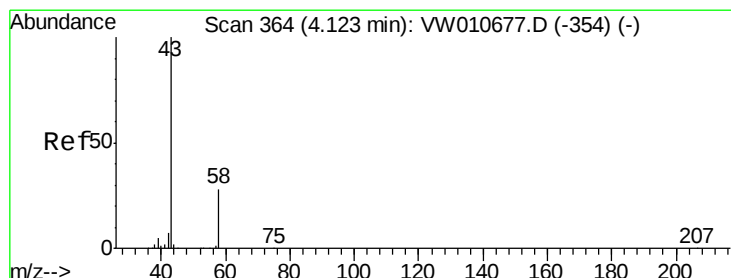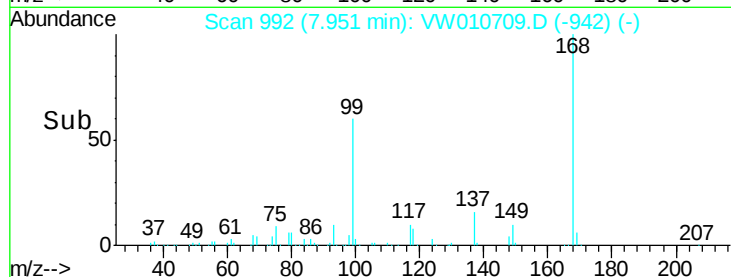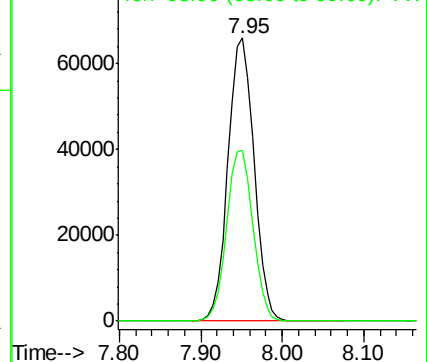

#16

Acetone

Concen: 27.502 ug/l

RT: 4.13 min Scan# 365

Delta R.T. 0.01 min

Lab File: VW010709.D


Acq: 06 Jun 2019 14:54

Tgt Ion: 43 Resp: 12673

Ion Ratio Lower Upper



43 100


58 25.1 22.1 33.1

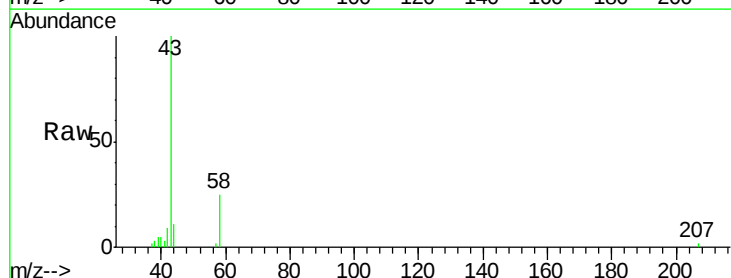

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW



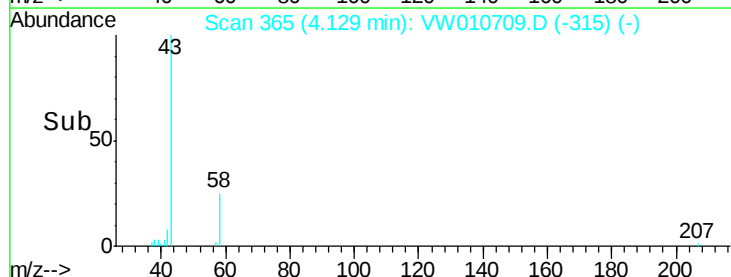
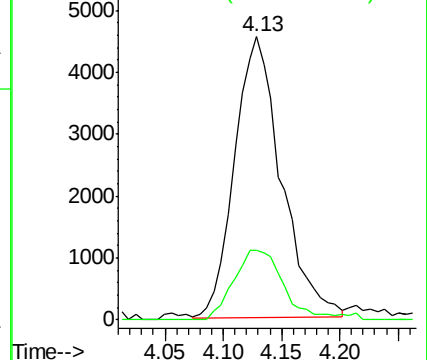


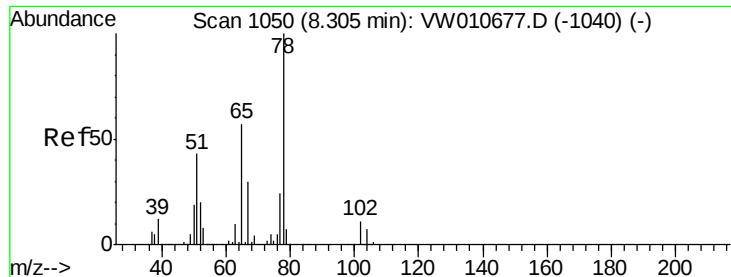

#33
 1,2-Dichloroethane-d4
 Concen: 52.773 ug/l
 RT: 8.30 min Scan# 1050
 Delta R.T. -0.00 min
 Lab File: VW010709.D
 Acq: 06 Jun 2019 14:54




Instrument :
 MSVOA_W
 ClientSampleId :
 RT-5124


Tot Ion: 65 Resp: 90757
 Ion Ratio Lower Upper
 65 100
 67 51.2 0.0 102.6

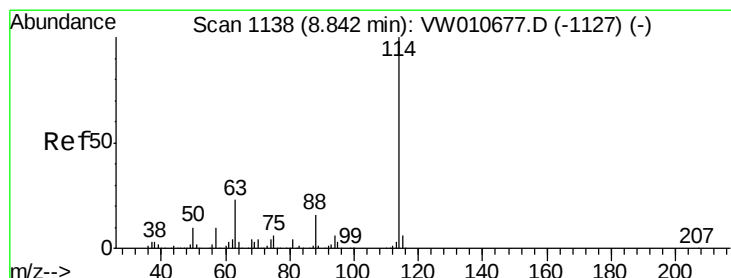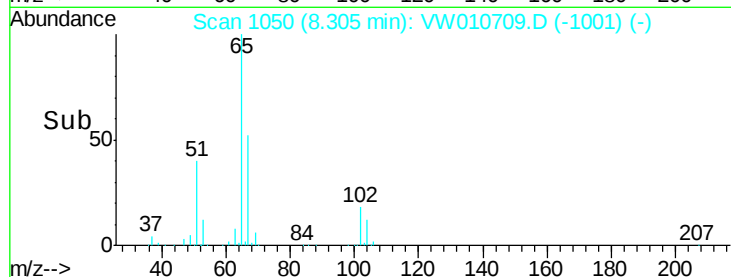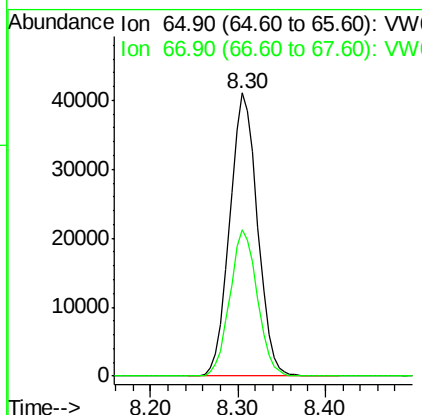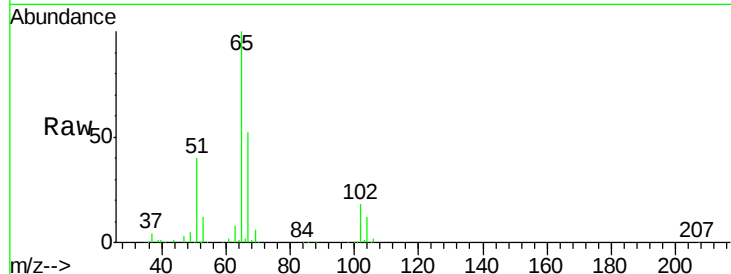

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.84 min Scan# 1138
 Delta R.T. -0.00 min
 Lab File: VW010709.D
 Acq: 06 Jun 2019 14:54

Tgt Ion: 114 Resp: 237293
 Ion Ratio Lower Upper
 114 100
 63 24.2 0.0 46.4
 88 16.2 0.0 32.2

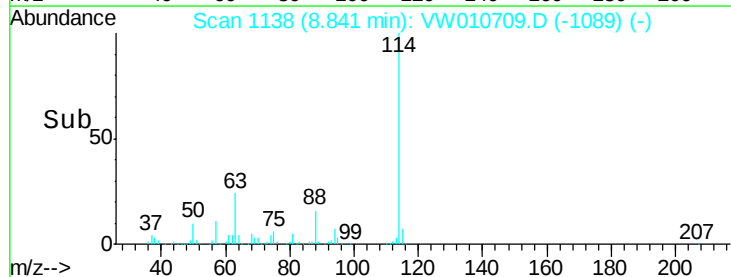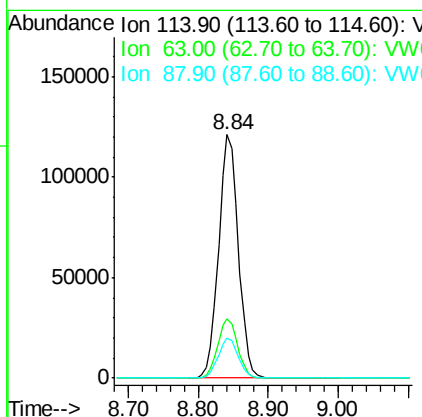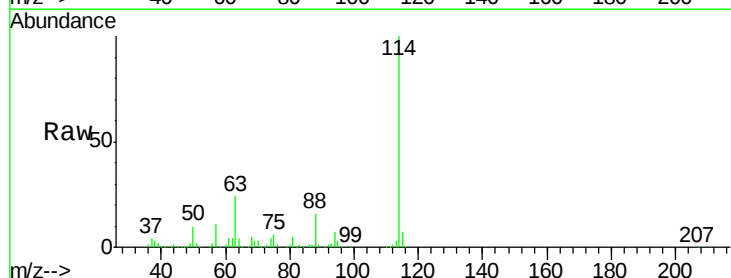


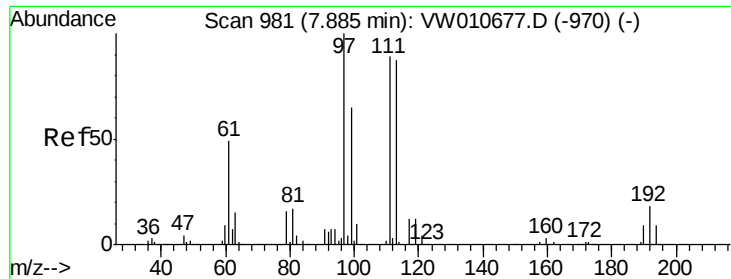




#35
 Dibromofluoromethane
 Concen: 50.990 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. -0.00 min
 Lab File: VW010709.D
 Acq: 06 Jun 2019 14:54

Instrument :
 MSVOA_W
 ClientSampleId :
 RT-5124

Tot Ion	Ratio	Lower	Upper
113	100		
111	102.9	82.6	123.8
192	19.9	16.4	24.6

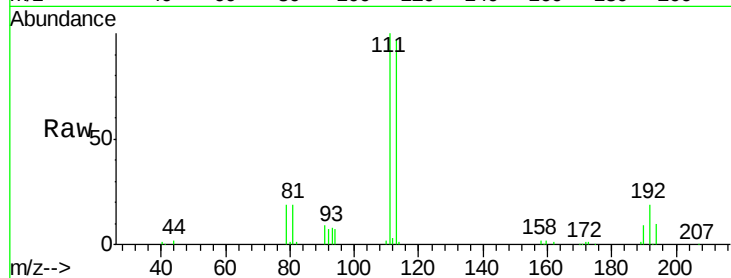


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

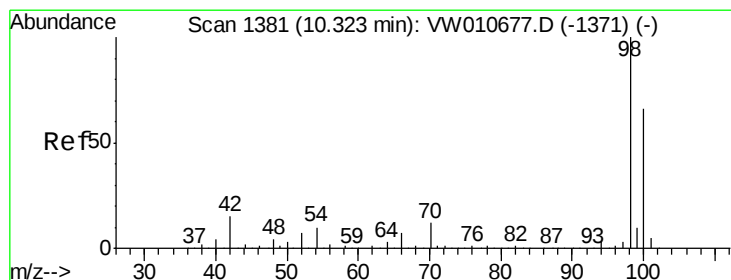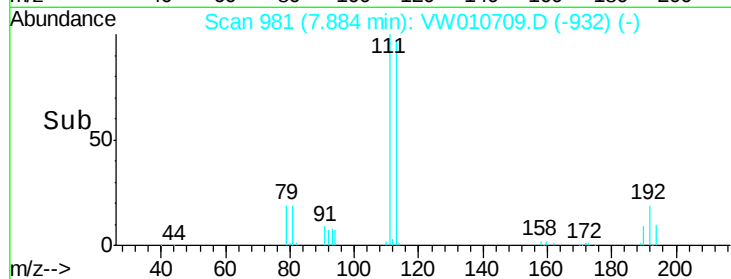
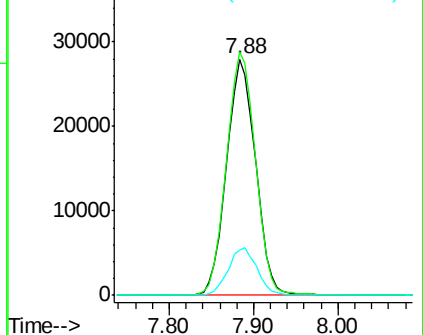



#50
 Toluene-d8
 Concen: 54.011 ug/l
 RT: 10.32 min Scan# 1381
 Delta R.T. -0.00 min
 Lab File: VW010709.D
 Acq: 06 Jun 2019 14:54

Tgt Ion	Ratio	Lower	Upper
98	100		
100	66.1	53.0	79.6

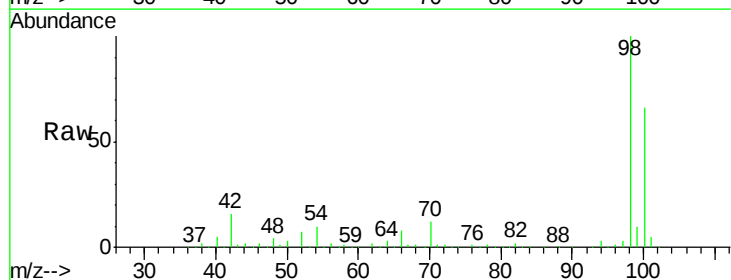

Abundance Ion 98.00 (97.70 to 98.70): VW
 Ion 100.00 (99.70 to 100.70): VW



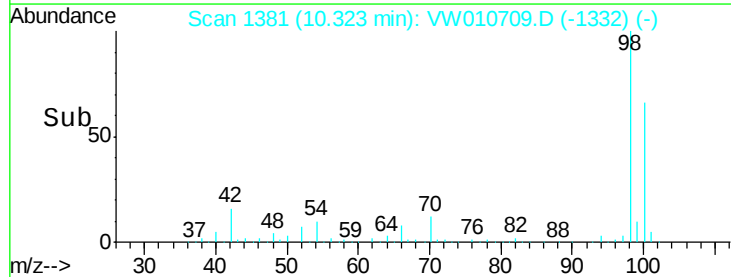
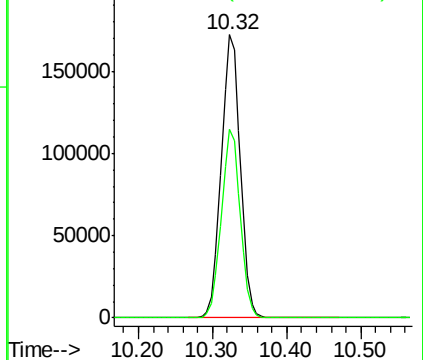


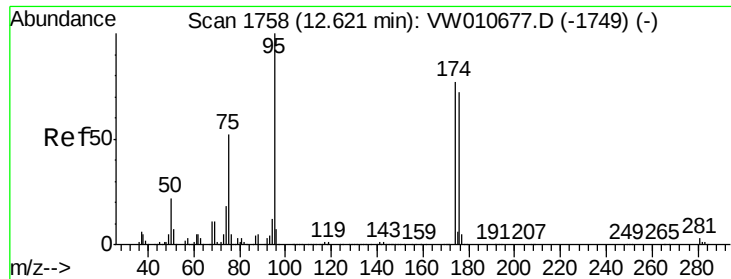

#62
4-Bromofluorobenzene
Concen: 50.816 ug/l
RT: 12.62 min Scan# 1758
Delta R.T. -0.00 min
Lab File: VW010709.D
Acq: 06 Jun 2019 14:54




Instrument :
MSVOA_W
ClientSampleId :
RT-5124


Tot Ion: 95 Resp: 104437
Ion Ratio Lower Upper
95 100
174 73.5 0.0 150.4
176 70.7 0.0 144.8

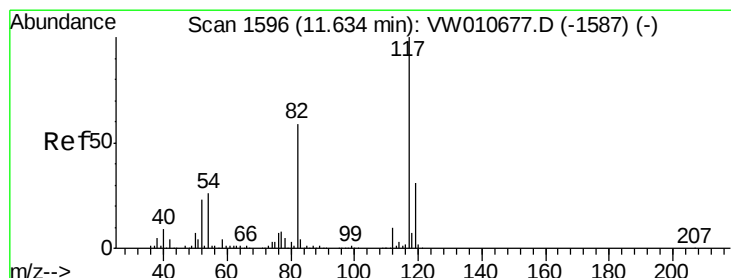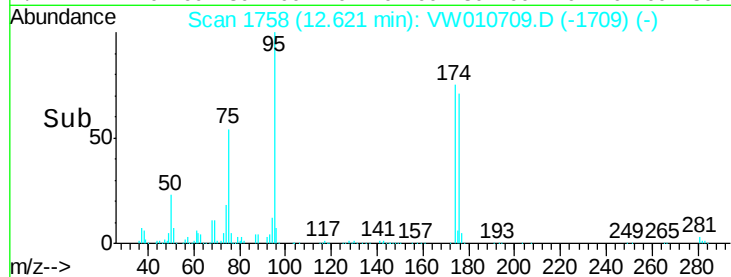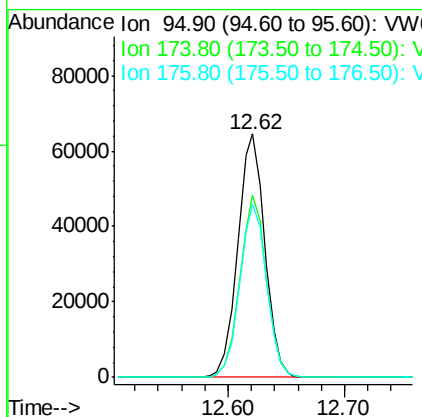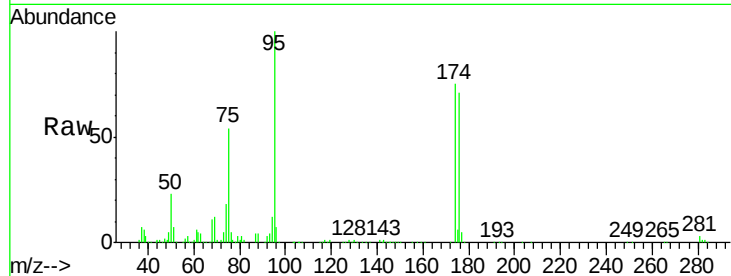

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. -0.00 min
Lab File: VW010709.D
Acq: 06 Jun 2019 14:54

Tgt Ion: 117 Resp: 201005
Ion Ratio Lower Upper
117 100
82 61.5 47.0 70.4
119 32.5 25.1 37.7

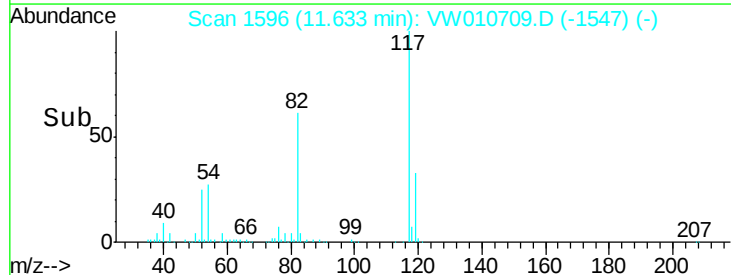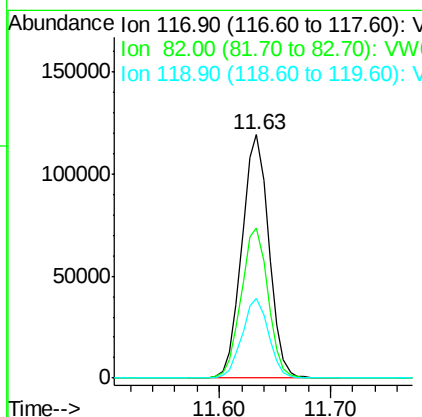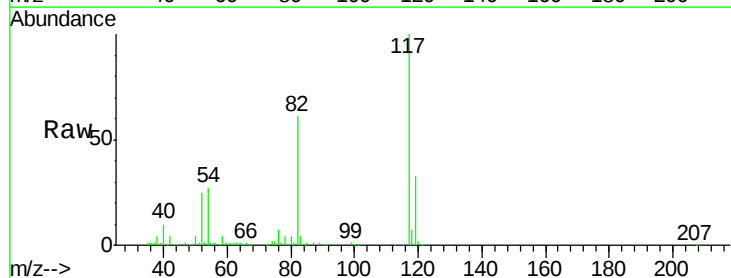

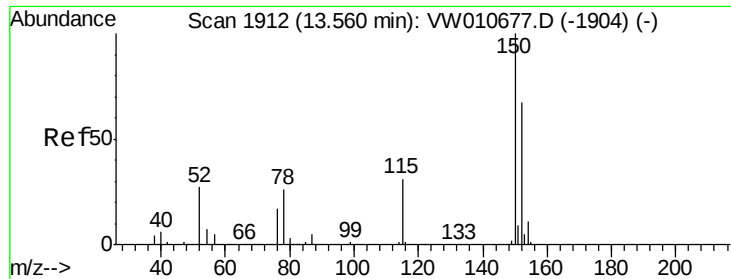

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. -0.00 min

Lab File: VW010709.D

Acq: 06 Jun 2019 14:54

Instrument :

MSVOA_W

ClientSampleId :

RT-5124


Tot Ion:152 Resp: 88497

Ion Ratio Lower Upper

152 100

115 61.5 29.8 89.3

150 159.2 0.0 345.0

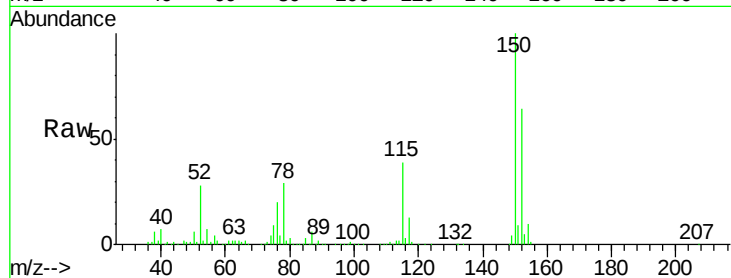

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

