

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060721\
 Data File : VW019147.D
 Acq On : 07 Jun 2021 14:36
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK128

Manual Integrations
 APPROVED

MMDadoda
 6/8/2021 4:44:15 PM

Quant Time: Jun 08 01:24:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 08 01:22:15 2021
 Response via : Initial Calibration

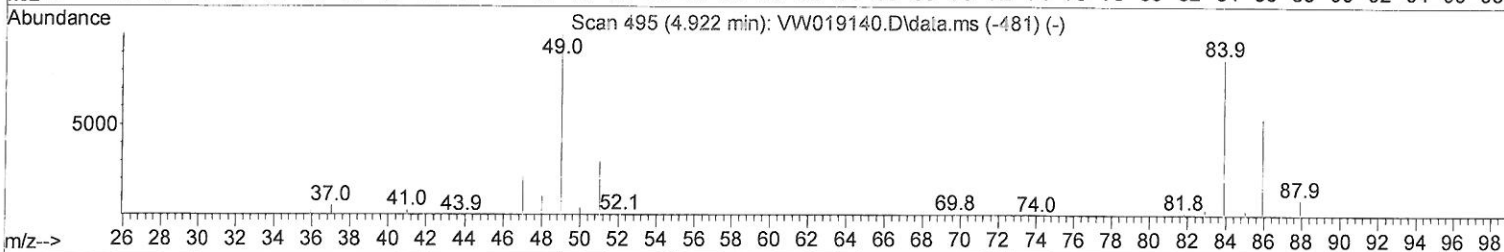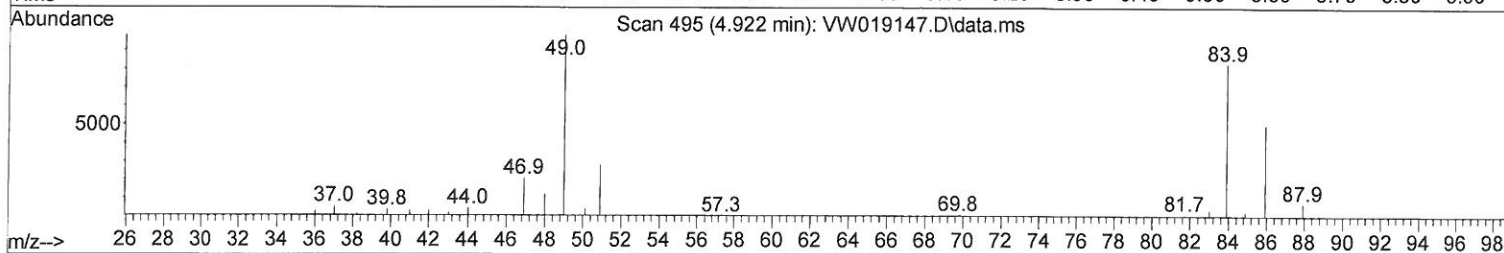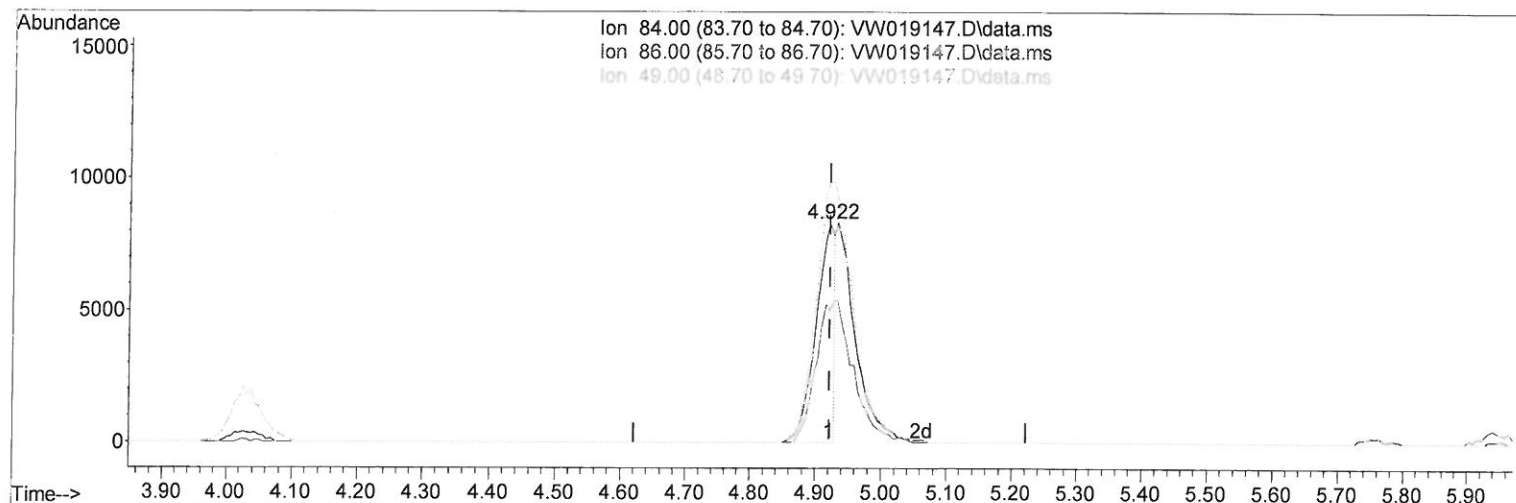

TIC: VW019147.D\data.ms

(16) Methylene chloride (T)

4.922min (+ 0.000) 1.59 ug/L

response 16350

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	60.00
49.00	123.70	118.38
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060721\
 Data File : VW019147.D
 Acq On : 07 Jun 2021 14:36
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 VIBLK128

Manual Integrations
 APPROVED

MMDadoda
 6/8/2021 4:44:15 PM

Quant Time: Jun 08 01:24:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 08 01:22:15 2021
 Response via : Initial Calibration

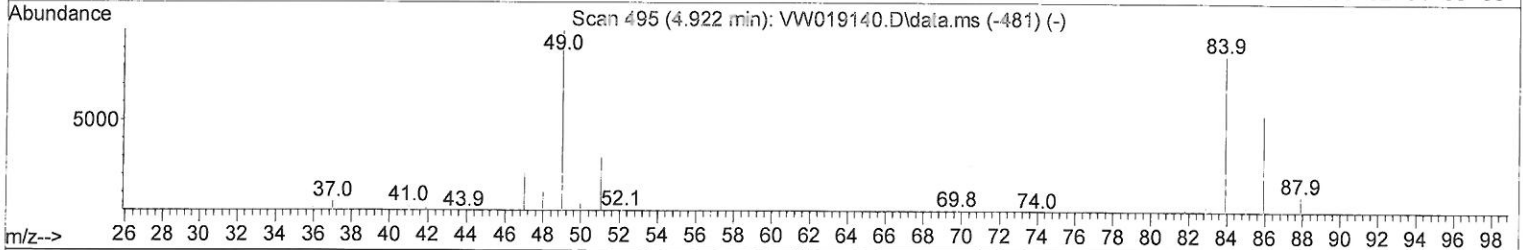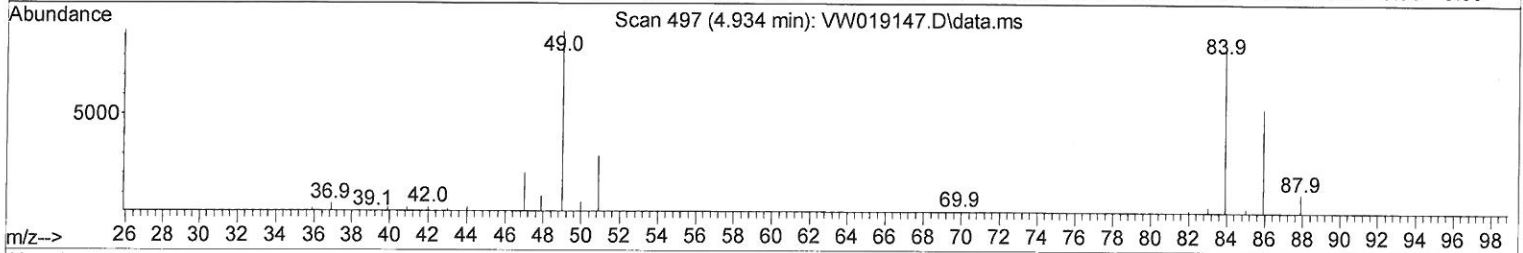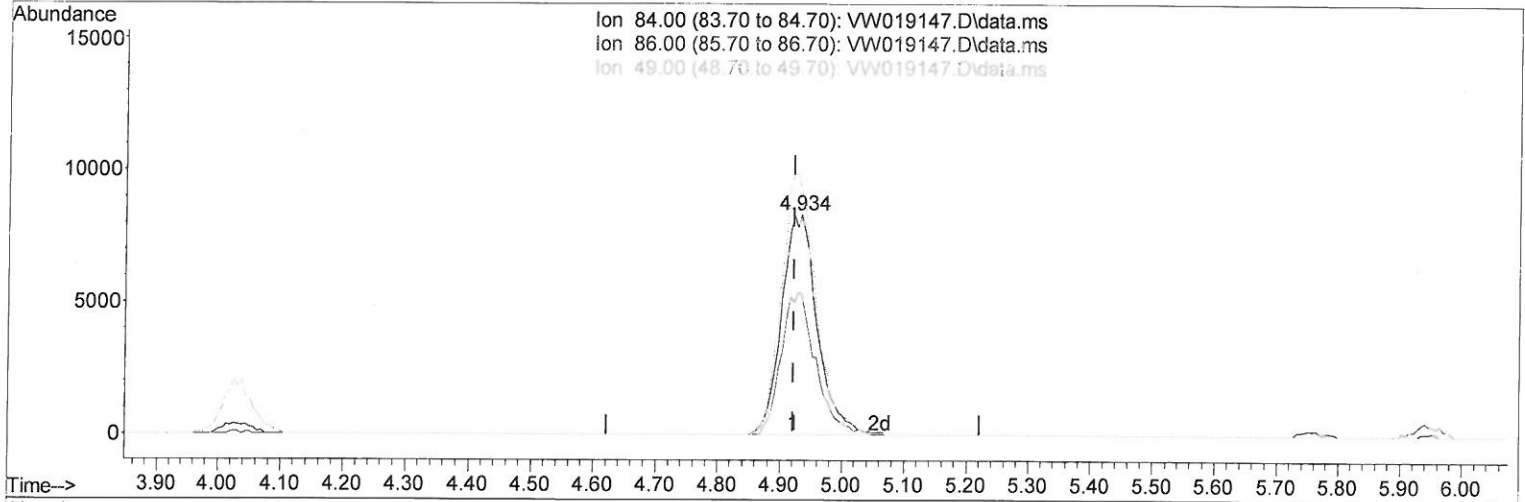

TIC: VW019147.D\data.ms

(16) Methylene chloride (T)

4.934min (+ 0.012) 3.22 ug/L m

response 33146

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	64.23
49.00	123.70	111.19
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060721\
 Data File : VW019147.D
 Acq On : 07 Jun 2021 14:36
 Operator : SY/VA
 Sample : VIBLK
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK128

Manual Integrations
 APPROVED

MMDadoda
 6/8/2021 4:44:15 PM

Quant Time: Jun 08 01:24:27 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 08 01:22:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	554568	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	499166	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	243328	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	152786	20.835	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	83.320%		
7) Chloroethane-d5	2.898	69	125876	20.154	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.600%		
11) 1,1-Dichloroethene-d2	4.025	63	222153	15.247	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	61.000%		
21) 2-Butanone-d5	7.080	46	88048	45.837	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	91.680%		
24) Chloroform-d	7.653	84	326984	21.931	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	87.720%		
26) 1,2-Dichloroethane-d4	8.311	65	185918	22.231	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	88.920%		
32) Benzene-d6	8.281	84	659591	23.193	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	92.760%		
36) 1,2-Dichloropropane-d6	9.275	67	200383	23.242	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	92.960%		
41) Toluene-d8	10.323	98	607792	23.271	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	93.080%		
43) trans-1,3-Dichloroprop...	10.579	79	82255	22.028	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	88.120%		
47) 2-Hexanone-d5	10.927	63	71214	48.709	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	97.420%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	162792	22.890	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	91.560%		
66) 1,2-Dichlorobenzene-d4	13.853	152	199705	23.514	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	94.040%		
Target Compounds						
16) Methylene chloride	4.934	84	33146m	3.221	ug/L	Qvalue
42) Toluene	10.390	91	11899	0.337	ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060721\
Data File : VW019147.D
Acq On : 07 Jun 2021 14:36
Operator : SY/VA
Sample : VIBLK
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK128

Manual Integrations
APPROVED

MMDadoda
6/8/2021 4:44:15 PM

Quant Time: Jun 08 01:24:27 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 08 01:22:15 2021
Response via : Initial Calibration

