

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060721\
 Data File : VW019141.D
 Acq On : 07 Jun 2021 11:22
 Operator : SY/VA
 Sample : VW0607SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK101

Quant Time: Jun 08 01:23:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 08 01:22:15 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	602565	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	554235	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	271959	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	189790	23.819	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.280%
7) Chloroethane-d5	2.898	69	157407	23.195	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.760%
11) 1,1-Dichloroethene-d2	4.025	63	277867	17.552	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.200%
21) 2-Butanone-d5	7.086	46	102062	48.900	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.800%
24) Chloroform-d	7.653	84	413622	25.532	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	102.120%
26) 1,2-Dichloroethane-d4	8.311	65	232036	25.535	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.120%
32) Benzene-d6	8.275	84	845057	26.762	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	107.040%
36) 1,2-Dichloropropane-d6	9.274	67	252827	26.411	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	105.640%
41) Toluene-d8	10.323	98	759138	26.177	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	104.720%
43) trans-1,3-Dichloroprop...	10.579	79	104384	25.177	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	100.720%
47) 2-Hexanone-d5	10.927	63	84564	52.093	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	104.180%
56) 1,1,2,2-Tetrachloroeth...	12.695	84	195098	24.706	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.840%
66) 1,2-Dichlorobenzene-d4	13.853	152	249656	26.301	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	105.200%
Target Compounds						Qvalue
16) Methylene chloride	4.922	84	22973	2.055	ug/L	99
42) Toluene	10.390	91	14614	0.373	ug/L	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060721\
Data File : VW019141.D
Acq On : 07 Jun 2021 11:22
Operator : SY/VA
Sample : VW0607SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK101

Quant Time: Jun 08 01:23:14 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 08 01:22:15 2021
Response via : Initial Calibration




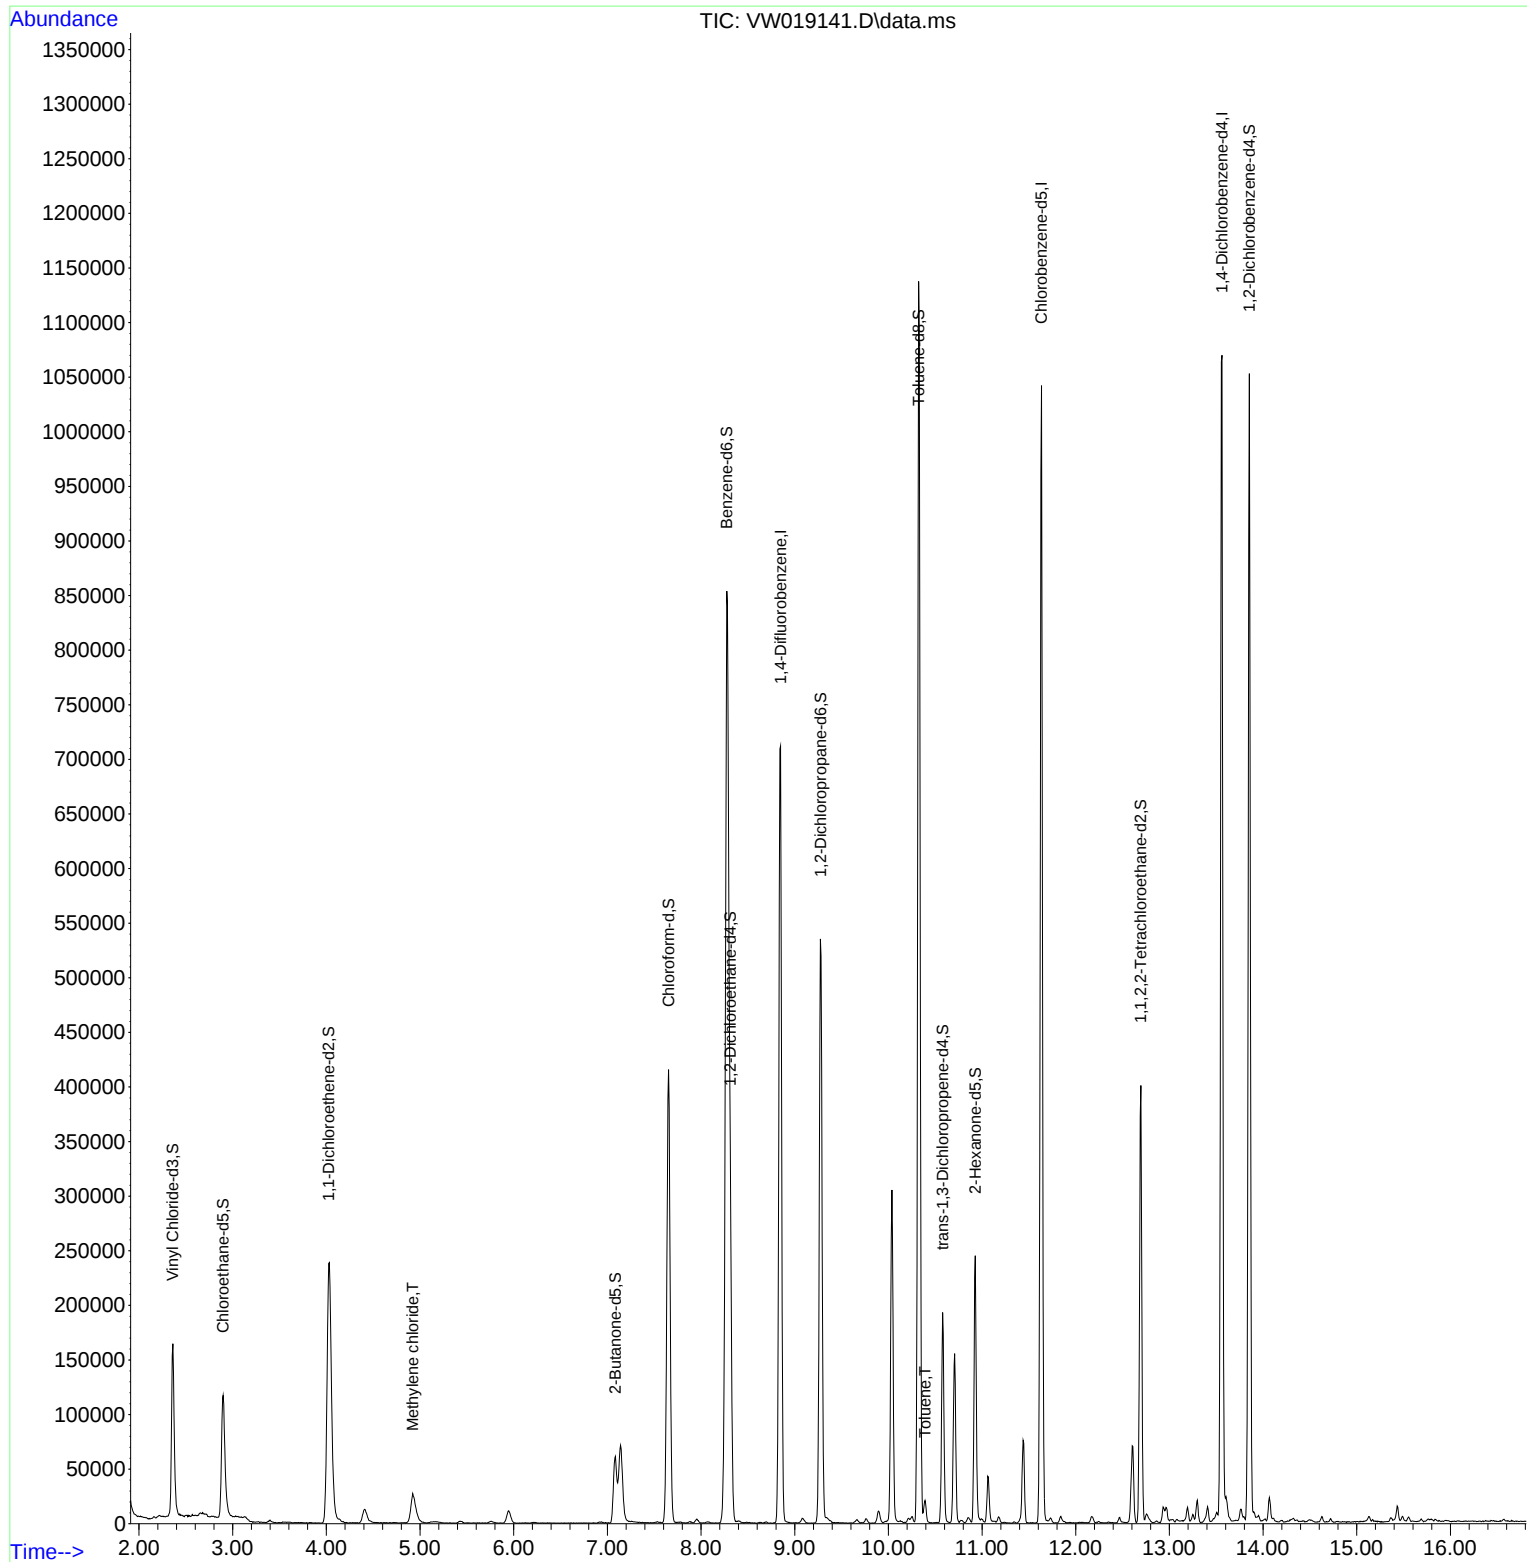


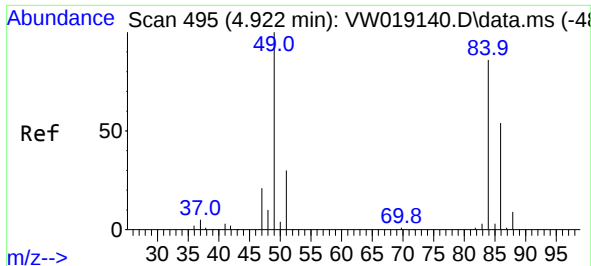

#16
Methylene chloride
Concen: 2.055 ug/L
RT: 4.922 min Scan# 495
Delta R.T. 0.000 min
Lab File: VW019141.D
Acq: 07 Jun 2021 11:22

Instrument :
MSVOA_W
ClientSampleId :
VBLK101

Tgt Ion:	84	Resp:	22973
Ion	Ratio	Lower	Upper
84	100		
86	64.5	45.3	84.1
49	122.7	86.6	160.8

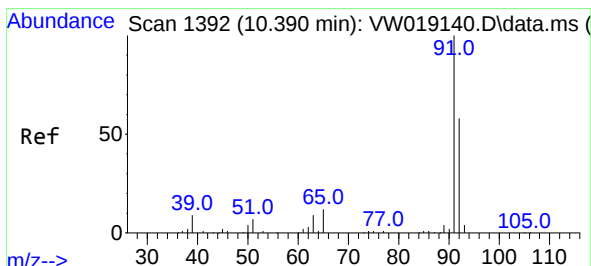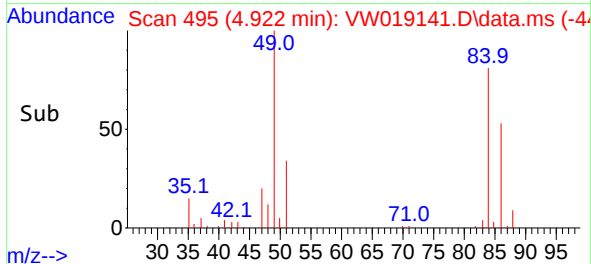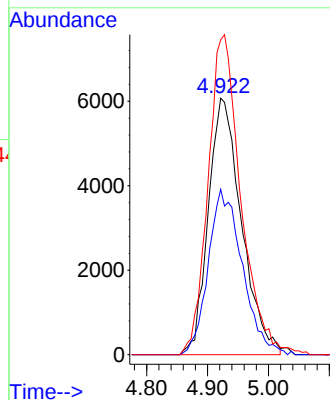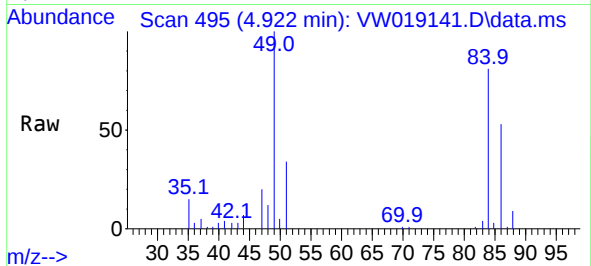

#42
Toluene
Concen: 0.373 ug/L
RT: 10.390 min Scan# 1392
Delta R.T. 0.000 min
Lab File: VW019141.D
Acq: 07 Jun 2021 11:22

Tgt Ion:	91	Resp:	14614
Ion	Ratio	Lower	Upper
91	100		
92	55.7	39.5	73.3

