

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060821\
 Data File : VW019156.D
 Acq On : 08 Jun 2021 14:04
 Operator : SY/VA
 Sample : M2649-06
 Misc : 4.40G/10ML/MSVOA_W/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG5J1

Manual Integrations
 APPROVED

MMDadoda
 6/9/2021 4:17:12 PM

Quant Time: Jun 09 01:05:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 09 01:04:22 2021
 Response via : Initial Calibration

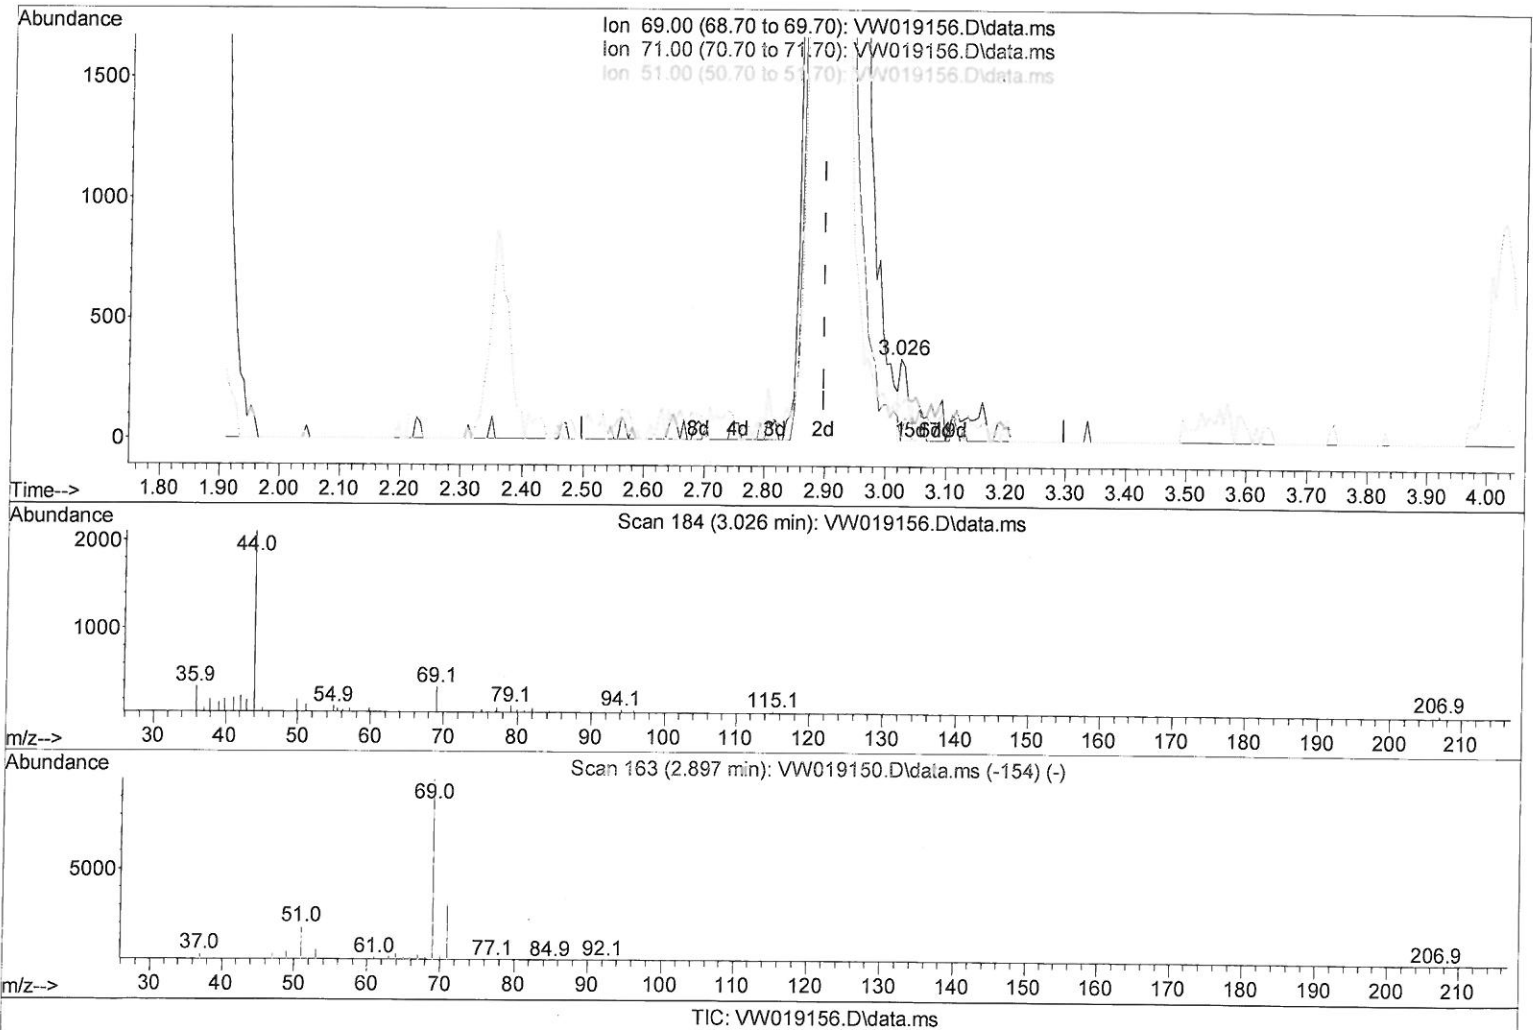

(7) Chloroethane-d5 (S)

3.026min (+ 0.128) 0.05 ug/L

response 360

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	33.33
51.00	28.40	35.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060821\
Data File : VW019156.D
Acq On : 08 Jun 2021 14:04
Operator : SY/VA
Sample : M2649-06
Misc : 4.40G/10ML/MSVOA_W/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampled :
BG5J1

Manual Integrations
APPROVED

MMDadoda
6/9/2021 4:17:12 PM

Quant Time: Jun 09 01:05:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 09 01:04:22 2021
Response via : Initial Calibration

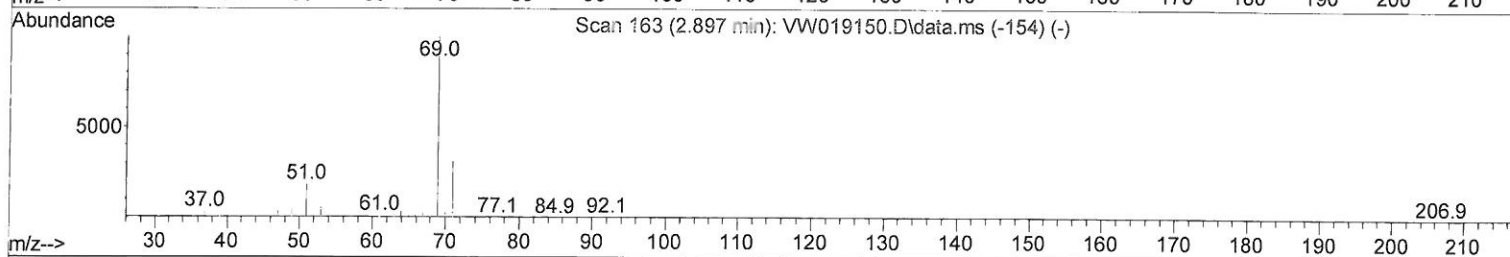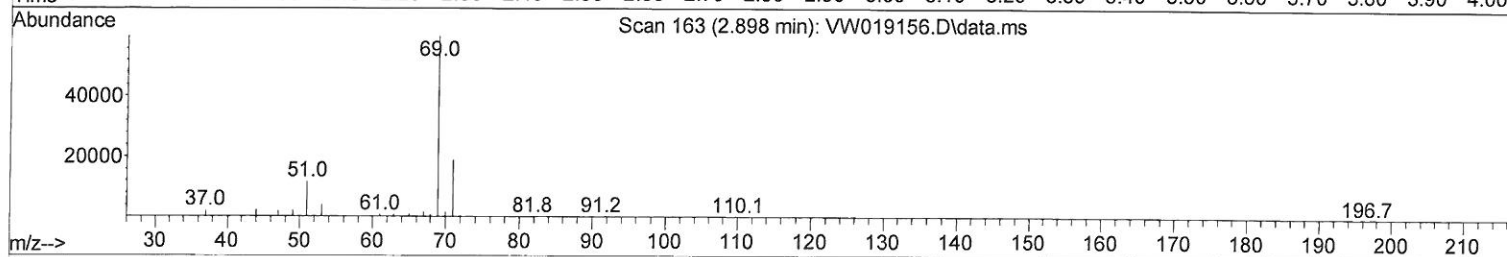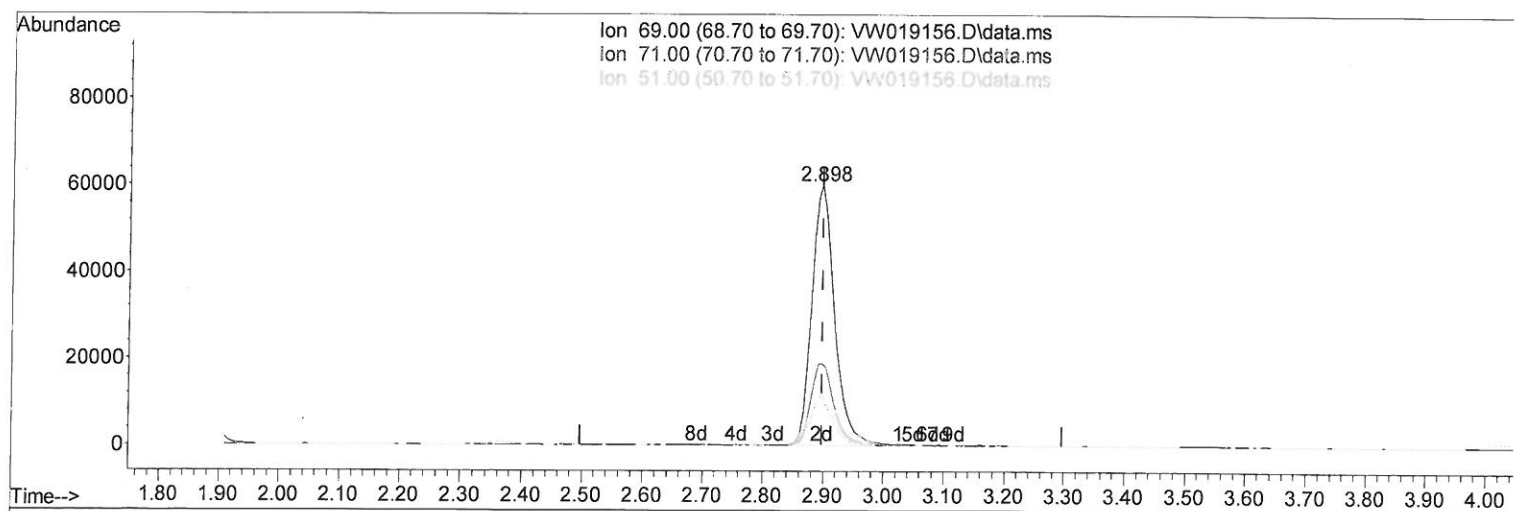

TIC: VW019156.D\data.ms

(7) Chloroethane-d5 (S)

2.898min (+ 0.000) 20.96 ug/L m

response 156935

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	0.08#
51.00	28.40	0.08#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060821\
 Data File : VW019156.D
 Acq On : 08 Jun 2021 14:04
 Operator : SY/VA
 Sample : M2649-06
 Misc : 4.40G/10ML/MSVOA_W/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG5J1

Manual Integrations
 APPROVED

MMDadoda
 6/9/2021 4:17:12 PM

Quant Time: Jun 09 01:05:53 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 09 01:04:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	664829	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	571720	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	256009	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	196141	22.311	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	89.240%		
7) Chloroethane-d5	2.898	69	156935m	20.959	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	83.840%		
11) 1,1-Dichloroethene-d2	4.025	63	269132	15.408	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	61.640%		
21) 2-Butanone-d5	7.086	46	78438	34.062	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	68.120%		
24) Chloroform-d	7.653	84	362957	20.306	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	81.240%		
26) 1,2-Dichloroethane-d4	8.311	65	197842	19.733	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	78.920%		
32) Benzene-d6	8.281	84	766841	23.542	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	94.160%		
36) 1,2-Dichloropropane-d6	9.274	67	227377	23.026	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	92.120%		
41) Toluene-d8	10.323	98	696941	23.298	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	93.200%		
43) trans-1,3-Dichloroprop...	10.579	79	86776	20.290	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	81.160%		
47) 2-Hexanone-d5	10.927	63	63592	37.976	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	75.960%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	145229	17.829	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	71.320%		
66) 1,2-Dichlorobenzene-d4	13.853	152	203160	22.736	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	90.960%		
Target Compounds						
25) Chloroform	7.683	83	10706	0.582	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060821\
Data File : VW019156.D
Acq On : 08 Jun 2021 14:04
Operator : SY/VA
Sample : M2649-06
Misc : 4.40G/10ML/MSVOA_W/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG5J1

Manual Integrations
APPROVED

MMDadoda
6/9/2021 4:17:12 PM

Quant Time: Jun 09 01:05:53 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 09 01:04:22 2021
Response via : Initial Calibration

