

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060821\
 Data File : VW019158.D
 Acq On : 08 Jun 2021 14:52
 Operator : SY/VA
 Sample : M2649-08
 Misc : 4.31G/10ML/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG5J3

Manual Integrations
 APPROVED

MMDadoda
 6/9/2021 4:17:17 PM

Quant Time: Jun 09 01:06:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 09 01:04:22 2021
 Response via : Initial Calibration

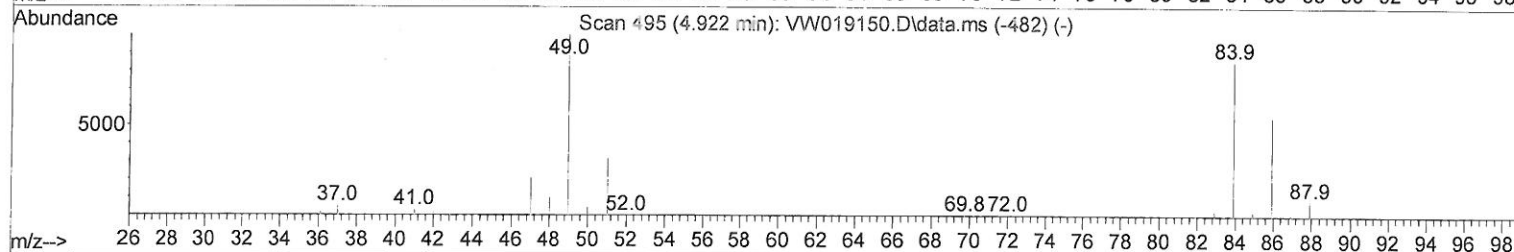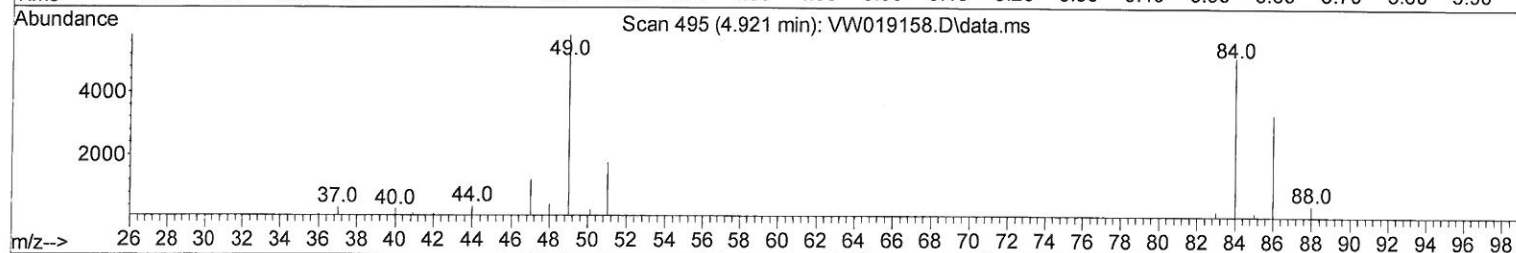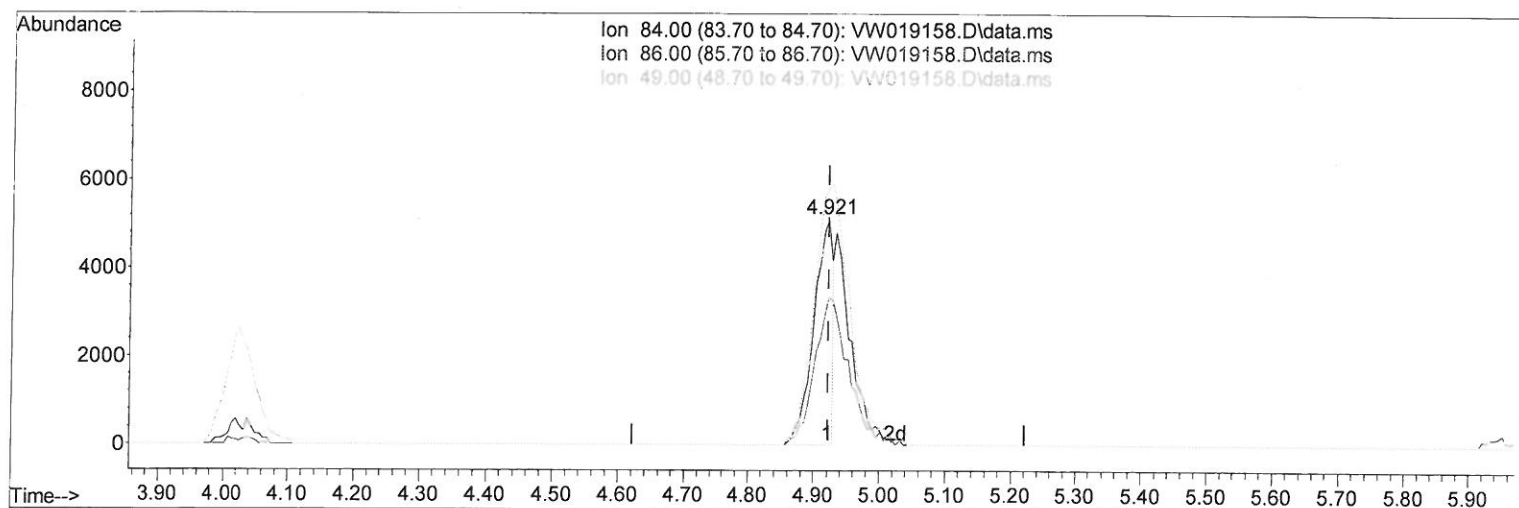

TIC: VW019158.D\data.ms

(16) Methylene chloride (T)

4.921min (-0.000) 0.97 ug/L

response 10244

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	64.82
49.00	123.70	113.16
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060821\
 Data File : VW019158.D
 Acq On : 08 Jun 2021 14:52
 Operator : SY/VA
 Sample : M2649-08
 Misc : 4.31G/10ML/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG5J3

Manual Integrations
 APPROVED

MMDadoda
 6/9/2021 4:17:17 PM

Quant Time: Jun 09 01:06:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 09 01:04:22 2021
 Response via : Initial Calibration

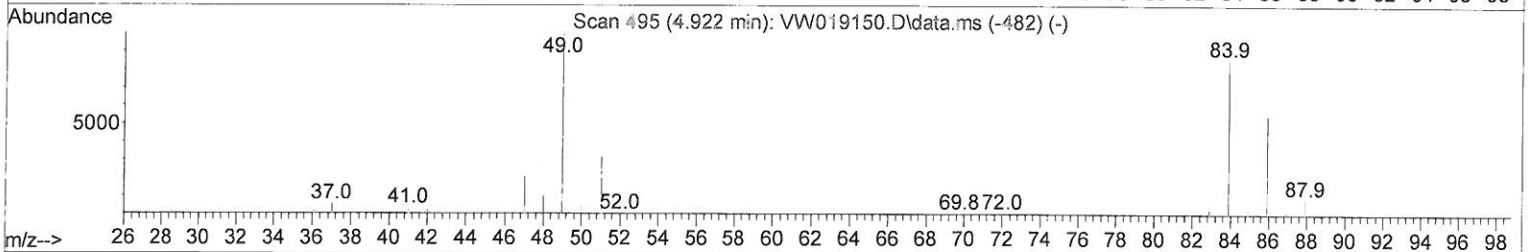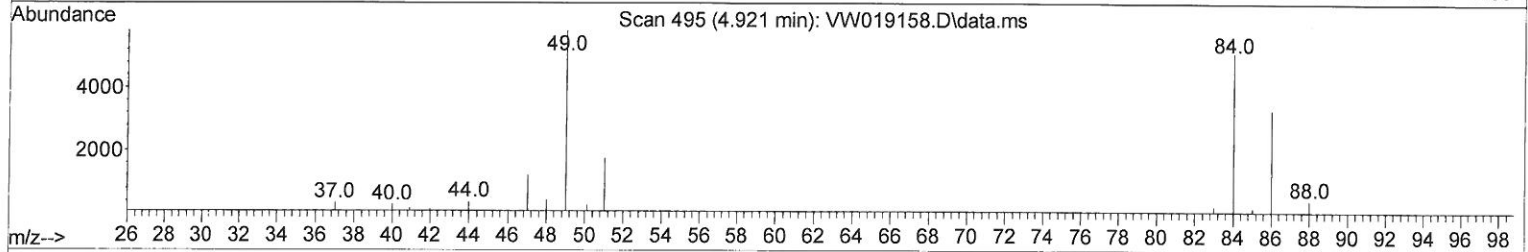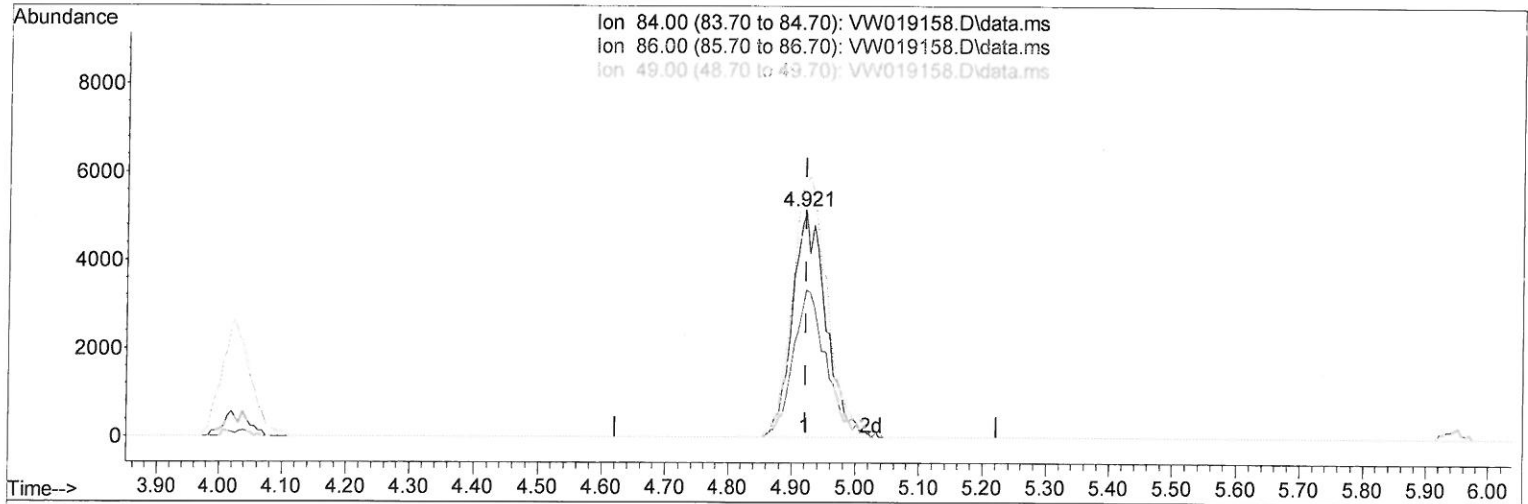

TIC: VW019158.D\data.ms

(16) Methylene chloride (T)

4.921min (-0.000) 1.77 ug/L m

response 18748

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	64.82
49.00	123.70	113.16
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060821\
 Data File : VW019158.D
 Acq On : 08 Jun 2021 14:52
 Operator : SY/VA
 Sample : M2649-08
 Misc : 4.31G/10ML/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG5J3

Manual Integrations
 APPROVED

MMDadoda
 6/9/2021 4:17:17 PM

Quant Time: Jun 09 01:06:14 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 09 01:04:22 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	570649	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	450182	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	149631	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	211927	28.085	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 112.360%			
7) Chloroethane-d5	2.891	69	171048	26.615	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 106.440%			
11) 1,1-Dichloroethene-d2	4.025	63	290216	19.358	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 77.440%			
21) 2-Butanone-d5	7.080	46	77095	39.004	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 78.000%			
24) Chloroform-d	7.653	84	414215	26.999	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 108.000%			
26) 1,2-Dichloroethane-d4	8.305	65	210668	24.480	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 97.920%			
32) Benzene-d6	8.275	84	798740	31.142	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 124.560%			
36) 1,2-Dichloropropane-d6	9.274	67	250113	32.166	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 128.680%#			
41) Toluene-d8	10.323	98	679166	28.833	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 115.320%			
43) trans-1,3-Dichloroprop...	10.579	79	84727	25.159	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 100.640%			
47) 2-Hexanone-d5	10.927	63	62592	47.470	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 94.940%			
56) 1,1,2,2-Tetrachloroeth...	12.694	84	159238	24.826	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 99.320%			
66) 1,2-Dichlorobenzene-d4	13.859	152	141377	27.070	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 108.280%			
Target Compounds						
16) Methylene chloride	4.921	84	18748m	1.771	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060821\
Data File : VW019158.D
Acq On : 08 Jun 2021 14:52
Operator : SY/VA
Sample : M2649-08
Misc : 4.31G/10ML/MSVOA_W/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG5J3

Manual Integrations
APPROVED

MMDadoda
6/9/2021 4:17:17 PM

Quant Time: Jun 09 01:06:14 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 09 01:04:22 2021
Response via : Initial Calibration

