

Quantitation Report (Qedit)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060921\
Data File : VW019166.D
Acq On : 09 Jun 2021 14:17
Operator : SY/VA
Sample : M2682-01
Misc : 3.74G/10ML/MSVOA_W/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDB0

Manual Integrations
APPROVED

MMDadoda
6/10/2021 5:24:38 PM




Quant Time: Jun 10 01:15:20 2021

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M

Quant Title : SFAM01.0

QLast Update : Thu Jun 10 01:14:29 2021

Response via : Initial Calibration

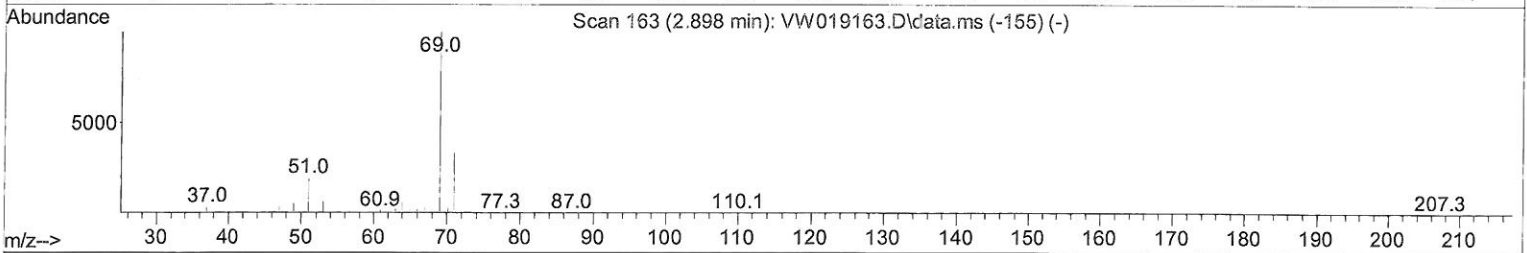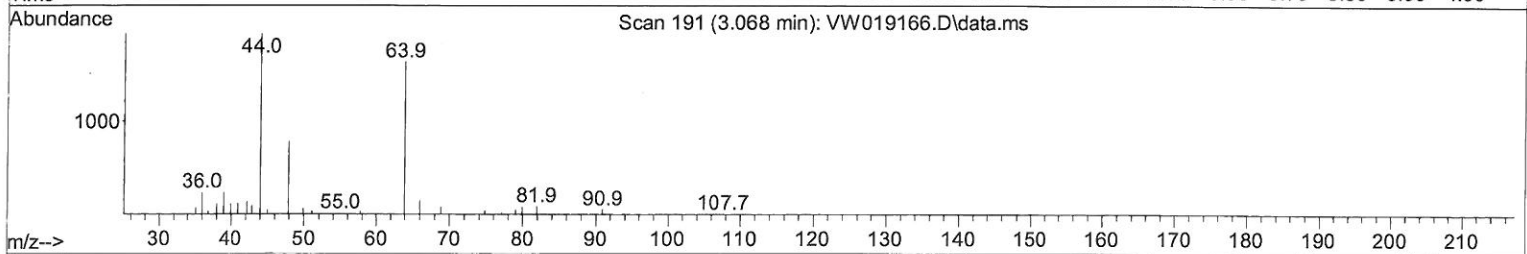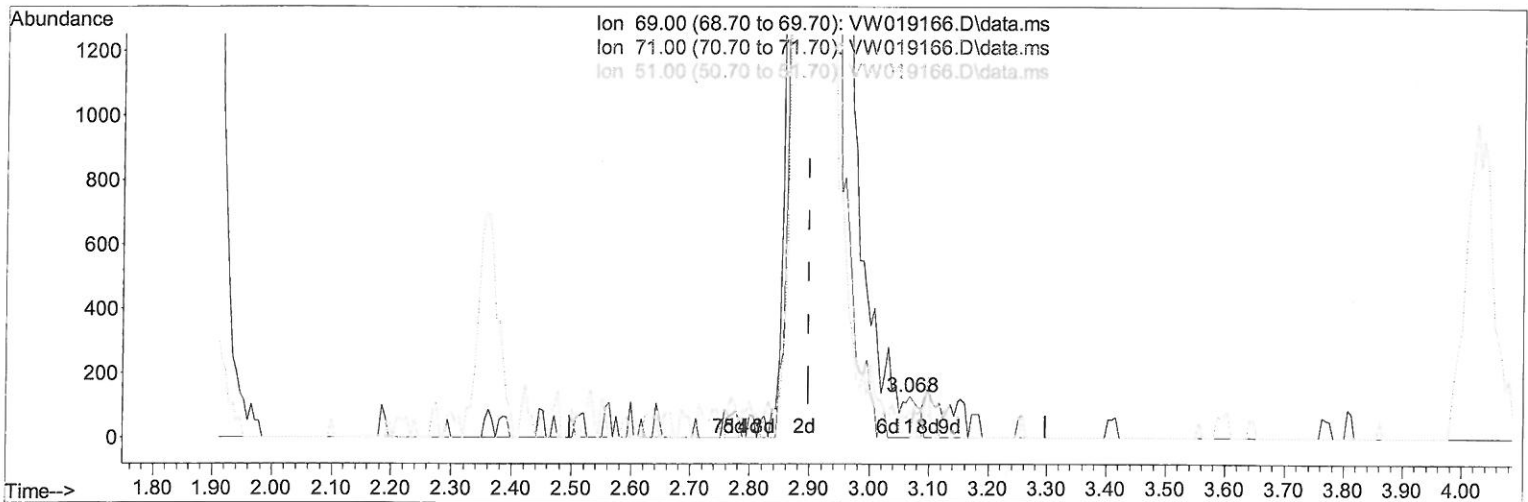

TIC: VW019166.D\data.ms

(7) Chloroethane-d5 (S)

3.068min (+ 0.171) 0.04 ug/L

response 238

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	38.24
51.00	28.40	28.57
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060921\
Data File : VW019166.D
Acq On : 09 Jun 2021 14:17
Operator : SY/VA
Sample : M2682-01
Misc : 3.74G/10ML/MSVOA_W/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDB0

Manual Integrations
APPROVED

MMDadoda
6/10/2021 5:24:38 PM

Quant Time: Jun 10 01:15:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 10 01:14:29 2021
Response via : Initial Calibration

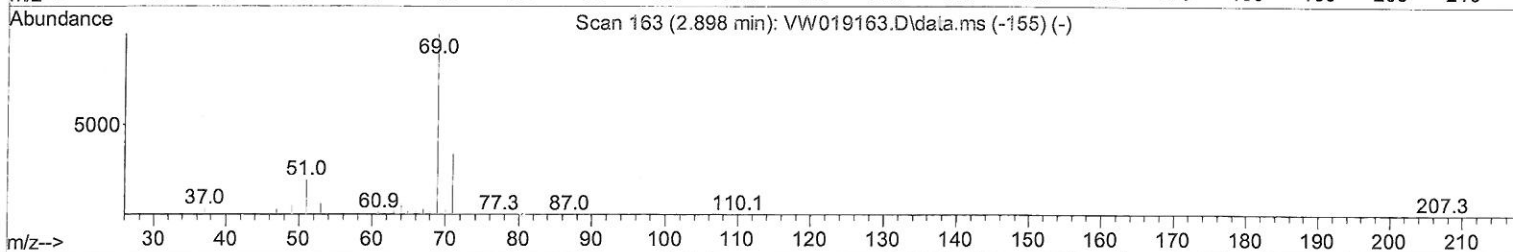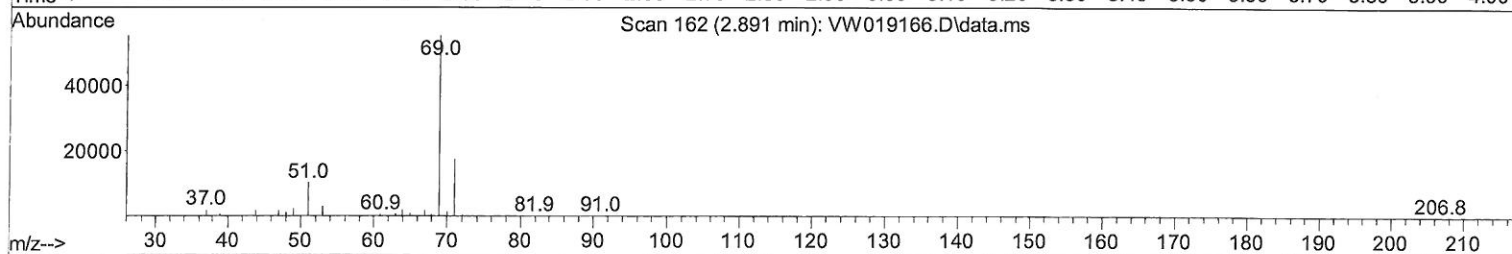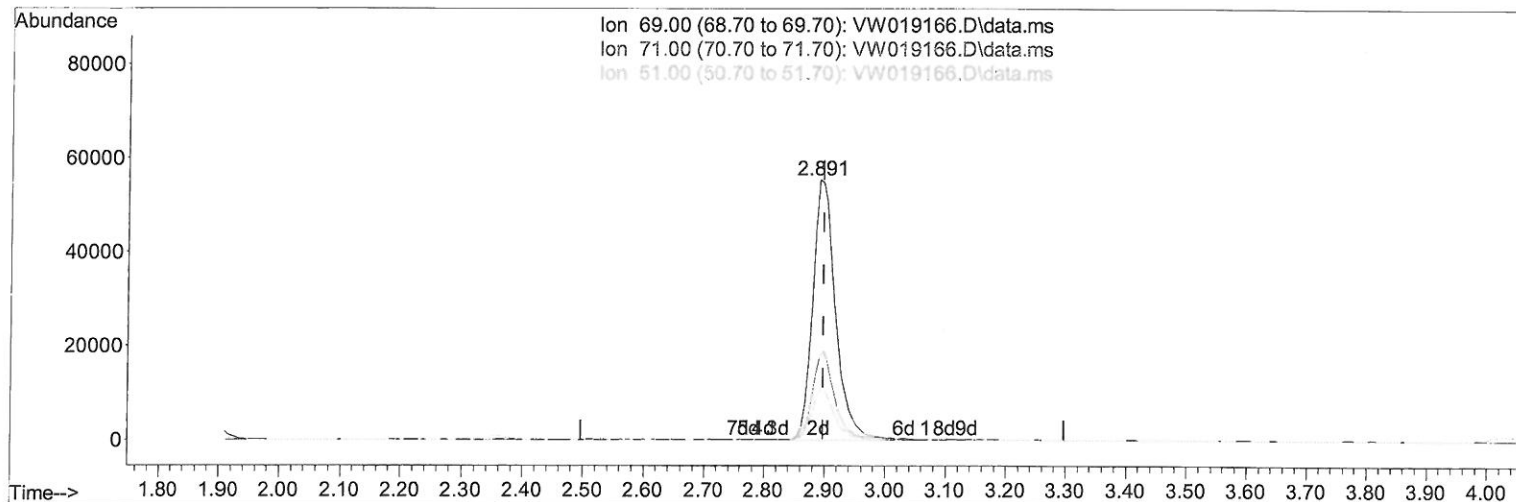

TIC: VW019166.D\data.ms

(7) Chloroethane-d5 (S)

2.891min (-0.006) 24.79 ug/L m

response 144557

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	0.06#
51.00	28.40	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060921\
 Data File : VW019166.D
 Acq On : 09 Jun 2021 14:17
 Operator : SY/VA
 Sample : M2682-01
 Misc : 3.74G/10ML/MSVOA_W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDB0

Manual Integrations
 APPROVED

MMDadoda
 6/10/2021 5:24:38 PM

Quant Time: Jun 10 01:15:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 10 01:14:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	517686	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	422236	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	142595	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	173202	25.301	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 101.200%			
7) Chloroethane-d5	2.891	69	144557m	24.794	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 99.160%			
11) 1,1-Dichloroethene-d2	4.025	63	247121	18.169	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 72.680%			
21) 2-Butanone-d5	7.086	46	58359	32.546	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 65.100%			
24) Chloroform-d	7.653	84	333659	23.973	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 95.880%			
26) 1,2-Dichloroethane-d4	8.311	65	169185	21.671	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 86.680%			
32) Benzene-d6	8.275	84	682990	28.391	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 113.560%			
36) 1,2-Dichloropropane-d6	9.274	67	198669	27.241	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 108.960%			
41) Toluene-d8	10.329	98	589370	26.677	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 106.720%			
43) trans-1,3-Dichloroprop...	10.579	79	67578	21.395	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 85.600%			
47) 2-Hexanone-d5	10.927	63	48056	38.858	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 77.720%			
56) 1,1,2,2-Tetrachloroeth...	12.695	84	117675	19.560	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 78.240%			
66) 1,2-Dichlorobenzene-d4	13.853	152	122868	24.687	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 98.760%			
Target Compounds						
13) Acetone	4.135	43	38964	24.522	ug/L	84
16) Methylene chloride	4.922	84	14950	1.556	ug/L	96
22) 2-Butanone	7.177	43	9199	4.330	ug/L	98
42) Toluene	10.390	91	11178	0.374	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

06/11/21 sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060921\
Data File : VW019166.D
Acq On : 09 Jun 2021 14:17
Operator : SY/VA
Sample : M2682-01
Misc : 3.74G/10ML/MSVOA_W/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDB0

Manual Integrations
APPROVED

MMDadoda
6/10/2021 5:24:38 PM

Quant Time: Jun 10 01:15:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 10 01:14:29 2021
Response via : Initial Calibration

