

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060921\
 Data File : VW019167.D
 Acq On : 09 Jun 2021 14:41
 Operator : SY/VA
 Sample : M2662-02
 Misc : 5.29G/10ML/MSVOA_W/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDB1

Manual Integrations
 APPROVED

MMDadoda
 6/10/2021 5:24:40 PM

Quant Time: Jun 10 01:15:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 10 01:14:29 2021
 Response via : Initial Calibration

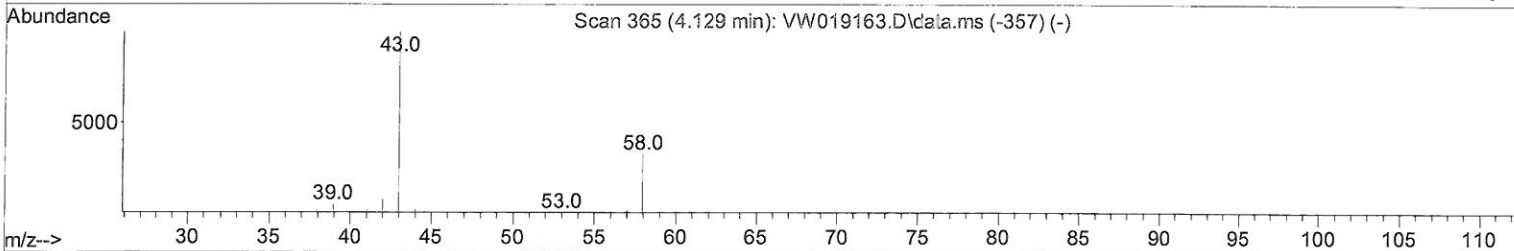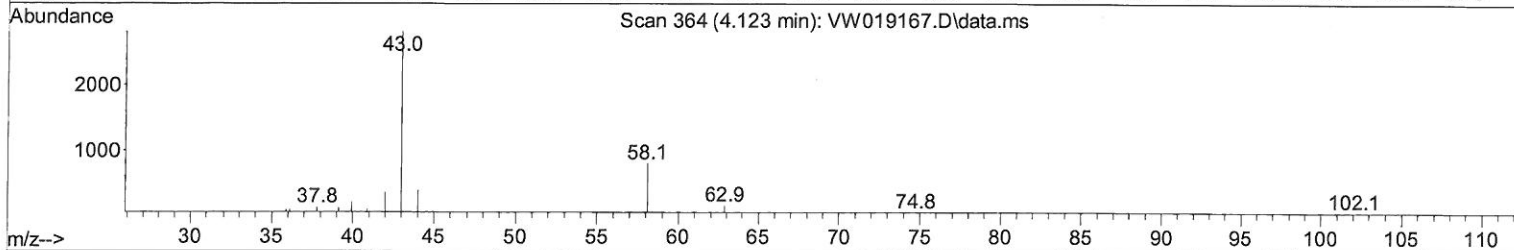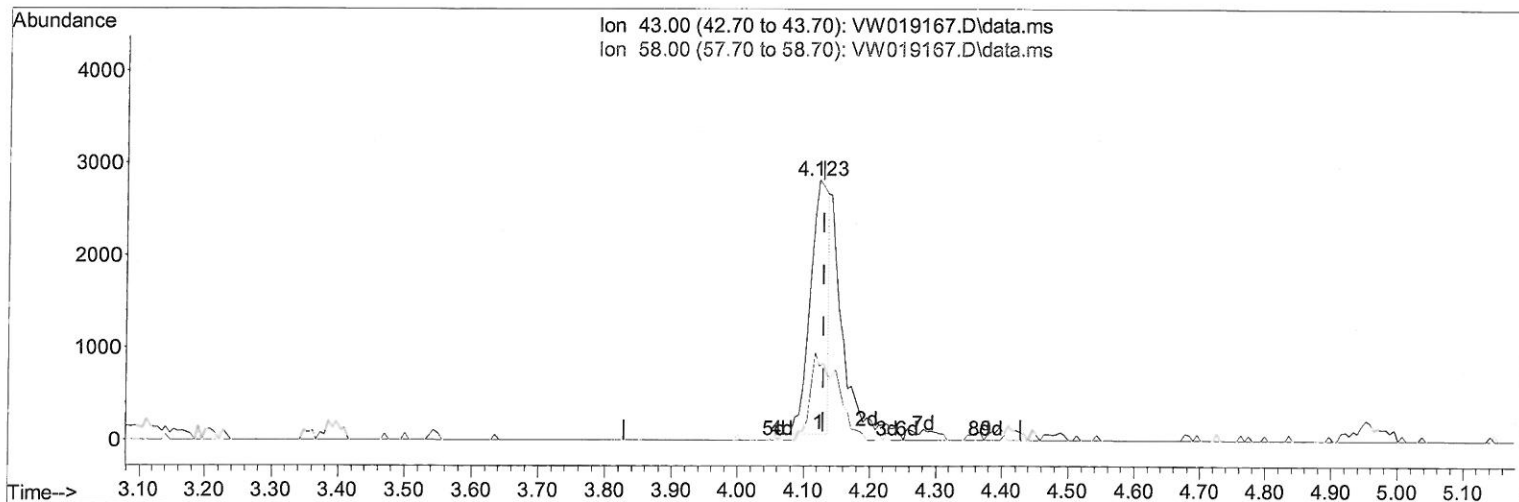

TIC: VW019167.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 5.51 ug/L

response 5197

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	34.73
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060921\
 Data File : VW019167.D
 Acq On : 09 Jun 2021 14:41
 Operator : SY/VA
 Sample : M2662-02
 Misc : 5.29G/10ML/MSVOA_W/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDB1

Manual Integrations
 APPROVED

MMDadoda
 6/10/2021 5:24:40 PM

Quant Time: Jun 10 01:15:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 10 01:14:29 2021
 Response via : Initial Calibration

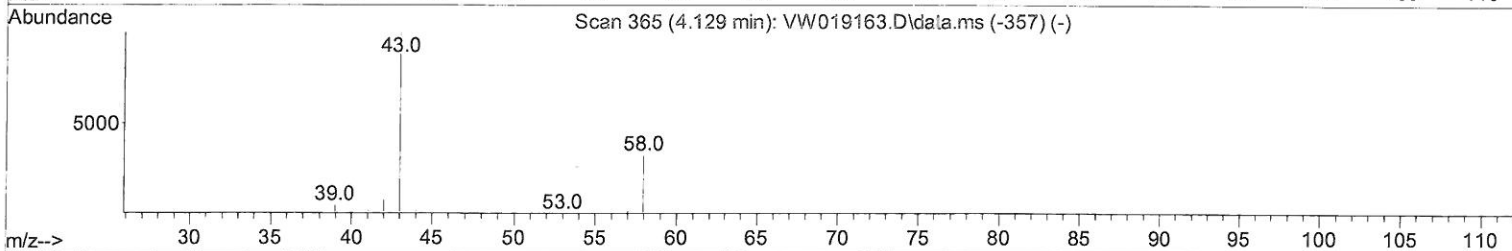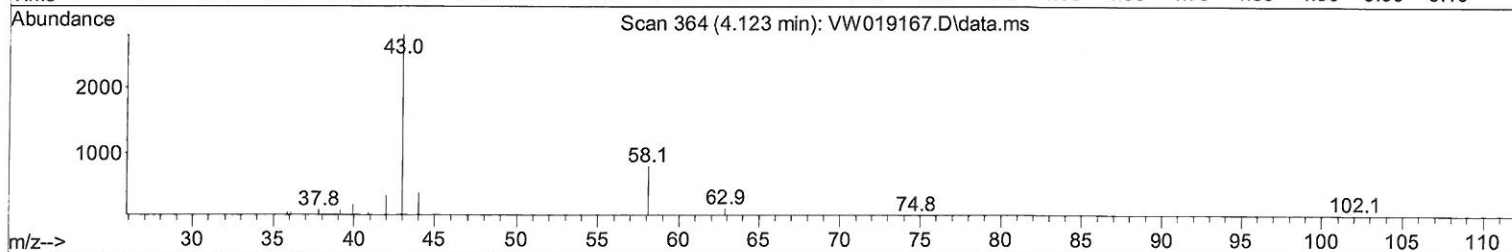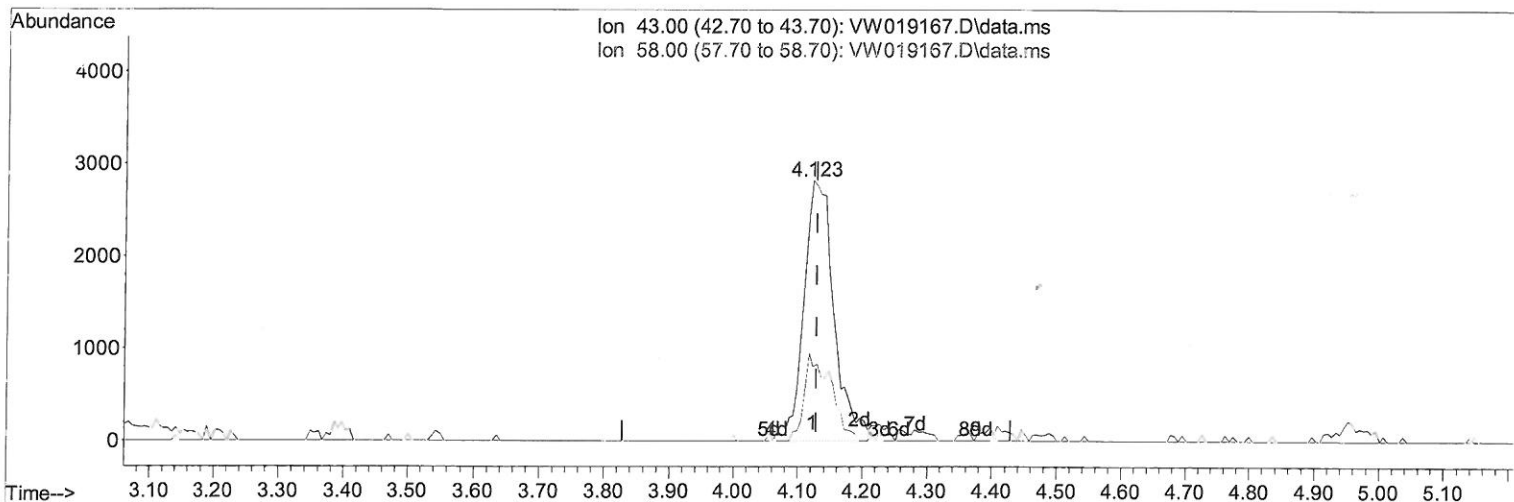

TIC: VW019167.D\data.ms

(13) Acetone (T)

4.123min (-0.006) 9.58 ug/L m

response 9038

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	19.97
0.00	0.00	0.00
0.00	0.00	0.00

70611121 57

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060921\
 Data File : VW019167.D
 Acq On : 09 Jun 2021 14:41
 Operator : SY/VA
 Sample : M2662-02
 Misc : 5.29G/10ML/MSVOA_W/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDB1

Manual Integrations
 APPROVED

MMDadoda
 6/10/2021 5:24:40 PM

Quant Time: Jun 10 01:15:30 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 10 01:14:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	307515	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	281944	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	124646	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	107830	26.518	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 106.080%			
7) Chloroethane-d5	2.891	69	90554	26.146	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 104.600%			
11) 1,1-Dichloroethene-d2	4.019	63	156908	19.421	ug/L	-0.01
Spiked Amount 25.000	Range 45 - 110		Recovery = 77.680%			
21) 2-Butanone-d5	7.086	46	43610	40.942	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 81.880%			
24) Chloroform-d	7.653	84	217611	26.321	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 105.280%			
26) 1,2-Dichloroethane-d4	8.311	65	116674	25.159	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 100.640%			
32) Benzene-d6	8.275	84	432517	26.926	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 107.720%			
36) 1,2-Dichloropropane-d6	9.281	67	129980	26.691	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 106.760%			
41) Toluene-d8	10.323	98	385468	26.129	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 104.520%			
43) trans-1,3-Dichloroprop...	10.579	79	49807	23.615	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 94.480%			
47) 2-Hexanone-d5	10.927	63	35338	42.793	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 85.580%			
56) 1,1,2,2-Tetrachloroeth...	12.695	84	92250	22.964	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 91.840%			
66) 1,2-Dichlorobenzene-d4	13.853	152	114827	26.393	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 105.560%			
Target Compounds						
13) Acetone	4.123	43	9038m	9.576	ug/L	Qvalue 6/11/21 84
16) Methylene chloride	4.922	84	10252	1.797	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060921\
Data File : VW019167.D
Acq On : 09 Jun 2021 14:41
Operator : SY/VA
Sample : M2662-02
Misc : 5.29G/10ML/MSVOA_W/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDB1

Manual Integrations
APPROVED

MMDadoda
6/10/2021 5:24:40 PM

Quant Time: Jun 10 01:15:30 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 10 01:14:29 2021
Response via : Initial Calibration

