

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060921\
 Data File : VW019164.D
 Acq On : 09 Jun 2021 13:29
 Operator : SY/VA
 Sample : VW0609SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK103

Quant Time: Jun 10 01:15:01 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 10 01:14:29 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	502986	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	468416	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	221021	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	152041	22.859	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	91.440%		
7) Chloroethane-d5	2.898	69	133346	23.539	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	94.160%		
11) 1,1-Dichloroethene-d2	4.032	63	219811	16.634	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	66.520%		
21) 2-Butanone-d5	7.086	46	91461	52.497	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	105.000%		
24) Chloroform-d	7.653	84	345671	25.562	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	102.240%		
26) 1,2-Dichloroethane-d4	8.305	65	191314	25.222	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	100.880%		
32) Benzene-d6	8.281	84	682849	25.587	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	102.360%		
36) 1,2-Dichloropropane-d6	9.274	67	211912	26.192	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	104.760%		
41) Toluene-d8	10.329	98	618656	25.242	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	100.960%		
43) trans-1,3-Dichloroprop...	10.579	79	84168	24.020	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	96.080%		
47) 2-Hexanone-d5	10.927	63	73856	53.832	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	107.660%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	173474	25.993	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	103.960%		
66) 1,2-Dichlorobenzene-d4	13.853	152	203374	26.363	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	105.440%		
Target Compounds					Qvalue	
42) Toluene	10.390	91	12409	0.374	ug/L	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW060921\
Data File : VW019164.D
Acq On : 09 Jun 2021 13:29
Operator : SY/VA
Sample : VW0609SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK103

Quant Time: Jun 10 01:15:01 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 10 01:14:29 2021
Response via : Initial Calibration

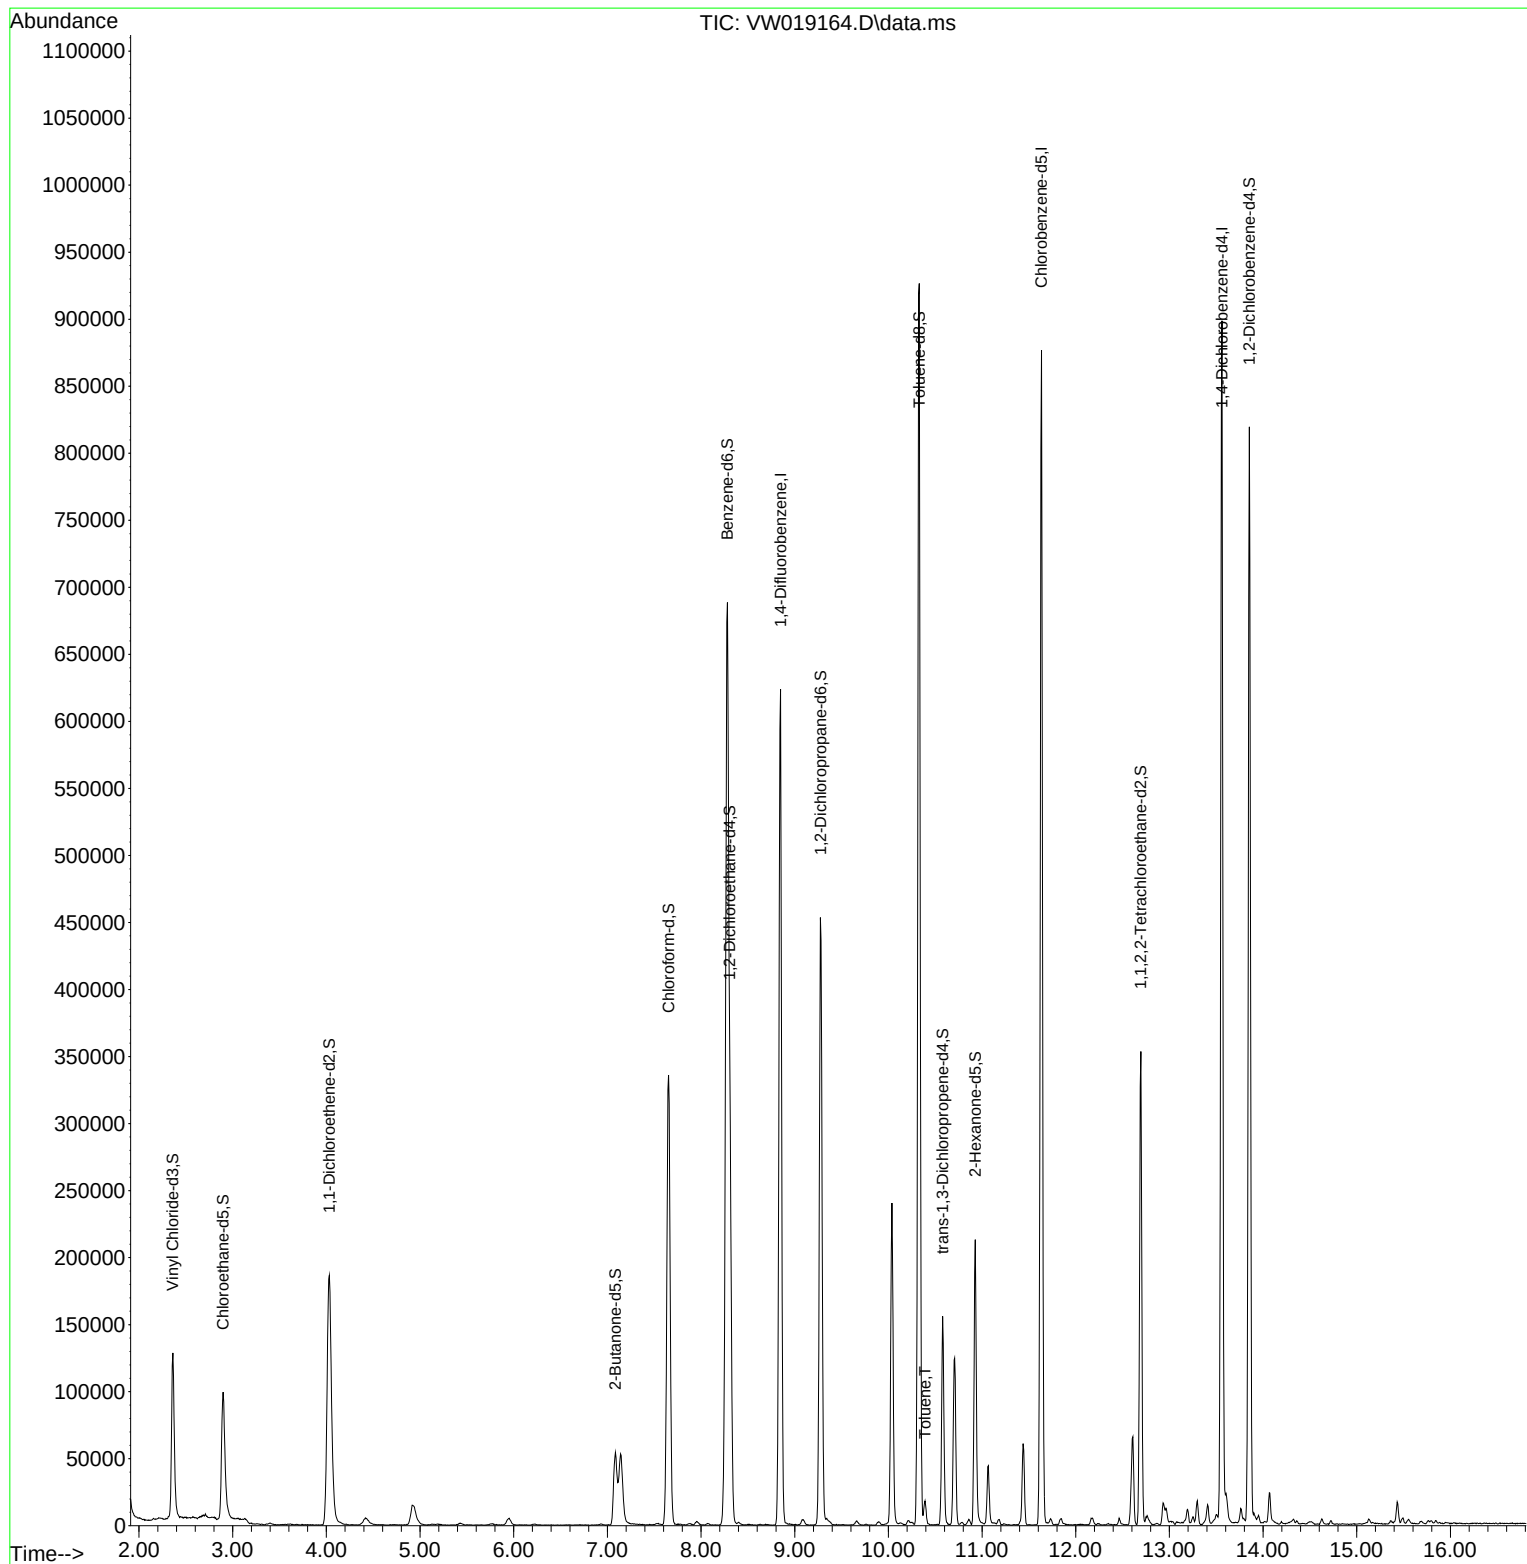

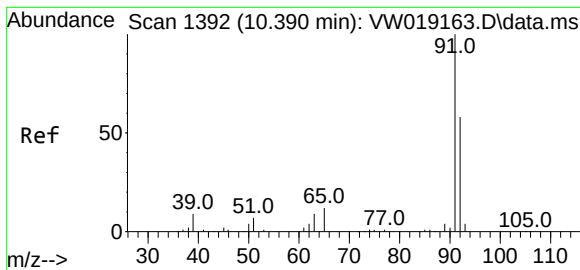

#42

Toluene

Concen: 0.374 ug/L

RT: 10.390 min Scan# 1392

Delta R.T. 0.000 min

Lab File: VW019164.D

Acq: 09 Jun 2021 13:29

Tgt Ion: 91 Resp: 12409

Ion Ratio Lower Upper

91 100

92 54.1 39.5 73.3

Instrument :

MSVOA_W

ClientSampleId :

VBLK103

