

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061021\
 Data File : VW019177.D
 Acq On : 10 Jun 2021 12:02
 Operator : SY/VA
 Sample : M2682-03
 Misc : 6.38G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDH2

Manual Integrations
 APPROVED

MMDadoda
 6/14/2021 4:26:02 PM

Quant Time: Jun 11 02:28:49 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 11 01:12:34 2021
 Response via : Initial Calibration

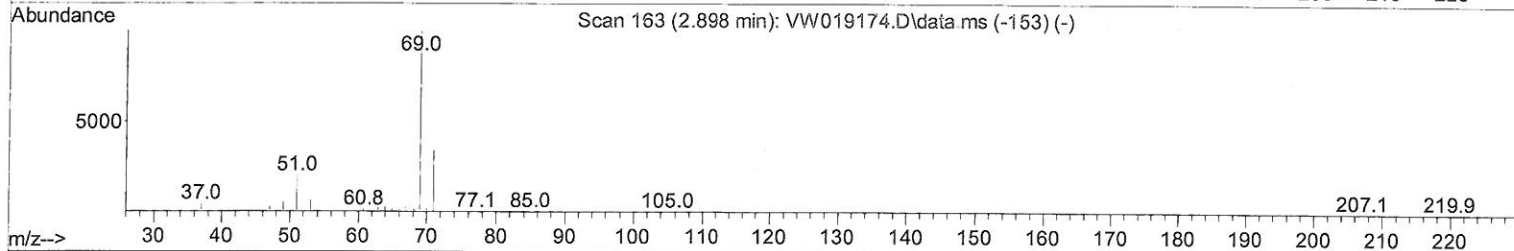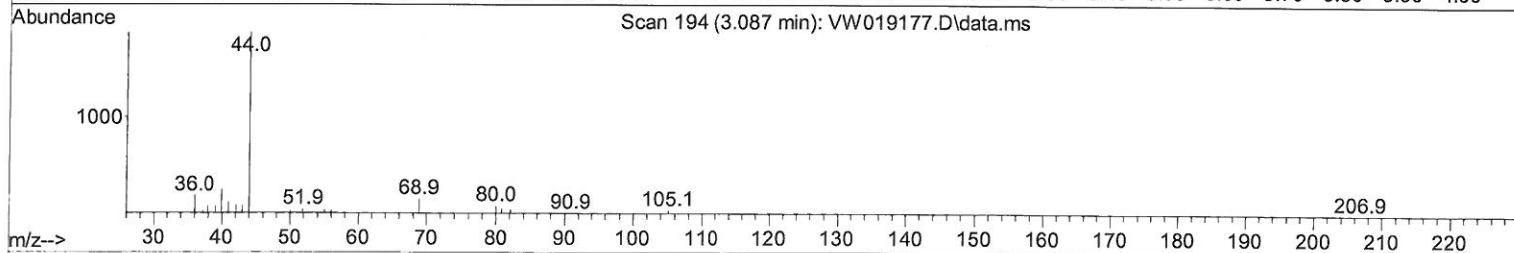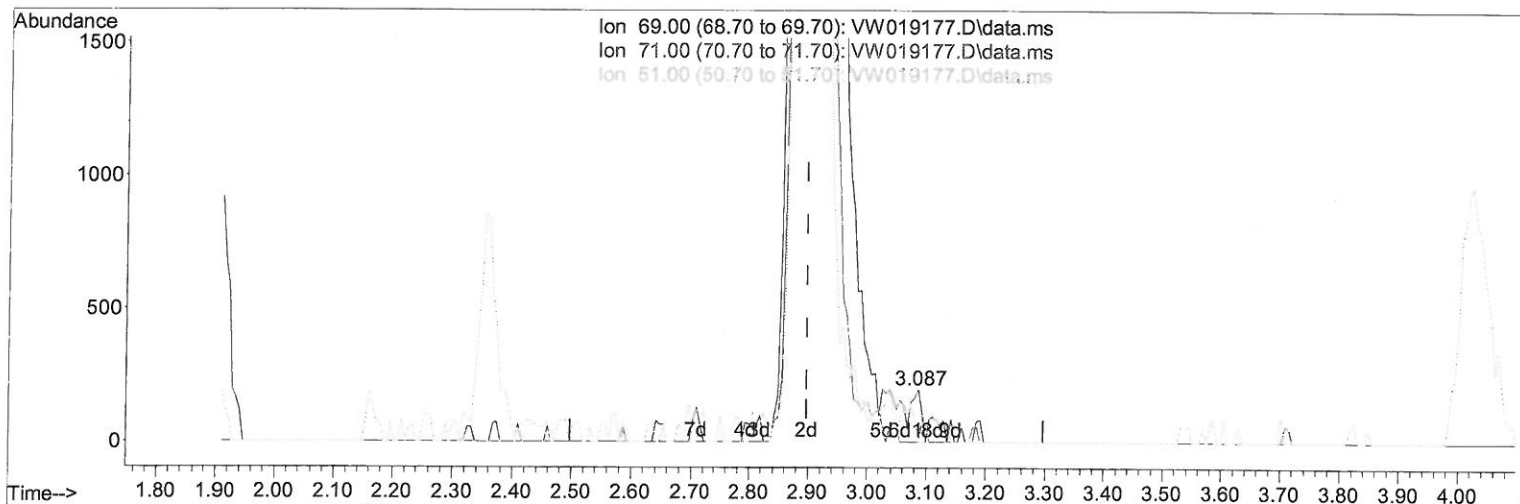

TIC: VW019177.D\data.ms

(7) Chloroethane-d5 (S)

3.087min (+ 0.189) 0.03 ug/L

response 225

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	22.67
51.00	28.40	30.22
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061021\
 Data File : VW019177.D
 Acq On : 10 Jun 2021 12:02
 Operator : SY/VA
 Sample : M2682-03
 Misc : 6.38G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDH2

Manual Integrations
 APPROVED

MMDadoda
 6/14/2021 4:26:02 PM

Quant Time: Jun 11 01:17:34 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 11 01:12:34 2021
 Response via : Initial Calibration

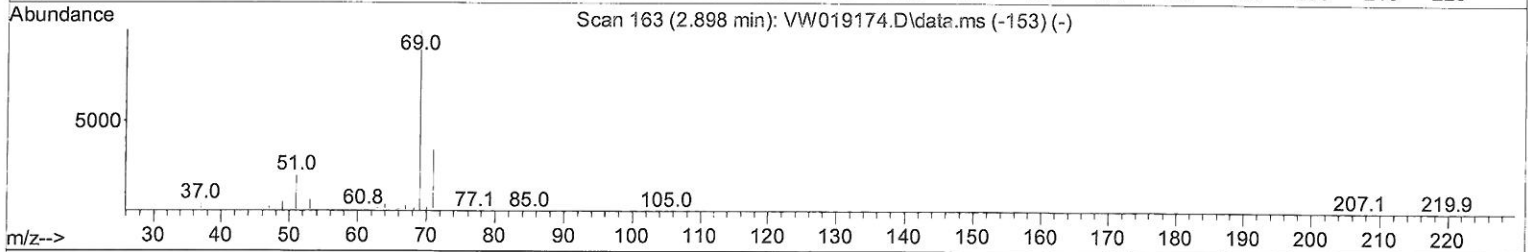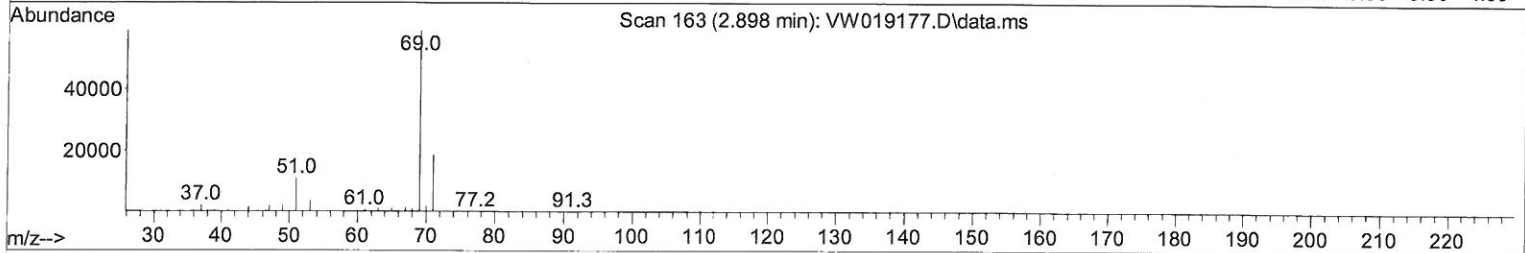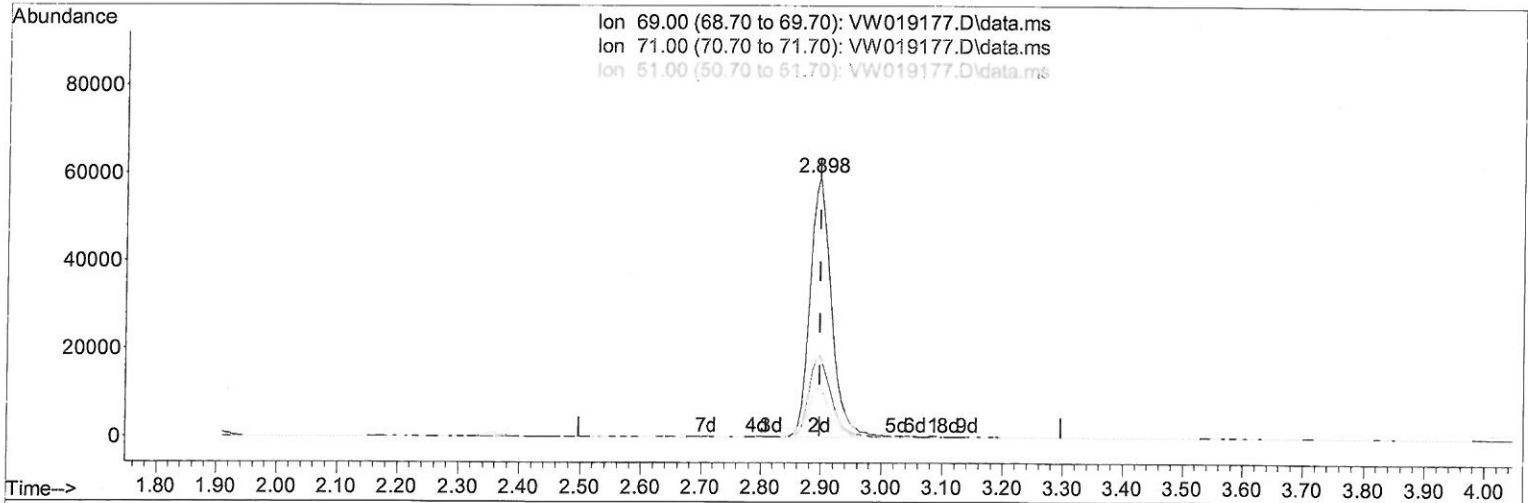

TIC: VW019177.D\data.ms

(7) Chloroethane-d5 (S)

2.898min (+ 0.000) 21.00 ug/L m

response 146485

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	0.03#
51.00	28.40	0.05#
0.00	0.00	0.00

706/15/21 SY

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061021\
 Data File : VW019177.D
 Acq On : 10 Jun 2021 12:02
 Operator : SY/VA
 Sample : M2682-03
 Misc : 6.38G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDH2

Manual Integrations
 APPROVED

MMDadoda
 6/14/2021 4:26:02 PM

Quant Time: Jun 11 01:17:34 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 11 01:12:34 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	619219	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	535904	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	214690	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	182326	22.267	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	89.080%		
7) Chloroethane-d5	2.898	69	146485m	21.005	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	84.000%		
11) 1,1-Dichloroethene-d2	4.025	63	259031	15.922	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	63.680%		
21) 2-Butanone-d5	7.086	46	67803	31.612	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	63.220%		
24) Chloroform-d	7.653	84	365090	21.930	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	87.720%		
26) 1,2-Dichloroethane-d4	8.311	65	190383	20.388	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	81.560%		
32) Benzene-d6	8.275	84	740024	24.237	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	96.960%		
36) 1,2-Dichloropropane-d6	9.274	67	220673	23.840	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	95.360%		
41) Toluene-d8	10.329	98	652290	23.262	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	93.040%		
43) trans-1,3-Dichloroprop...	10.579	79	84089	20.976	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	83.920%		
47) 2-Hexanone-d5	10.927	63	56875	36.235	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	72.460%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	142450	18.656	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	74.640%		
66) 1,2-Dichlorobenzene-d4	13.853	152	167532	22.357	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	89.440%		
Target Compounds						
13) Acetone	4.141	43	61027	32.110	ug/L	88
16) Methylene chloride	4.922	84	17755	1.545	ug/L	97
22) 2-Butanone	7.183	43	16357	6.437	ug/L	91

(#) = qualifier out of range (m) = manual integration (+) = signals summed

06/15/21 SY

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061021\
Data File : VW019177.D
Acq On : 10 Jun 2021 12:02
Operator : SY/VA
Sample : M2682-03
Misc : 6.38G/10ML/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDH2

Manual Integrations
APPROVED

MMDadoda
6/14/2021 4:26:02 PM

Quant Time: Jun 11 01:17:34 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 11 01:12:34 2021
Response via : Initial Calibration

