


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061025\
Data File : VW031710.D
Acq On : 10 Jun 2025 07:37
Operator : SY/MD
Sample : BFB435
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB435

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061025SMA.M
Title : SFAM01.0
Last Update : Wed Jun 25 07:47:11 2025

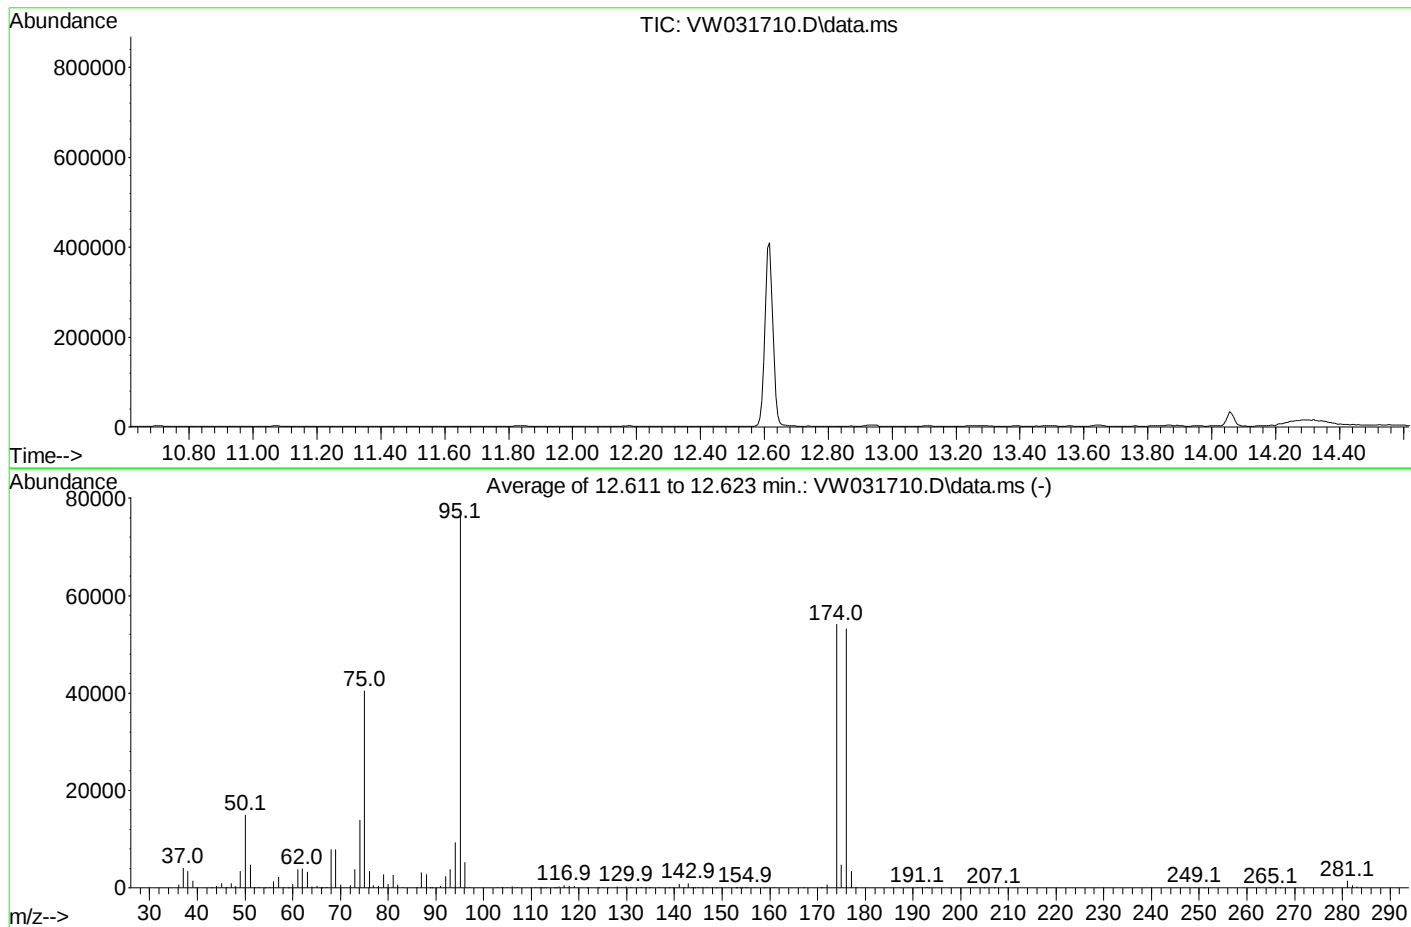

AutoFind: Scans 1759, 1760, 1761; Background Corrected with Scan 1751

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.6	14950	PASS
75	95	30	80	53.0	40499	PASS
95	95	100	100	100.0	76376	PASS
96	95	5	9	6.9	5268	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.9	54155	PASS
175	174	5	9	8.7	4728	PASS
176	174	95	101	98.3	53211	PASS
177	176	5	9	6.3	3378	PASS