


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW061120\
 Data File : VW015578.D
 Acq On : 11 Jun 2020 08:35
 Operator : SY/VA
 Sample : BFB08
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB08

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM052620S.M
 Title : VOC Analysis
 Last Update : Fri Jun 12 05:02:36 2020

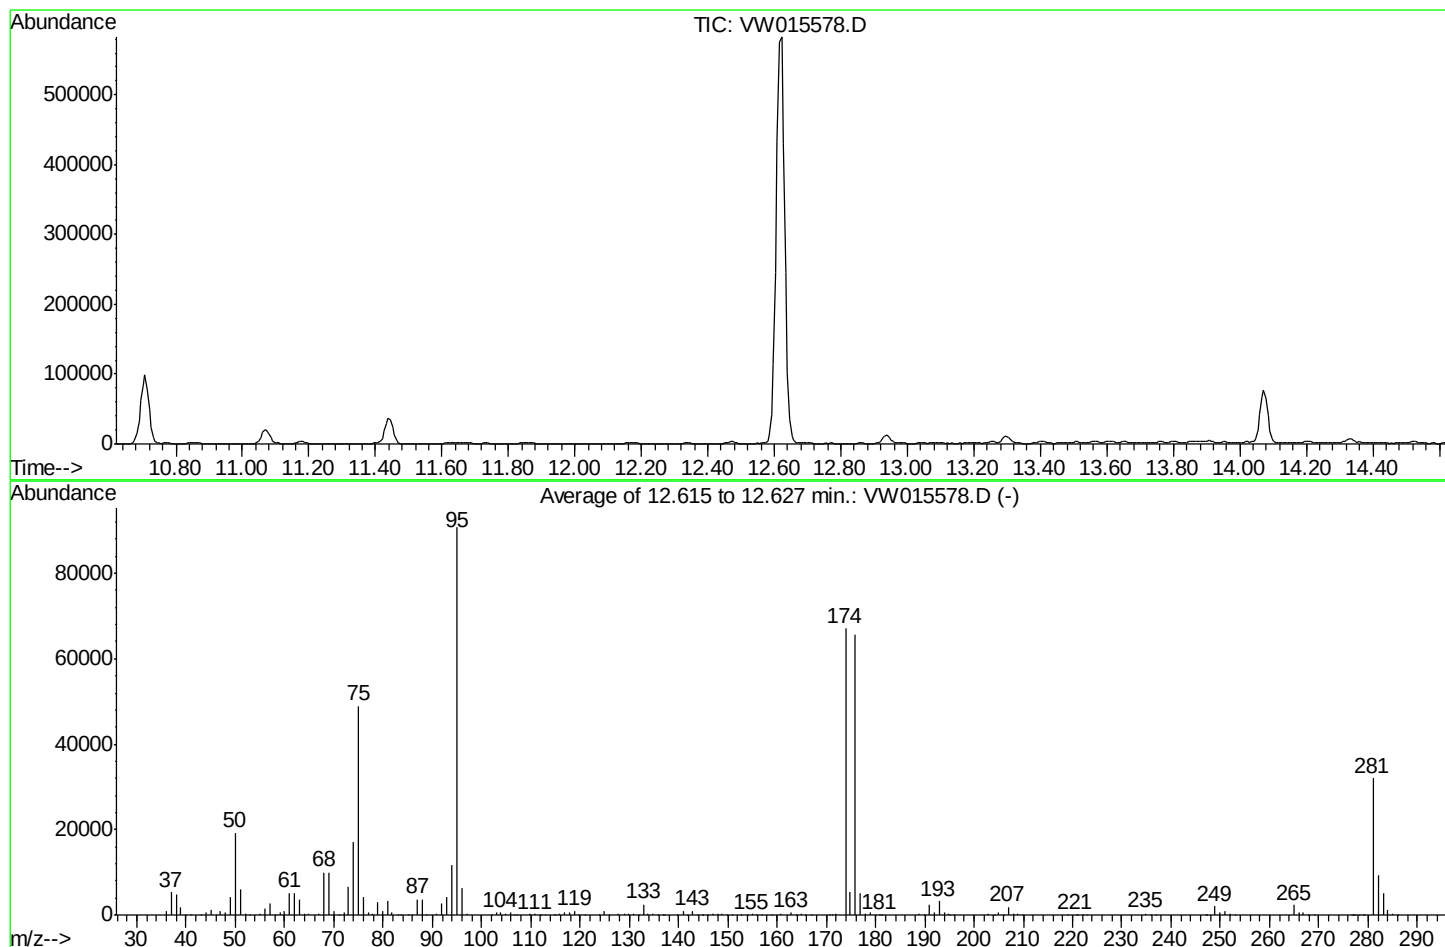

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	19255	PASS
75	95	30	80	54.0	48976	PASS
95	95	100	100	100.0	90770	PASS
96	95	5	9	6.8	6163	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.9	67120	PASS
175	174	5	9	8.2	5531	PASS
176	174	95	101	97.9	65730	PASS
177	176	5	9	8.0	5230	PASS

m/z	Abundance
36.00	1059.0
37.00	5903.0
38.00	4928.0
39.00	1850.0
39.80	200.0
40.90	135.0
42.90	252.0
43.90	1044.0
45.00	1759.0
46.00	204.0
47.00	1288.0
47.90	740.0
49.00	4610.0
50.00	20368.0
51.00	6368.0
52.00	351.0
55.00	319.0
56.00	1628.0
57.00	2956.0
58.10	176.0
59.00	823.0
60.00	1117.0
61.00	5504.0
62.00	5313.0
63.00	3894.0
64.00	416.0
65.00	289.0
67.00	398.0
68.00	10752.0
69.00	10576.0
69.90	889.0
70.90	123.0
72.00	574.0
73.00	8771.0
74.00	17968.0
75.00	51696.0
76.00	4815.0
76.90	632.0
77.90	416.0
78.90	3300.0
79.90	904.0
80.90	3382.0
81.90	739.0
83.00	118.0
83.70	81.0
85.10	93.0
87.00	3949.0
87.90	3603.0
88.80	302.0
90.90	385.0
92.00	2723.0
93.00	3824.0
94.00	11844.0
95.00	93280.0
96.00	6552.0
96.90	360.0
102.10	84.0
103.00	840.0
103.90	698.0
104.80	310.0
105.90	473.0
106.70	144.0
110.00	252.0
110.80	302.0
111.80	185.0
112.80	167.0
114.80	379.0
115.80	358.0
116.90	822.0
117.90	778.0
118.90	1193.0
119.80	111.0
120.90	166.0
124.90	1355.0
127.90	437.0
128.90	177.0
129.90	324.0
130.90	244.0
131.80	141.0
133.00	4208.0
134.90	536.0
135.90	65.0
136.70	117.0
137.10	135.0
140.90	796.0
142.90	916.0
143.80	75.0
144.80	194.0
146.00	152.0
146.90	562.0
147.80	279.0
148.80	285.0

Instrument :
MSVOA_W
ClientSampleId :
BFB08

149.80	113.0
150.80	62.0
152.80	95.0
154.00	73.0
154.90	200.0
157.00	154.0
158.90	119.0
160.90	397.0
162.00	54.0
162.90	782.0
164.00	116.0
165.00	509.0
165.80	73.0
166.90	83.0
172.00	400.0
173.90	62080.0
174.90	5357.0
175.90	60480.0
176.90	5475.0
177.90	441.0
178.90	1198.0
179.90	139.0
180.70	127.0
181.20	72.0
189.00	426.0
191.00	3636.0
192.00	759.0
192.90	4808.0
194.00	925.0
194.80	495.0
195.90	74.0
203.00	462.0
204.10	136.0
204.90	1033.0
206.10	228.0
206.90	2984.0
208.00	604.0
209.00	441.0
209.90	71.0
219.00	155.0
220.80	152.0
221.90	75.0
223.00	67.0
234.90	491.0
235.90	143.0
236.80	93.0
246.90	103.0
248.90	2969.0
250.00	812.0
250.90	1435.0
251.90	362.0
253.00	123.0
265.00	3450.0
266.00	844.0
266.90	681.0
267.90	193.0
269.00	119.0
277.00	78.0
277.30	77.0
281.00	47920.0
282.00	14379.0
283.10	7703.0
283.90	1639.0
284.90	573.0
285.90	82.0

Instrument :
MSVOA_W
ClientSampleId :
BFB08

m/z	Abundance
36.00	1168.0
37.00	5877.0
38.00	5285.0
39.00	2208.0
39.90	190.0
41.10	99.0
43.00	187.0
44.00	915.0
45.00	1254.0
46.00	118.0
46.90	961.0
48.00	739.0
49.00	4820.0
50.00	21800.0
51.00	6613.0
52.00	267.0
53.00	74.0
55.10	361.0
55.90	1702.0
57.00	3010.0
57.90	146.0
59.00	510.0
59.90	1132.0
61.00	5785.0
62.00	5335.0
63.00	4199.0
64.00	360.0
64.90	263.0
67.00	262.0
68.00	11160.0
69.00	10949.0
70.00	944.0
71.00	105.0
72.00	691.0
73.00	6812.0
74.00	19360.0
75.00	54496.0
76.00	4721.0
77.00	609.0
77.90	445.0
78.90	3429.0
79.90	1101.0
80.90	3851.0
81.90	829.0
82.90	141.0
83.60	120.0
86.00	134.0
86.90	4250.0
87.90	4057.0
88.90	135.0
91.00	480.0
91.90	3293.0
93.00	4797.0
94.00	12896.0
95.00	99360.0
96.00	6859.0
97.00	248.0
103.00	507.0
103.80	573.0
104.90	234.0
105.90	536.0
106.70	122.0
109.90	189.0
110.90	305.0
112.00	188.0
112.90	107.0
115.00	220.0
115.90	449.0
116.90	889.0
117.80	722.0
118.90	932.0
119.80	77.0
120.80	110.0
123.90	80.0
125.00	732.0
125.80	200.0
127.70	271.0
127.90	274.0
128.90	229.0
129.80	330.0
130.80	244.0
131.90	83.0
132.90	2267.0
133.80	644.0
134.80	414.0
135.80	70.0
137.00	173.0
139.60	58.0
140.90	892.0
141.80	136.0
142.90	993.0
143.80	90.0

Instrument :
MSVOA_W
ClientSampleId :
BFB08

144.80	214.0
145.80	215.0
146.90	314.0
147.90	281.0
148.90	218.0
149.90	120.0
152.80	58.0
154.90	233.0
156.80	167.0
158.90	199.0
160.80	362.0
162.80	445.0
163.90	95.0
164.90	241.0
167.00	55.0
170.60	53.0
172.00	415.0
173.90	76464.0
174.90	6174.0
175.90	74304.0
176.90	5822.0
177.90	229.0
178.90	520.0
180.00	65.0
180.90	97.0
188.80	280.0
189.90	148.0
190.90	2276.0
191.90	514.0
192.90	3571.0
194.00	579.0
195.00	362.0
195.90	66.0
202.90	203.0
204.10	73.0
204.90	584.0
207.00	1955.0
208.00	327.0
208.90	257.0
218.80	81.0
220.60	107.0
221.00	117.0
222.00	53.0
222.90	57.0
234.90	316.0
235.90	78.0
236.90	87.0
246.90	90.0
248.90	2032.0
249.90	520.0
251.00	831.0
251.90	164.0
253.00	123.0
265.00	2264.0
266.00	699.0
266.90	564.0
267.90	110.0
269.10	104.0
276.70	54.0
277.60	61.0
278.30	106.0
279.00	161.0
281.00	33168.0
282.00	9514.0
283.00	5086.0
284.00	1155.0
285.00	388.0

Instrument :
MSVOA_W
ClientSampleId :
BFB08

m/z	Abundance
35.90	885.0
37.00	4153.0
38.00	3950.0
39.00	1630.0
39.90	195.0
40.80	81.0
41.10	65.0
43.00	151.0
43.90	664.0
45.00	813.0
46.00	93.0
46.90	756.0
48.00	640.0
49.00	3566.0
50.00	15597.0
51.00	5133.0
52.00	159.0
55.00	268.0
56.00	1372.0
57.00	2632.0
58.00	130.0
58.90	147.0
59.90	831.0
61.00	4088.0
62.00	4296.0
63.00	3068.0
63.90	319.0
65.00	209.0
66.90	255.0
68.00	8215.0
69.00	8339.0
69.90	576.0
71.10	83.0
72.00	450.0
73.00	4539.0
74.00	14207.0
75.00	40736.0
76.00	3314.0
77.00	521.0
77.80	317.0
78.90	2638.0
79.90	722.0
80.90	2836.0
81.80	645.0
82.90	121.0
85.90	108.0
86.90	2902.0
87.90	3181.0
90.90	324.0
92.00	2309.0
93.00	3731.0
94.00	10335.0
95.00	79672.0
96.00	5078.0
96.90	165.0
103.00	212.0
103.80	522.0
104.90	185.0
105.90	455.0
107.10	73.0
109.80	126.0
110.90	121.0
112.10	123.0
113.00	77.0
114.90	138.0
115.90	283.0
116.90	501.0
117.90	427.0
118.80	640.0
123.90	88.0
124.80	269.0
125.80	150.0
127.90	307.0
128.90	174.0
129.80	404.0
130.80	111.0
131.90	65.0
132.90	1037.0
133.70	323.0
134.90	274.0
135.70	54.0
136.90	162.0
140.90	852.0
141.90	105.0
142.80	983.0
143.80	68.0
145.00	114.0
145.90	108.0
146.80	224.0
148.00	203.0
148.80	142.0
149.90	78.0

Instrument :
MSVOA_W
ClientSampleId :
BFB08

152.80	88.0
154.90	234.0
155.70	53.0
156.90	124.0
159.00	97.0
160.90	183.0
163.00	231.0
164.80	140.0
170.60	53.0
171.10	60.0
172.00	343.0
173.90	62816.0
174.90	5064.0
175.90	62408.0
176.90	4393.0
177.90	250.0
178.90	244.0
179.90	58.0
188.90	131.0
190.90	897.0
191.80	197.0
193.00	1416.0
194.00	233.0
194.80	175.0
202.90	122.0
204.10	59.0
204.90	288.0
205.90	56.0
207.00	809.0
208.10	145.0
209.10	127.0
220.80	55.0
234.80	133.0
247.20	55.0
249.00	1040.0
249.80	240.0
250.90	405.0
251.80	149.0
252.90	69.0
264.90	1203.0
265.90	279.0
267.00	332.0
267.90	87.0
277.50	56.0
279.20	103.0
281.00	14767.0
282.00	4402.0
283.00	2655.0
283.90	474.0
285.00	175.0

Instrument :
MSVOA_W
ClientSampleId :
BFB08

Scan 1750 (12.573 min): VW015578.D
BFB08

m/z	Abundance
35.90	77.0
38.80	57.0
39.90	156.0
41.10	90.0
43.10	83.0
44.00	353.0
56.90	74.0
73.10	80.0
207.00	51.0
280.70	77.0

Instrument :
MSVOA_W
ClientSampleId :
BFB08