

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061121\
 Data File : VW019199.D
 Acq On : 11 Jun 2021 15:53
 Operator : SY/VA
 Sample : M2680-05
 Misc : 6.05G/10ML/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDD1

Manual Integrations
 APPROVED

MMDadoda
 6/14/2021 4:26:41 PM

Quant Time: Jun 12 00:24:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 12 00:22:09 2021
 Response via : Initial Calibration

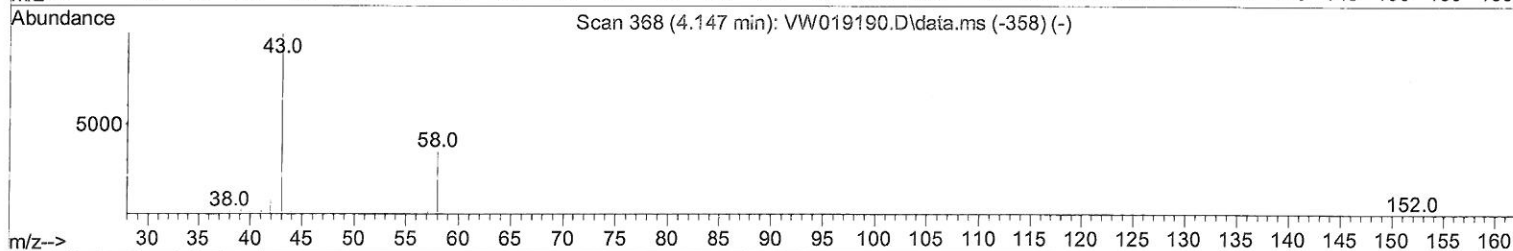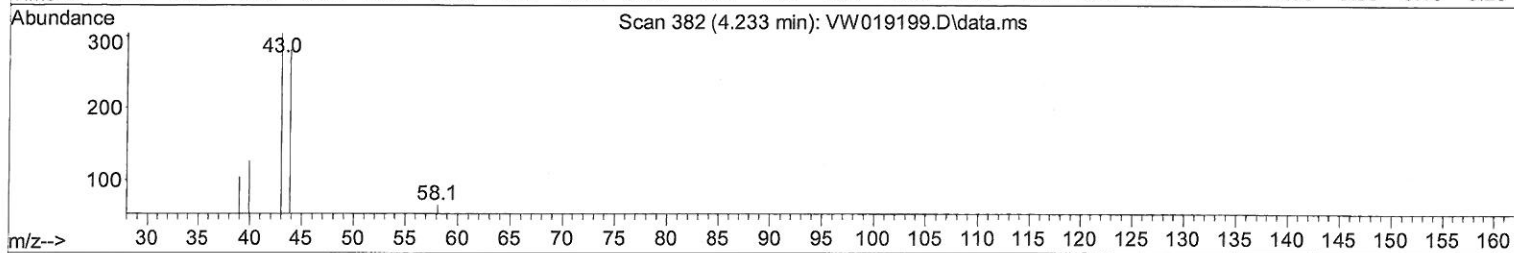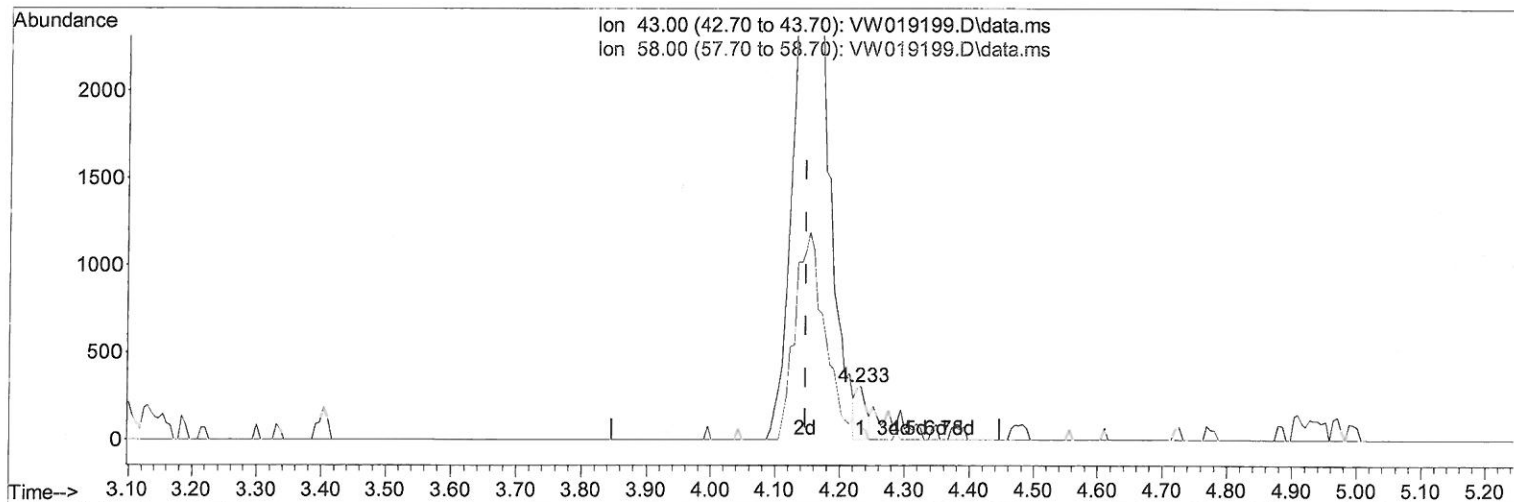

TIC: VW019199.D\data.ms

(13) Acetone (T)

4.233min (+ 0.086) 0.21 ug/L

response 338

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	6.80
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061121\
Data File : VW019199.D
Acq On : 11 Jun 2021 15:53
Operator : SY/VA
Sample : M2680-05
Misc : 6.05G/10ML/MSVOA_W/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDD1

Manual Integrations
APPROVED

MMDadoda
6/14/2021 4:26:41 PM

Quant Time: Jun 12 00:24:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 12 00:22:09 2021
Response via : Initial Calibration

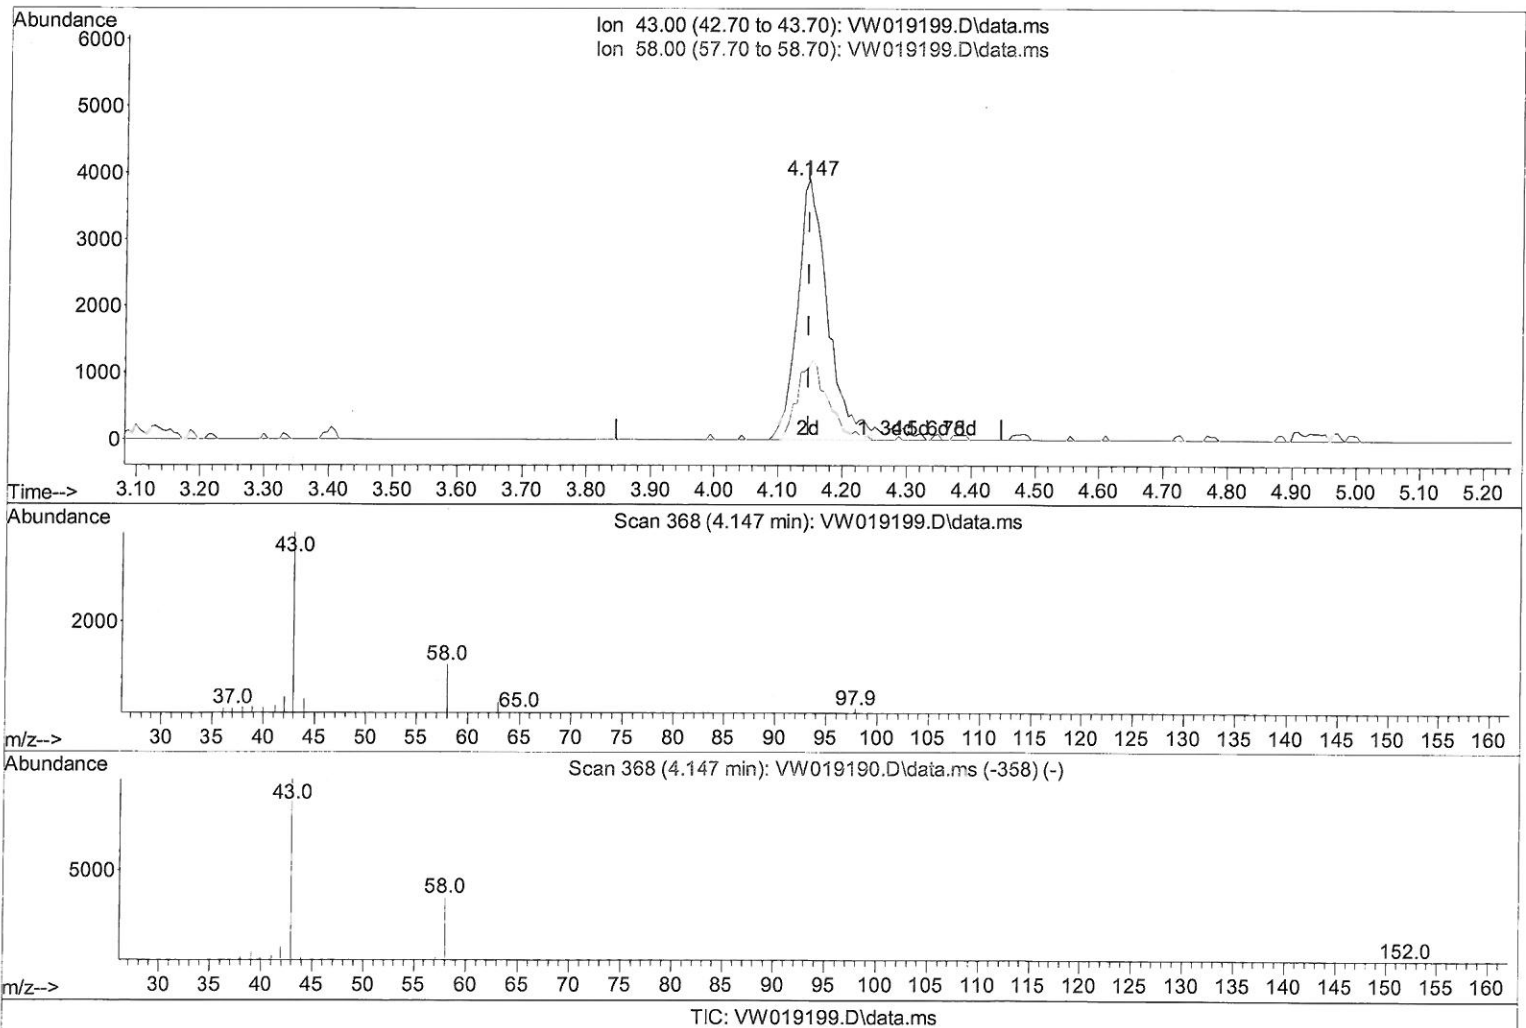

(13) Acetone (T)

4.147min (+ 0.000) 7.89 ug/L m

response 12675

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	0.18
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061121\
 Data File : VW019199.D
 Acq On : 11 Jun 2021 15:53
 Operator : SY/VA
 Sample : M2680-05
 Misc : 6.05G/10ML/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BGDD1

Manual Integrations
 APPROVED

MMDadoda
 6/14/2021 4:26:41 PM

Quant Time: Jun 12 00:24:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 12 00:22:09 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc Units	Dev(Min)
Internal Standards					
1) 1,4-Difluorobenzene	8.848	114	523419	25.000 ug/L	0.00
28) Chlorobenzene-d5	11.634	117	469245	25.000 ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	184719	25.000 ug/L	0.00
System Monitoring Compounds					
4) Vinyl Chloride-d3	2.355	65	170537	24.639 ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	98.560%	
7) Chloroethane-d5	2.898	69	141702	24.038 ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	96.160%	
11) 1,1-Dichloroethene-d2	4.025	63	240244	17.470 ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	69.880%	
21) 2-Butanone-d5	7.086	46	65596	36.181 ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	72.360%	
24) Chloroform-d	7.653	84	349254	24.819 ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	99.280%	
26) 1,2-Dichloroethane-d4	8.311	65	182776	23.155 ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	92.640%	
32) Benzene-d6	8.275	84	707289	26.456 ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	105.840%	
36) 1,2-Dichloropropane-d6	9.275	67	213839	26.384 ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	105.520%	
41) Toluene-d8	10.329	98	617948	25.168 ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	100.680%	
43) trans-1,3-Dichloroprop...	10.579	79	73874	21.045 ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	84.200%	
47) 2-Hexanone-d5	10.927	63	55750	40.563 ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	81.120%	
56) 1,1,2,2-Tetrachloroeth...	12.695	84	138184	20.668 ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	82.680%	
66) 1,2-Dichlorobenzene-d4	13.853	152	175023	27.146 ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	108.600%	
Target Compounds					
13) Acetone	4.147	43	12675m	7.890 ug/L	Qvalue 99
16) Methylene chloride	4.928	84	44014	4.532 ug/L	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061121\
Data File : VW019199.D
Acq On : 11 Jun 2021 15:53
Operator : SY/VA
Sample : M2680-05
Misc : 6.05G/10ML/MSVOA_W/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDD1

Manual Integrations
APPROVED

MMDadoda
6/14/2021 4:26:41 PM

Quant Time: Jun 12 00:24:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 12 00:22:09 2021
Response via : Initial Calibration

