


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW061220\
 Data File : VW015595.D
 Acq On : 12 Jun 2020 08:18
 Operator : SY/VA
 Sample : BFB09
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB09

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM052620S.M
 Title : VOC Analysis
 Last Update : Sat Jun 13 00:17:50 2020

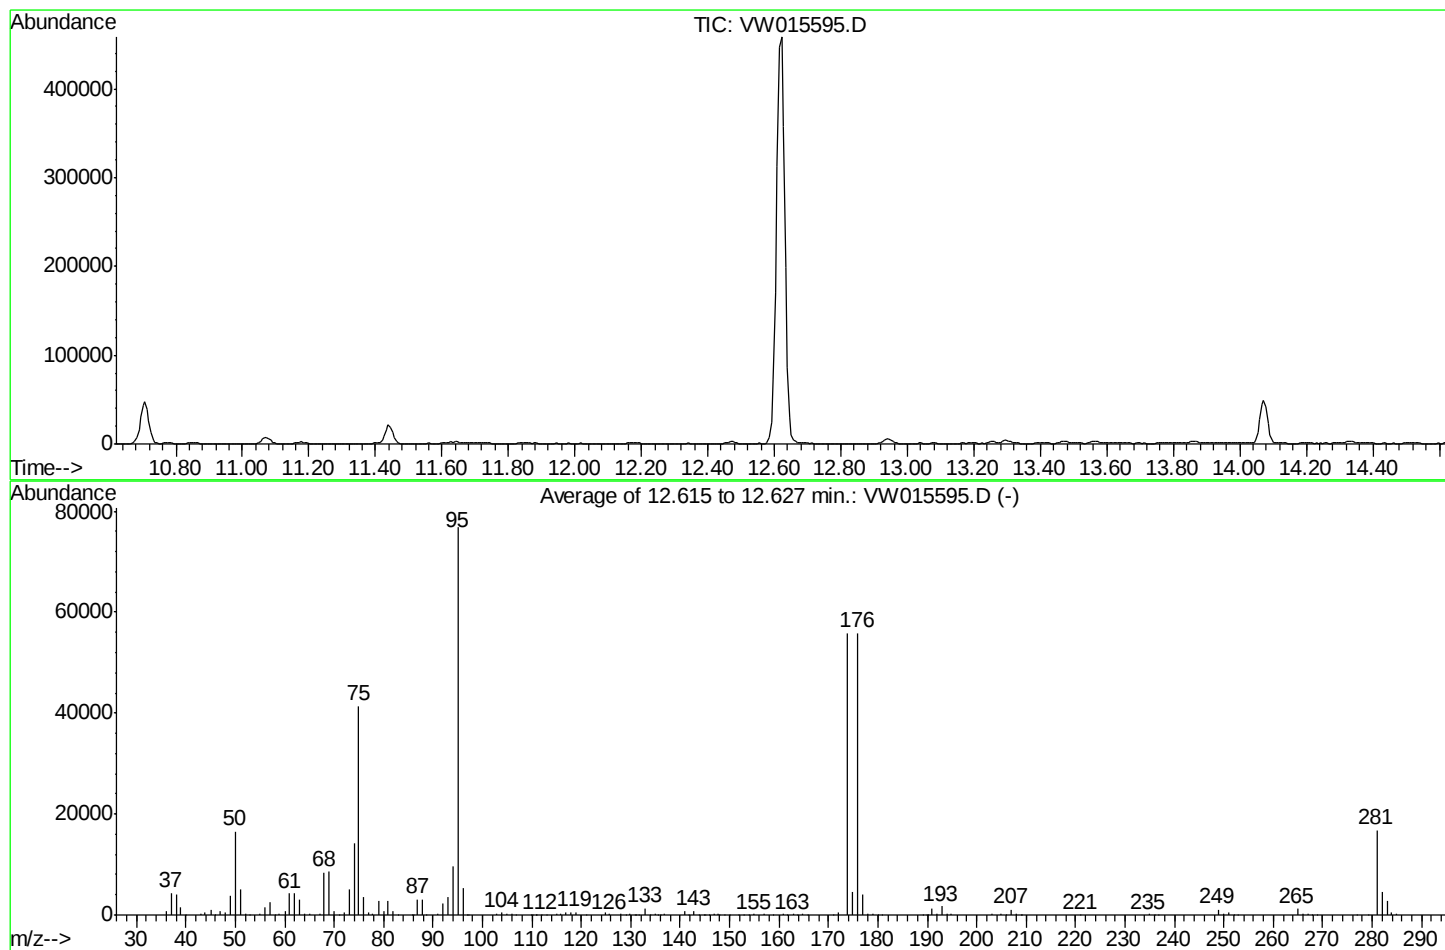

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	16548	PASS
75	95	30	80	53.9	41416	PASS
95	95	100	100	100.0	76826	PASS
96	95	5	9	6.9	5319	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.8	55896	PASS
175	174	5	9	8.4	4685	PASS
176	174	95	101	100.1	55941	PASS
177	176	5	9	7.2	4049	PASS

m/z	Abundance
36.00	848.0
37.00	4807.0
38.00	4234.0
39.00	1719.0
40.00	226.0
43.10	206.0
43.90	933.0
45.00	1223.0
46.00	111.0
46.90	878.0
48.00	562.0
49.00	4105.0
50.00	17712.0
51.00	5614.0
52.00	227.0
52.80	64.0
55.00	344.0
56.00	1496.0
57.00	2639.0
58.00	121.0
58.90	377.0
60.00	805.0
61.00	4530.0
62.00	4130.0
63.00	3363.0
64.00	428.0
65.00	199.0
67.00	251.0
68.00	9036.0
69.00	8564.0
70.00	874.0
72.10	550.0
73.00	5905.0
74.00	14876.0
75.00	43904.0
76.00	3931.0
77.00	526.0
77.70	306.0
78.90	2883.0
79.90	815.0
80.90	2853.0
81.90	684.0
83.00	89.0
85.70	97.0
86.90	3452.0
87.90	3200.0
91.00	361.0
92.00	2365.0
93.00	3440.0
94.00	9830.0
95.00	78360.0
96.00	5497.0
96.90	287.0
102.80	525.0
103.90	471.0
104.90	274.0
105.90	365.0
106.90	88.0
109.80	209.0
110.90	225.0
111.80	167.0
112.90	54.0
114.90	226.0
115.80	330.0
116.90	610.0
117.90	540.0
118.80	782.0
120.90	103.0
124.80	740.0
125.70	296.0
127.90	279.0
128.90	141.0
129.80	237.0
130.70	146.0
131.70	98.0
132.90	2103.0
134.90	363.0
135.60	53.0
136.90	148.0
140.90	703.0
141.80	135.0
142.90	817.0
143.70	63.0
144.80	116.0
145.80	103.0
146.80	371.0
147.80	298.0
148.90	165.0
149.90	79.0
152.70	51.0
154.90	167.0
156.80	143.0

Instrument :
MSVOA_W
ClientSampleId :
BFB09

158.80	70.0
161.00	308.0
161.70	68.0
162.90	404.0
163.70	74.0
164.90	289.0
165.80	70.0
170.80	63.0
171.90	455.0
173.90	51696.0
175.00	4402.0
175.90	53128.0
176.90	4288.0
177.80	211.0
179.00	573.0
179.90	55.0
180.90	89.0
189.00	222.0
189.80	61.0
190.90	1876.0
192.00	468.0
192.90	2774.0
193.90	548.0
194.90	287.0
202.90	256.0
204.90	458.0
205.90	142.0
207.00	1595.0
207.90	365.0
208.90	198.0
221.00	81.0
234.90	233.0
235.90	83.0
236.80	79.0
248.90	1453.0
250.00	397.0
250.80	696.0
252.00	142.0
252.80	79.0
265.00	1940.0
265.90	592.0
266.90	475.0
267.90	88.0
268.90	62.0
276.90	64.0
279.20	185.0
280.90	24480.0
282.10	6782.0
283.00	4225.0
283.90	866.0
285.00	260.0

Instrument :
MSVOA_W
ClientSampleId :
BFB09

m/z	Abundance
35.90	797.0
37.00	4834.0
38.00	4438.0
39.00	1673.0
39.90	209.0
42.90	167.0
43.90	815.0
45.00	1001.0
46.00	107.0
47.00	912.0
47.90	615.0
49.00	4009.0
50.00	17840.0
51.00	5587.0
52.10	273.0
54.90	288.0
56.00	1543.0
57.00	2728.0
57.90	125.0
59.00	294.0
60.00	862.0
61.00	4771.0
62.00	4971.0
63.00	3463.0
64.00	323.0
64.90	226.0
67.00	309.0
68.00	9050.0
69.00	10020.0
70.00	713.0
71.10	53.0
72.00	535.0
73.00	5328.0
74.00	15684.0
75.00	45304.0
76.00	3760.0
77.00	504.0
77.80	385.0
78.90	2990.0
80.00	988.0
80.90	3289.0
81.90	762.0
82.90	90.0
86.00	141.0
86.90	3256.0
87.90	3419.0
88.70	178.0
90.90	301.0
91.90	2559.0
93.00	3947.0
94.00	10678.0
95.00	84376.0
96.00	5951.0
97.10	134.0
102.80	287.0
103.90	379.0
104.90	235.0
105.90	459.0
106.80	68.0
110.00	132.0
110.70	179.0
111.80	95.0
112.90	105.0
114.90	171.0
115.90	362.0
116.90	644.0
117.90	472.0
118.90	631.0
121.00	64.0
124.80	391.0
125.80	133.0
127.90	252.0
129.00	130.0
129.80	337.0
130.90	161.0
131.70	65.0
133.00	1347.0
134.80	246.0
136.10	54.0
136.80	170.0
140.90	951.0
141.70	82.0
142.90	989.0
144.70	122.0
145.80	164.0
146.80	230.0
147.70	136.0
148.00	145.0
148.90	129.0
149.90	109.0
151.70	61.0
153.90	73.0

Instrument :
MSVOA_W
ClientSampleId :
BFB09

155.00	250.0
156.90	140.0
158.80	117.0
160.80	244.0
162.90	195.0
163.80	56.0
164.70	123.0
170.90	63.0
171.90	430.0
173.90	59168.0
174.90	5049.0
175.90	64432.0
176.90	4090.0
177.90	209.0
179.00	340.0
179.90	52.0
189.00	138.0
190.00	55.0
190.90	1339.0
191.90	293.0
193.00	1608.0
193.90	343.0
194.90	160.0
203.00	170.0
204.90	358.0
205.80	121.0
207.00	974.0
208.00	155.0
209.10	117.0
220.90	104.0
234.90	109.0
236.70	58.0
248.90	1104.0
249.90	204.0
250.90	456.0
252.00	114.0
252.90	111.0
265.00	1183.0
266.00	358.0
266.90	299.0
267.90	52.0
279.10	169.0
281.00	16472.0
282.00	4968.0
283.00	2740.0
284.00	620.0
285.00	180.0

Instrument :
MSVOA_W
ClientSampleId :
BFB09

m/z	Abundance
36.00	675.0
37.00	3689.0
38.00	3360.0
39.00	1184.0
39.90	213.0
42.90	94.0
43.90	642.0
44.90	657.0
45.90	68.0
46.90	719.0
47.90	539.0
49.00	3185.0
50.00	14092.0
51.00	4207.0
52.00	203.0
54.90	311.0
56.00	1178.0
57.00	1983.0
58.00	107.0
58.90	107.0
60.00	605.0
61.00	3449.0
62.00	3750.0
63.00	2549.0
64.00	359.0
65.00	156.0
68.00	7394.0
69.00	7585.0
69.90	567.0
72.00	334.0
73.00	3707.0
74.00	12443.0
75.00	35040.0
76.00	2894.0
76.90	359.0
78.90	2312.0
79.90	670.0
80.90	2466.0
81.90	554.0
82.90	88.0
85.90	82.0
86.90	2603.0
87.90	2666.0
90.80	285.0
92.00	2128.0
93.00	3057.0
94.00	8346.0
95.00	67744.0
96.00	4509.0
97.00	105.0
102.90	125.0
103.90	327.0
105.00	139.0
105.90	344.0
106.70	61.0
109.80	78.0
111.00	134.0
111.90	94.0
112.90	55.0
115.00	76.0
115.80	266.0
116.90	469.0
117.90	402.0
118.90	502.0
124.90	134.0
127.90	215.0
128.90	123.0
129.80	299.0
131.00	130.0
133.00	583.0
133.90	125.0
134.90	155.0
136.90	147.0
140.80	765.0
142.80	686.0
144.60	66.0
145.10	63.0
145.80	94.0
146.90	161.0
147.80	160.0
148.80	99.0
149.80	92.0
153.80	71.0
154.90	120.0
156.90	126.0
158.90	60.0
160.90	118.0
162.70	70.0
162.90	70.0
164.90	88.0
171.00	76.0
171.90	328.0

Instrument :
MSVOA_W
ClientSampleId :
BFB09

173.90	56824.0
174.90	4605.0
175.90	50264.0
176.90	3769.0
177.90	160.0
178.90	170.0
190.90	457.0
191.90	154.0
193.00	667.0
193.80	140.0
195.00	97.0
203.10	70.0
205.00	121.0
206.90	485.0
208.00	108.0
234.90	79.0
249.00	568.0
250.00	208.0
250.90	190.0
251.90	64.0
264.80	639.0
266.00	192.0
267.00	124.0
281.00	9372.0
282.00	2290.0
283.10	1220.0
284.00	231.0
285.00	54.0

Instrument :
MSVOA_W
ClientSampleId :
BFB09

Scan 1749 (12.566 min): VW015595.D
BFB09

m/z	Abundance
39.90	110.0
44.00	204.0

Instrument :
MSVOA_W
ClientSampleId :
BFB09