


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW061318\
 Data File : VW003245.D
 Acq On : 13 Jun 2018 12:46
 Operator : JC/SY
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W061318S.M
 Title : SW846 8260
 Last Update : Sat Jun 16 05:18:54 2018

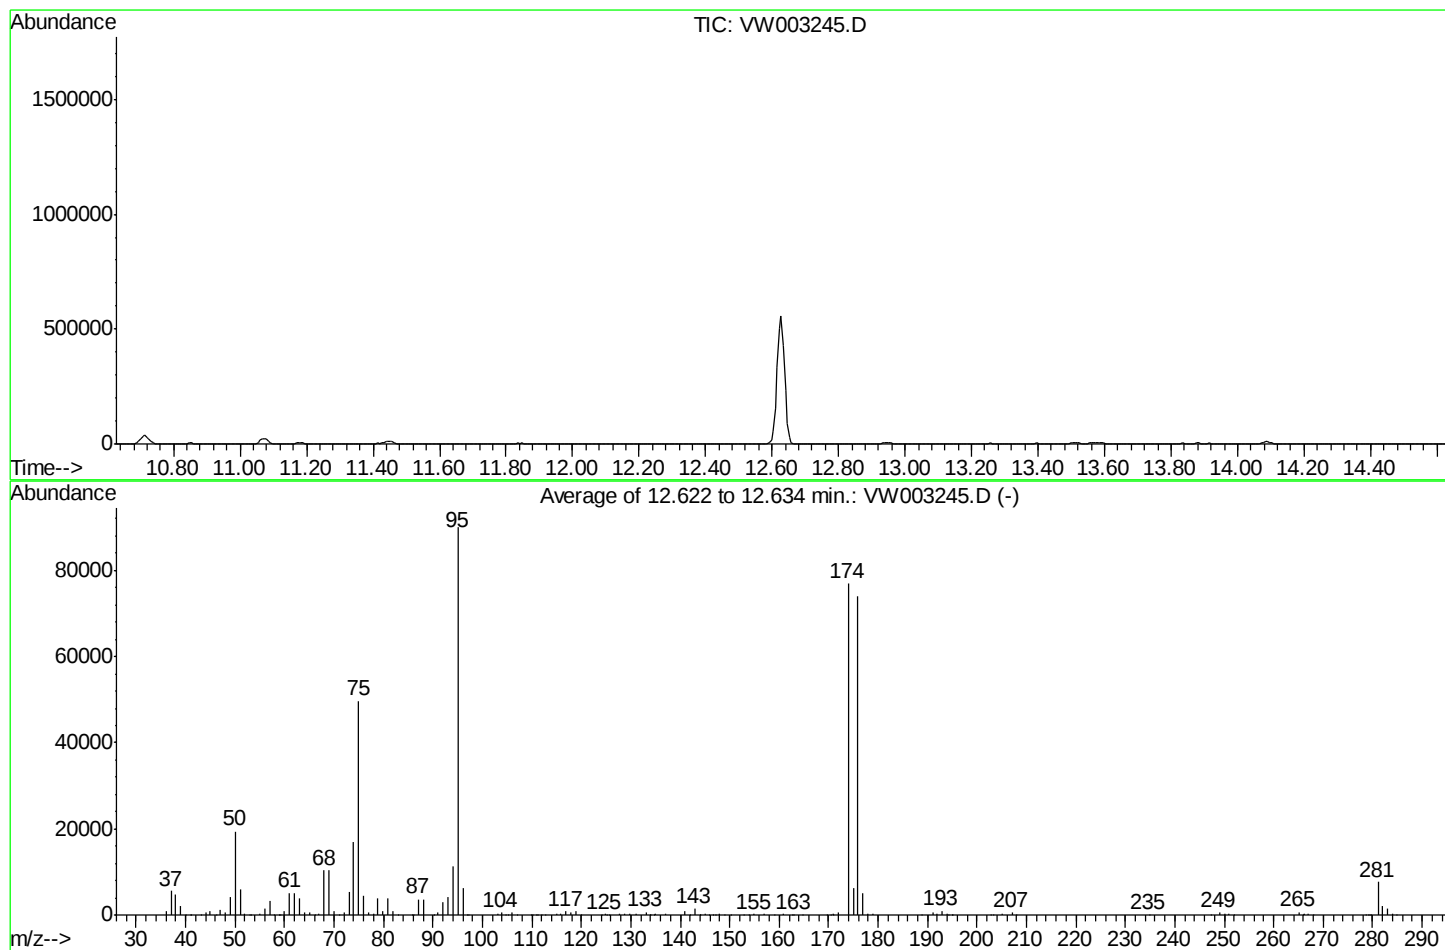

AutoFind: Scans 1810, 1811, 1812; Background Corrected with Scan 1801

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	19429	PASS
75	95	30	60	55.3	49768	PASS
95	95	100	100	100.0	90010	PASS
96	95	5	9	6.9	6202	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.4	76848	PASS
175	174	5	9	8.2	6312	PASS
176	174	95	101	96.4	74114	PASS
177	176	5	9	6.7	4999	PASS