


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW061419\
 Data File : VW010805.D
 Acq On : 14 Jun 2019 09:18
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W060419S.M
 Title : SW846 8260
 Last Update : Wed Jun 05 03:21:19 2019

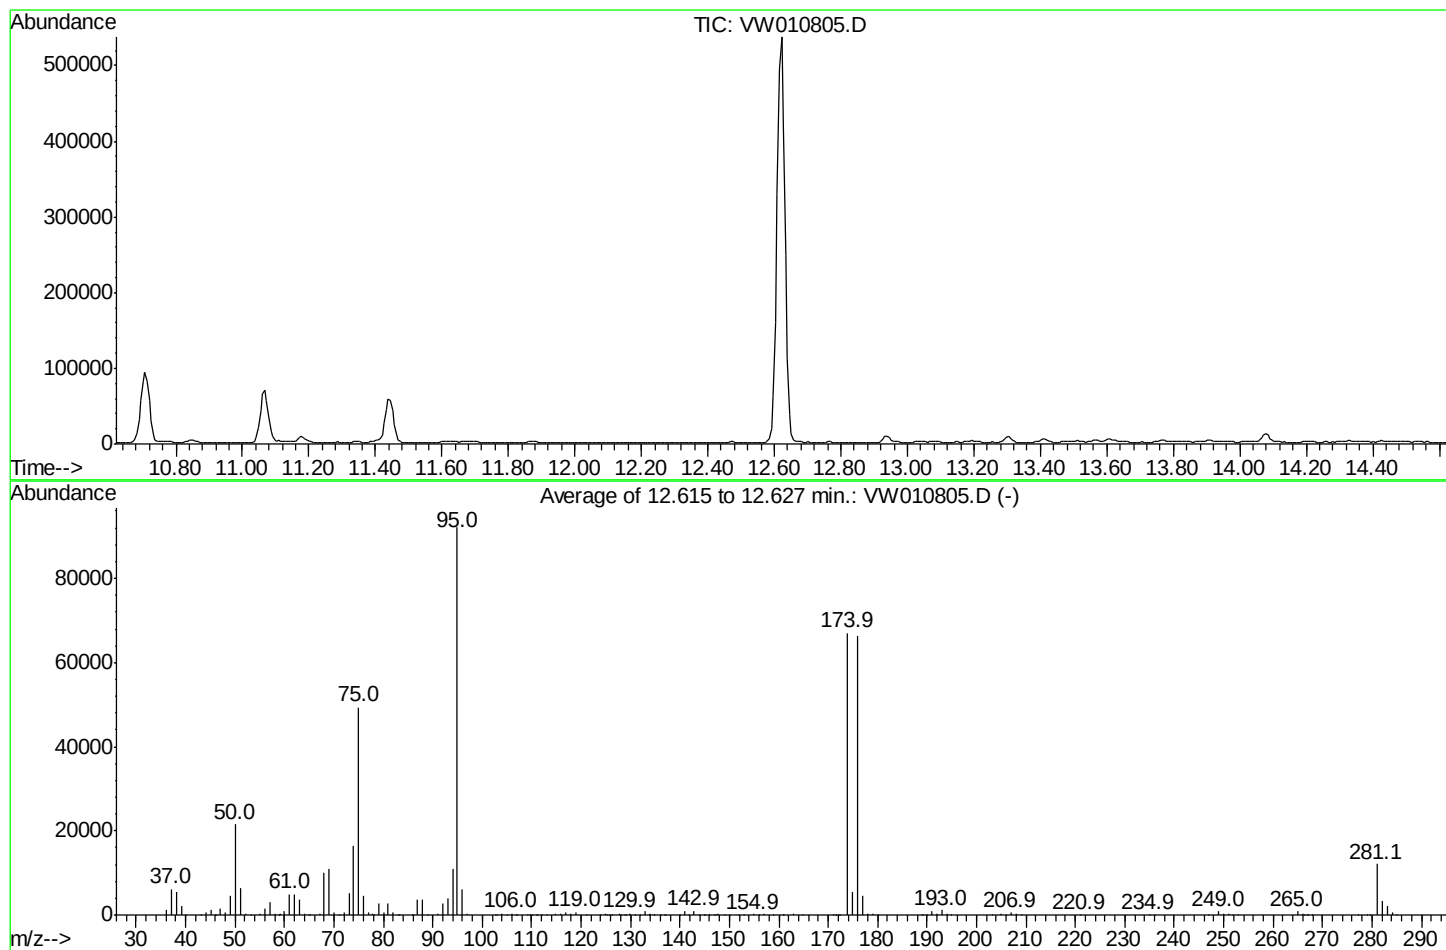

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.4	21592	PASS
75	95	30	60	53.6	49416	PASS
95	95	100	100	100.0	92133	PASS
96	95	5	9	6.7	6154	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.8	67069	PASS
175	174	5	9	8.4	5628	PASS
176	174	95	101	98.9	66357	PASS
177	176	5	9	6.8	4524	PASS