

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061421\
 Data File : VW019205.D
 Acq On : 14 Jun 2021 10:34
 Operator : SY/VA
 Sample : VW0614SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK106

Manual Integrations
 APPROVED

MMDadoda
 6/15/2021 5:14:00 PM

Quant Time: Jun 15 01:17:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 15 01:16:33 2021
 Response via : Initial Calibration

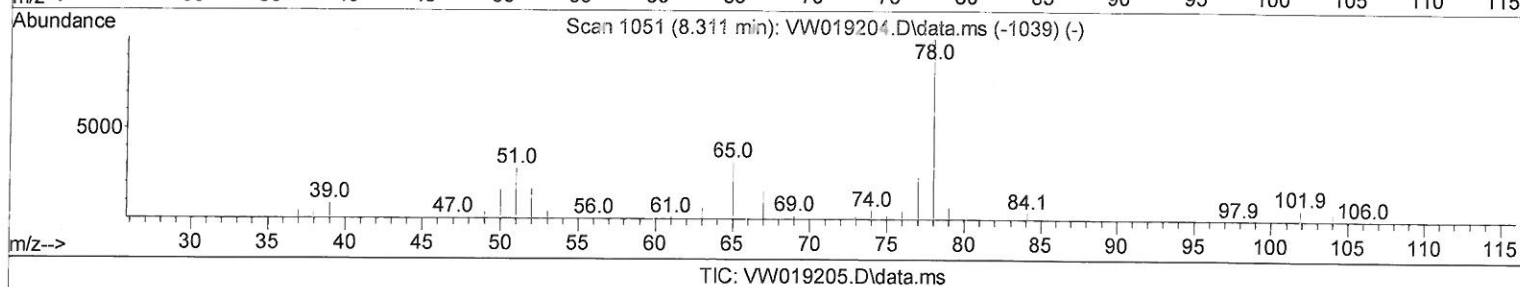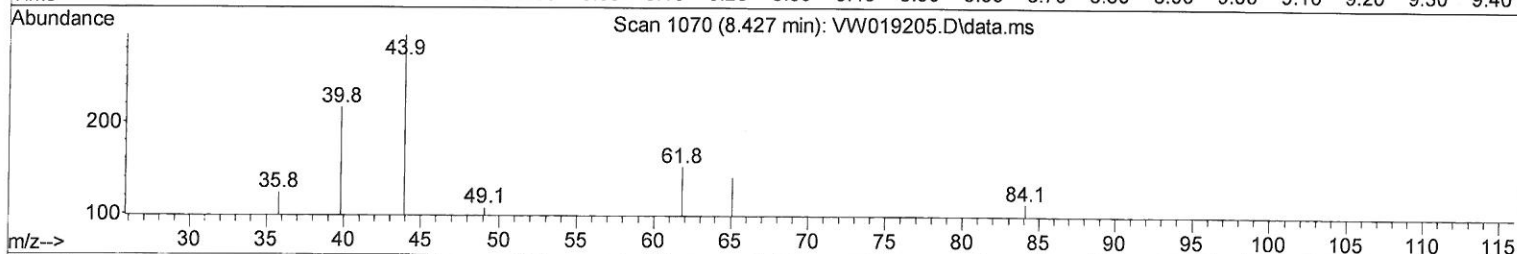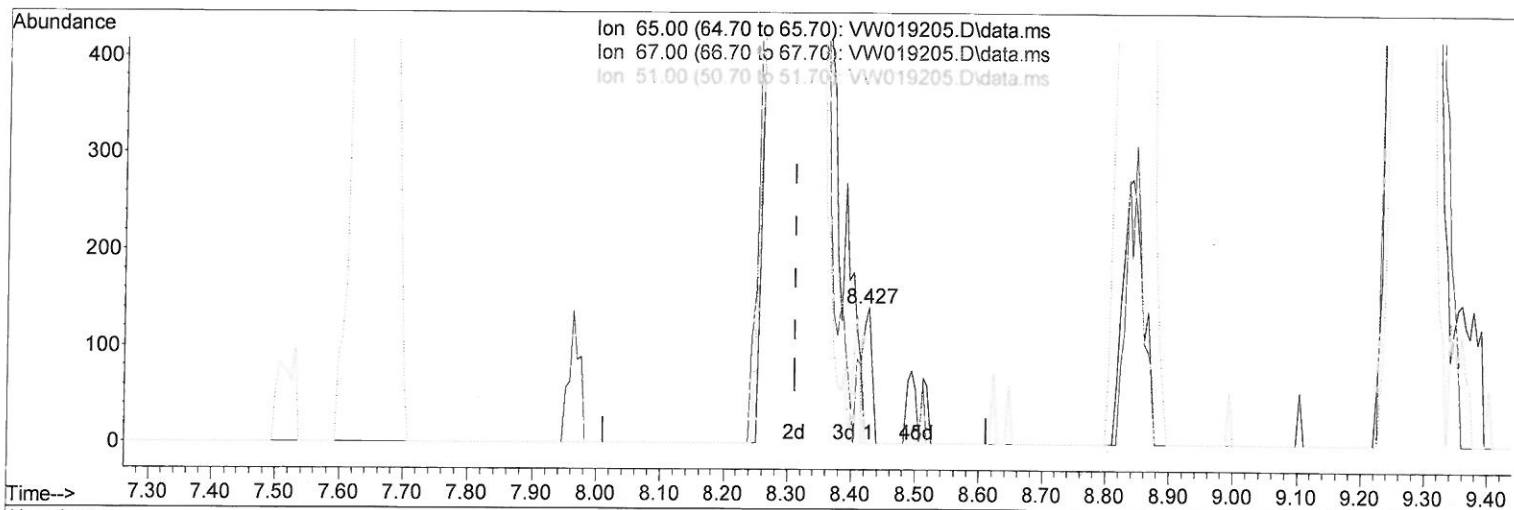

(26) 1,2-Dichloroethane-d4 (S)

8.427min (+ 0.116) 0.02 ug/L

response 124

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	51.70	50.00
51.00	98.00	95.16
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061421\
 Data File : VW019205.D
 Acq On : 14 Jun 2021 10:34
 Operator : SY/VA
 Sample : VW0614SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK106

Manual Integrations
 APPROVED

MMDadoda
 6/15/2021 5:14:00 PM

Quant Time: Jun 15 01:17:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 15 01:16:33 2021
 Response via : Initial Calibration

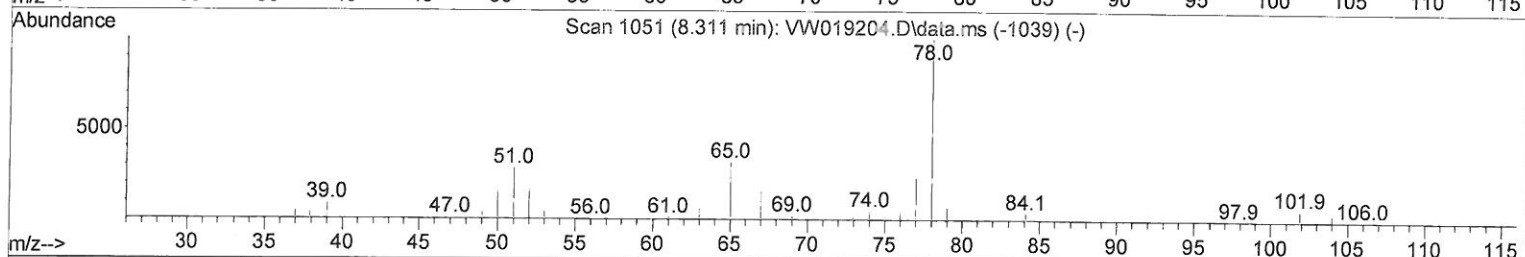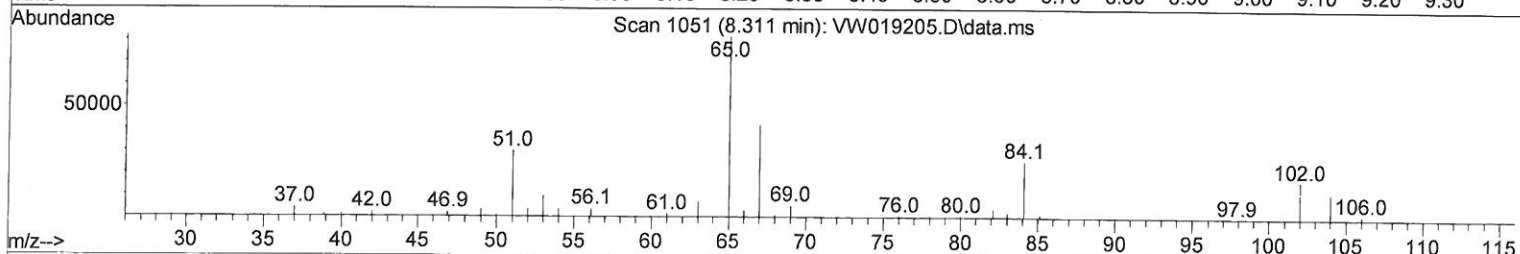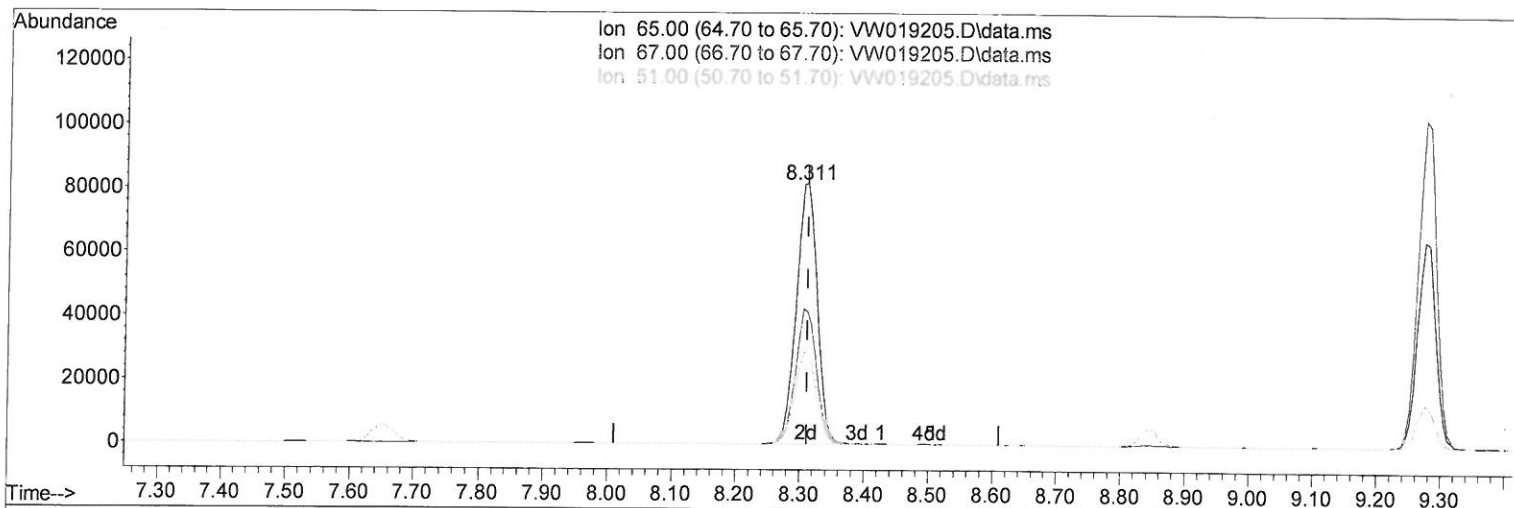

TIC: VW019205.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.311min (-0.000) 24.02 ug/L m

response 184431

Ion Exp% Act%

65.00 100.00 100.00

67.00 51.70 0.03#

51.00 98.00 0.06#

0.00 0.00 0.00

206/16/2022

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061421\
 Data File : VW019205.D
 Acq On : 14 Jun 2021 10:34
 Operator : SY/VA
 Sample : VW0614SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK106

Manual Integrations
 APPROVED

MMDadoda
 6/15/2021 5:14:00 PM

Quant Time: Jun 15 01:17:26 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 15 01:16:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	509218	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	470944	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	225048	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	144198	21.415	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	85.640%		
7) Chloroethane-d5	2.897	69	130835	22.813	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	91.240%		
11) 1,1-Dichloroethene-d2	4.025	63	219782	16.428	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	65.720%		
21) 2-Butanone-d5	7.092	46	81312	46.100	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	92.200%		
24) Chloroform-d	7.653	84	332879	24.315	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	97.240%		
26) 1,2-Dichloroethane-d4	8.311	65	184431m	24.017	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	96.080%		
32) Benzene-d6	8.281	84	654805	24.404	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	97.600%		
36) 1,2-Dichloropropane-d6	9.274	67	206645	25.404	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	101.600%		
41) Toluene-d8	10.323	98	585747	23.771	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	95.080%		
43) trans-1,3-Dichloroprop...	10.579	79	79073	22.445	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	89.800%		
47) 2-Hexanone-d5	10.927	63	65203	47.270	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	94.540%		
56) 1,1,2,2-Tetrachloroeth...	12.694	84	160503	23.920	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	95.680%		
66) 1,2-Dichlorobenzene-d4	13.853	152	181897	23.157	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	92.640%		
Target Compounds						
42) Toluene	10.390	91	11567	0.347	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

06/16/21 Sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061421\
Data File : VW019205.D
Acq On : 14 Jun 2021 10:34
Operator : SY/VA
Sample : VW0614SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK106

Manual Integrations
APPROVED

MMDadoda
6/15/2021 5:14:00 PM

Quant Time: Jun 15 01:17:26 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 15 01:16:33 2021
Response via : Initial Calibration

