

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061421\
 Data File : VW019210.D
 Acq On : 14 Jun 2021 12:48
 Operator : SY/VA
 Sample : M2682-16
 Misc : 5.32G/10ML/MSVOA_W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDC0

Manual Integrations
 APPROVED

MMDadoda
 6/15/2021 5:14:01 PM

Quant Time: Jun 15 01:18:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 15 01:16:33 2021
 Response via : Initial Calibration

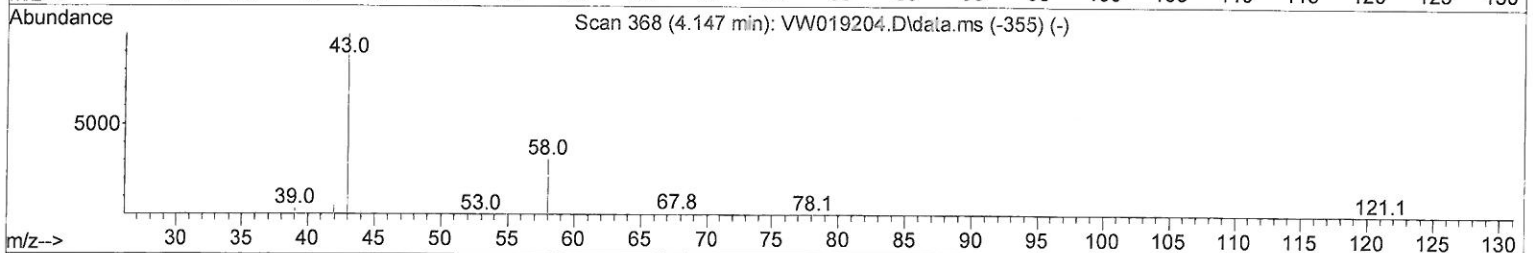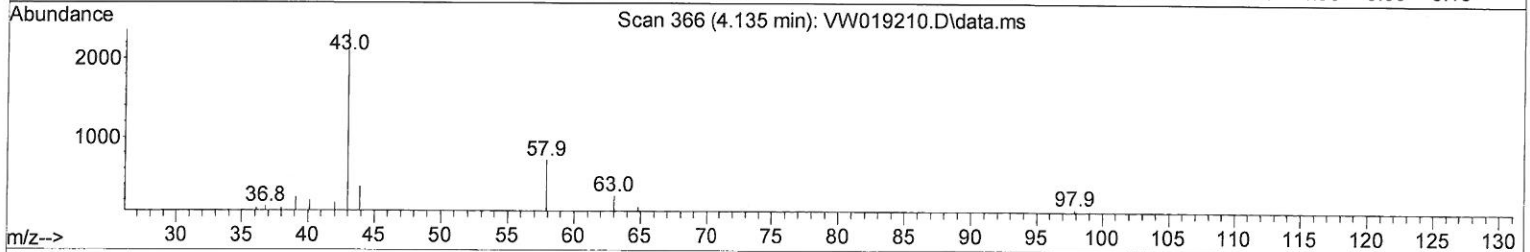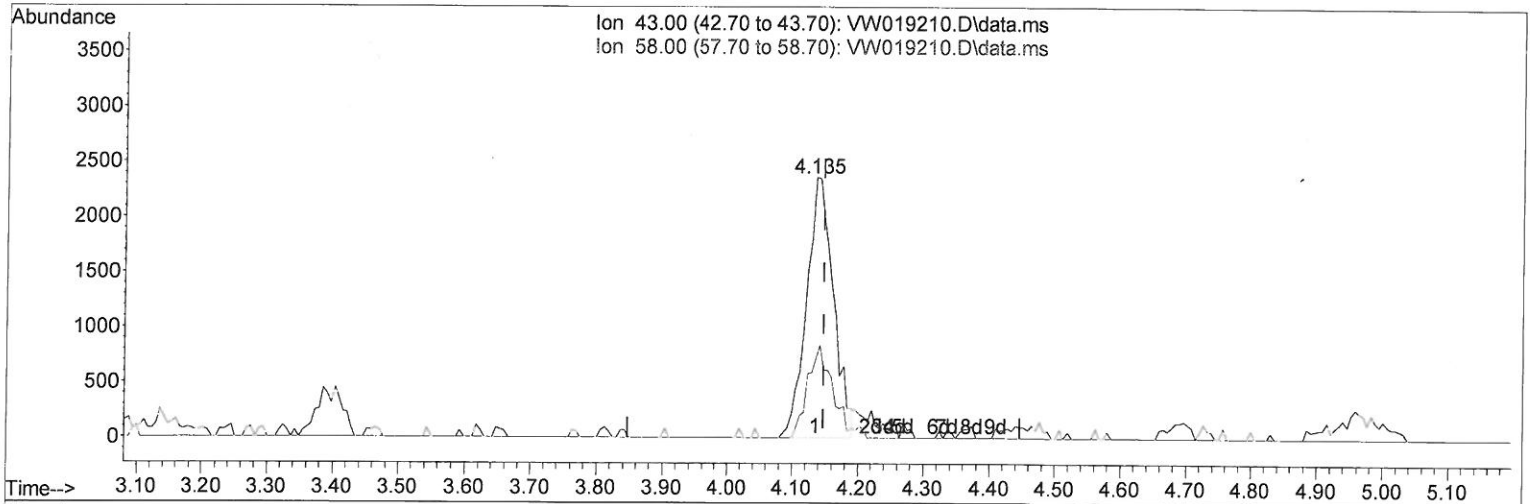

TIC: VW019210.D\data.ms

(13) Acetone (T)

4.135min (-0.012) 5.29 ug/L

response 6712

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	30.24
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061421\
 Data File : VW019210.D
 Acq On : 14 Jun 2021 12:48
 Operator : SY/VA
 Sample : M2682-16
 Misc : 5.32G/10ML/MSVOA_W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDC0

Manual Integrations
 APPROVED

MMDadoda
 6/15/2021 5:14:01 PM

Quant Time: Jun 15 01:18:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 15 01:16:33 2021
 Response via : Initial Calibration

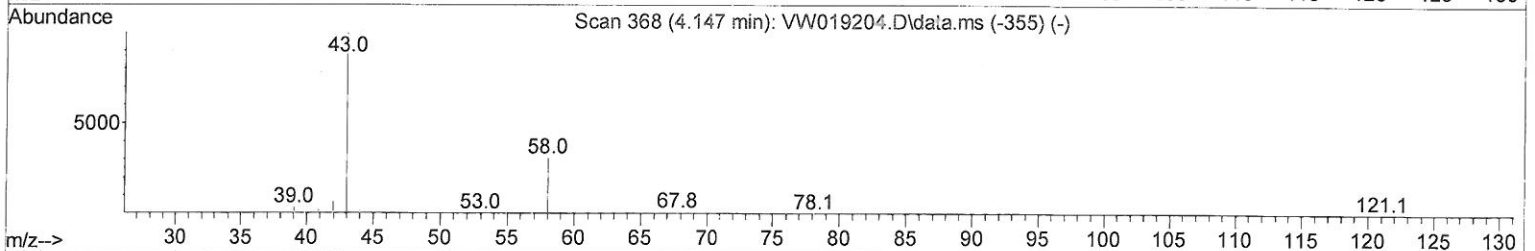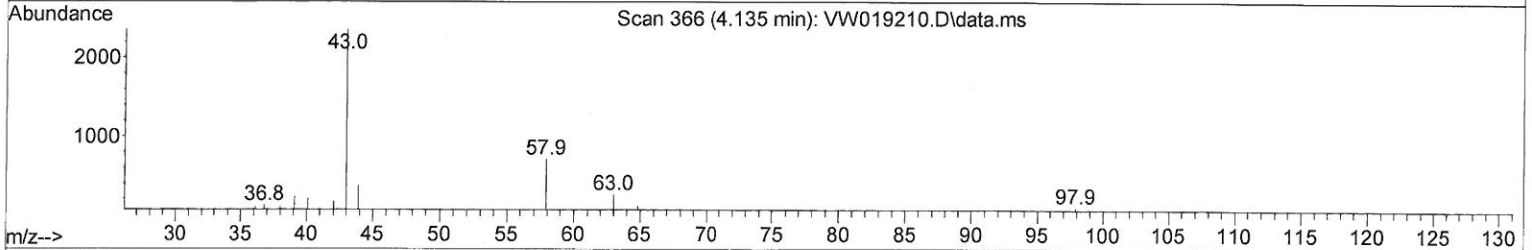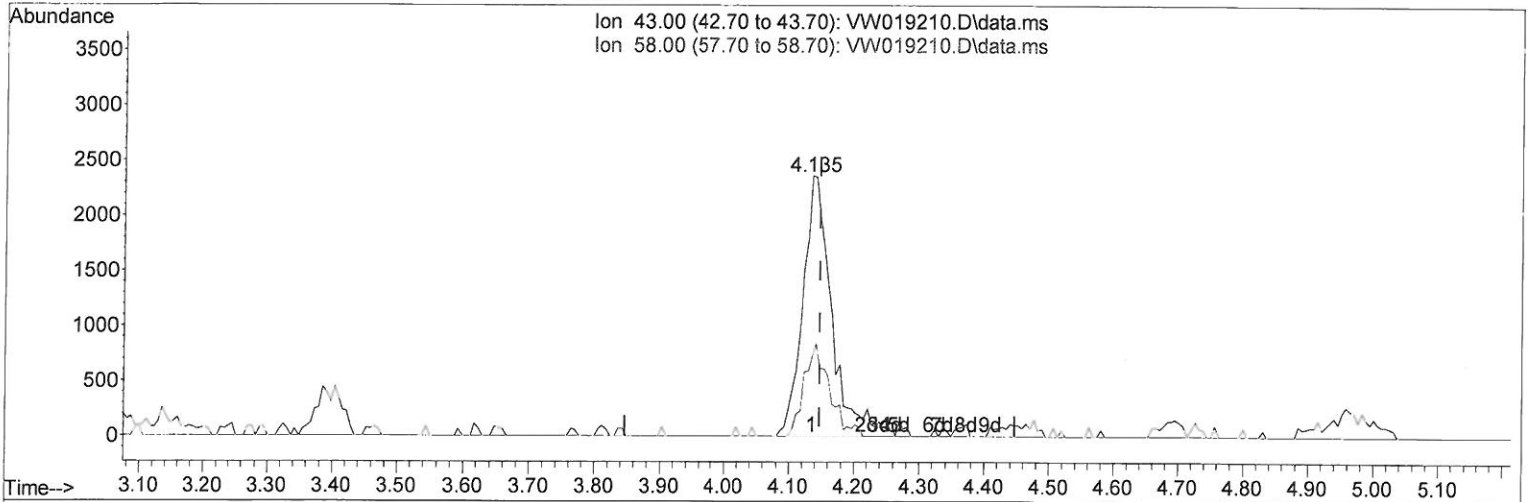

TIC: VW019210.D\data.ms

(13) Acetone (T)

4.135min (-0.012) 5.52 ug/L m

response 7000

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	29.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061421\
 Data File : VW019210.D
 Acq On : 14 Jun 2021 12:48
 Operator : SY/VA
 Sample : M2682-16
 Misc : 5.32G/10ML/MSVOA_W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDC0

Manual Integrations
 APPROVED

MMDadoda
 6/15/2021 5:14:01 PM

Quant Time: Jun 15 01:18:20 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 15 01:16:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	413365	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	339539	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	117045	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	136061	24.892	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	99.560%		
7) Chloroethane-d5	2.898	69	111911	24.039	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery =	96.160%		
11) 1,1-Dichloroethene-d2	4.026	63	197215	18.160	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery =	72.640%		
21) 2-Butanone-d5	7.086	46	50577	35.324	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	70.640%		
24) Chloroform-d	7.653	84	263260	23.689	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery =	94.760%		
26) 1,2-Dichloroethane-d4	8.305	65	137523	22.061	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery =	88.240%		
32) Benzene-d6	8.281	84	525369	27.158	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery =	108.640%		
36) 1,2-Dichloropropane-d6	9.275	67	157433	26.845	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery =	107.360%		
41) Toluene-d8	10.329	98	455194	25.622	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery =	102.480%		
43) trans-1,3-Dichloroprop...	10.579	79	54896	21.613	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery =	86.440%		
47) 2-Hexanone-d5	10.927	63	40266	40.489	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery =	80.980%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	96220	19.890	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery =	79.560%		
66) 1,2-Dichlorobenzene-d4	13.853	152	96525	23.627	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery =	94.520%		
Target Compounds						
13) Acetone	4.135	43	7000m	5.517	ug/L	Qvalue 87
16) Methylene chloride	4.928	84	14688	1.915	ug/L	87

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061421\
Data File : VW019210.D
Acq On : 14 Jun 2021 12:48
Operator : SY/VA
Sample : M2682-16
Misc : 5.32G/10ML/MSVOA_W/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDC0

Manual Integrations
APPROVED

MMDadoda
6/15/2021 5:14:01 PM

Quant Time: Jun 15 01:18:20 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 15 01:16:33 2021
Response via : Initial Calibration

