

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061421\
 Data File : VW019216.D
 Acq On : 14 Jun 2021 15:33
 Operator : SY/VA
 Sample : M2704-11
 Misc : 6.60G/10ML/MSVOA_W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDD4

Manual Integrations
 APPROVED

MMDadoda
 6/15/2021 5:14:07 PM

Quant Time: Jun 15 01:19:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 15 01:16:33 2021
 Response via : Initial Calibration

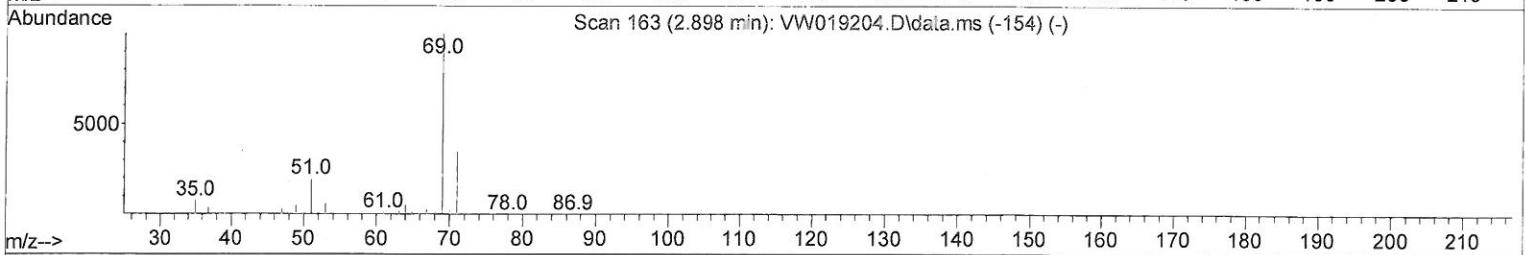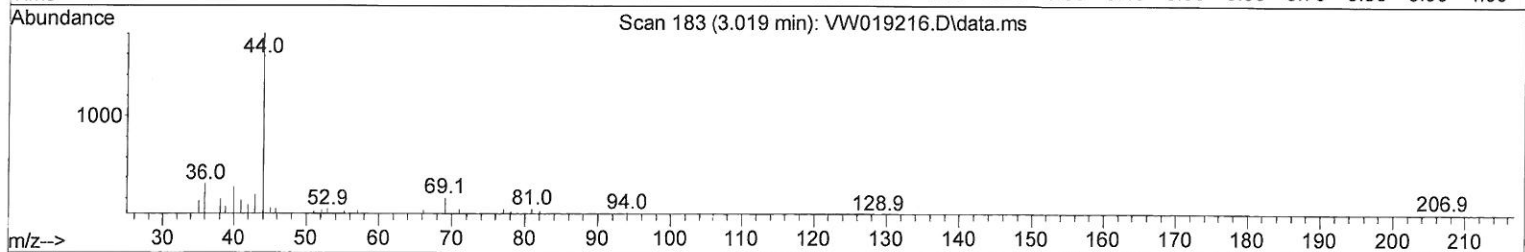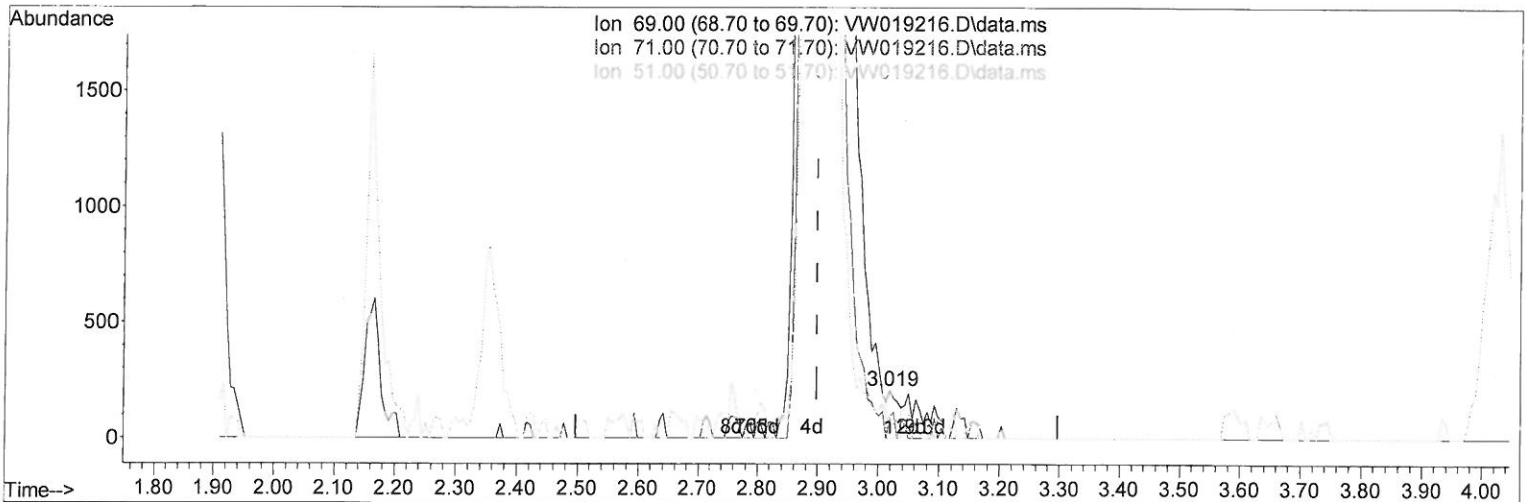

TIC: VW019216.D\data.ms

(7) Chloroethane-d5 (S)

3.019min (+ 0.122) 0.04 ug/L

response 246

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	30.49
51.00	28.40	32.93
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061421\
 Data File : VW019216.D
 Acq On : 14 Jun 2021 15:33
 Operator : SY/VA
 Sample : M2704-11
 Misc : 6.60G/10ML/MSVOA_W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDD4

Manual Integrations
 APPROVED

MMDadoda
 6/15/2021 5:14:07 PM

Quant Time: Jun 15 01:19:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 15 01:16:33 2021
 Response via : Initial Calibration

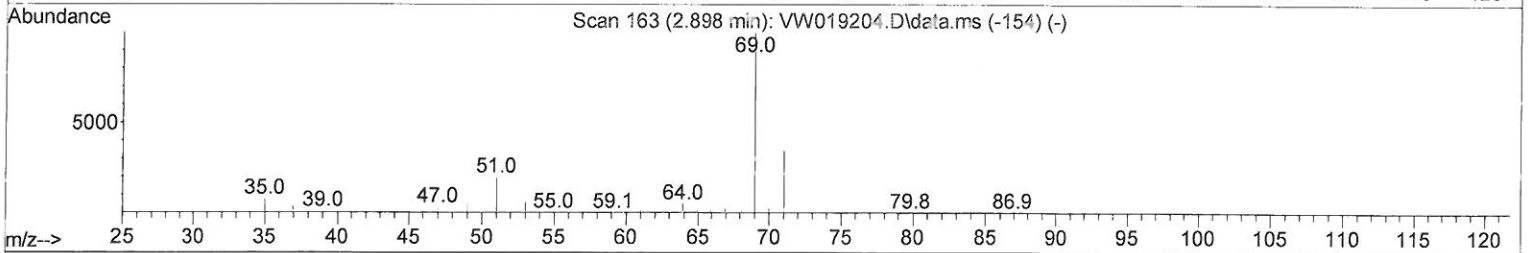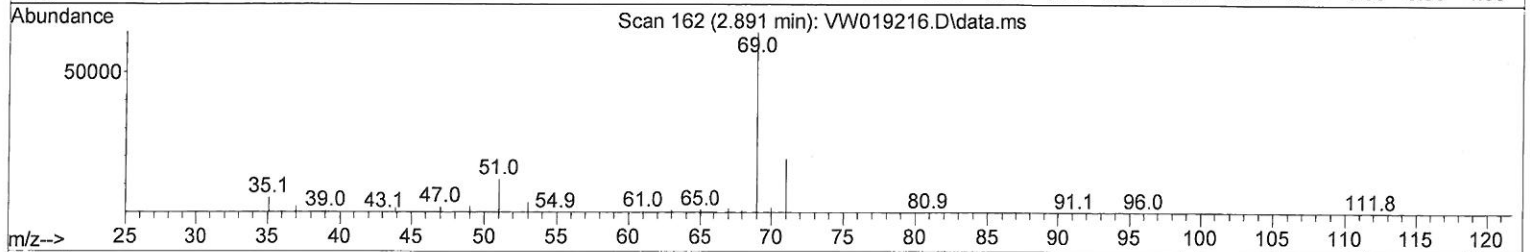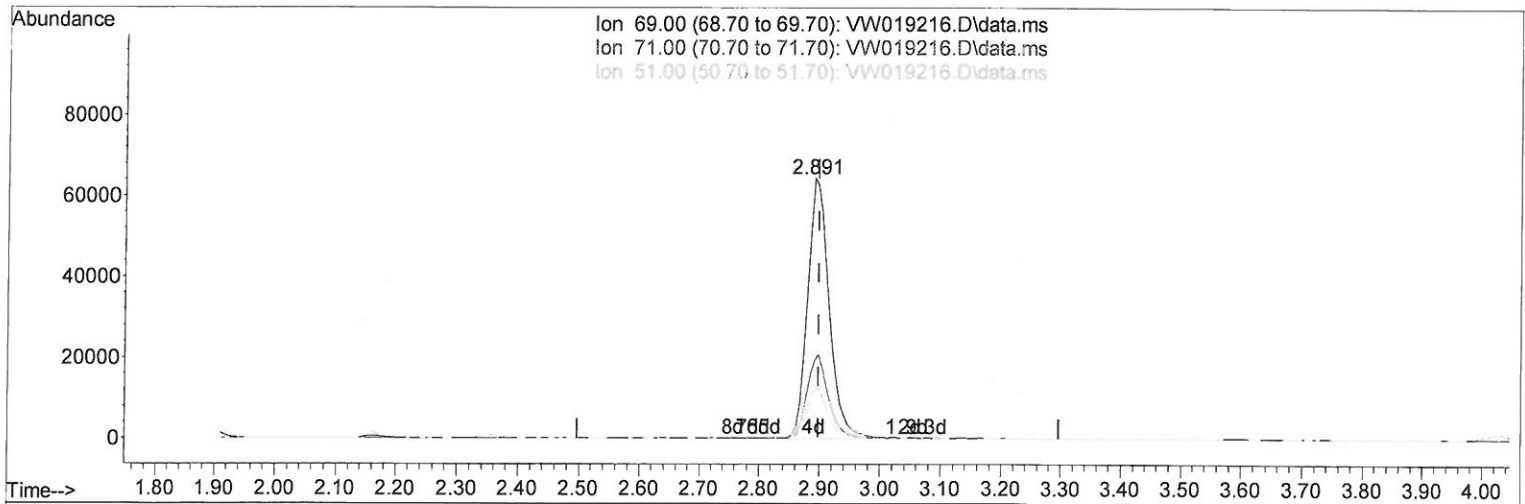

TIC: VW019216.D\data.ms

(7) Chloroethane-d5 (S)

2.891min (-0.006) 22.94 ug/L m

response 159485

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	0.05#
51.00	28.40	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061421\
 Data File : VW019216.D
 Acq On : 14 Jun 2021 15:33
 Operator : SY/VA
 Sample : M2704-11
 Misc : 6.60G/10ML/MSVOA_W/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDD4

Manual Integrations
 APPROVED

MMDadoda
 6/15/2021 5:14:07 PM

Quant Time: Jun 15 01:19:29 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 15 01:16:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	617345	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	567741	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	244972	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	189397	23.201	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	92.800%		
7) Chloroethane-d5	2.891	69	159485m	22.938	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	91.760%		
11) 1,1-Dichloroethene-d2	4.025	63	276041	17.019	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	68.080%		
21) 2-Butanone-d5	7.086	46	64559	30.191	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	60.380%		
24) Chloroform-d	7.653	84	401095	24.166	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	96.680%		
26) 1,2-Dichloroethane-d4	8.305	65	194734	20.917	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	83.680%		
32) Benzene-d6	8.275	84	803082	24.828	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	99.320%		
36) 1,2-Dichloropropane-d6	9.274	67	238107	24.281	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	97.120%		
41) Toluene-d8	10.323	98	716879	24.132	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	96.520%		
43) trans-1,3-Dichloroprop...	10.579	79	87536	20.611	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	82.440%		
47) 2-Hexanone-d5	10.927	63	53626	32.249	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	64.500%		
56) 1,1,2,2-Tetrachloroeth...	12.694	84	147306	18.210	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	72.840%		
66) 1,2-Dichlorobenzene-d4	13.853	152	205915	24.082	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	96.320%		
Target Compounds						
13) Acetone	4.153	43	9837	5.192	ug/L	87
16) Methylene chloride	4.922	84	43266	3.777	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

06/16/21 sy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061421\
Data File : VW019216.D
Acq On : 14 Jun 2021 15:33
Operator : SY/VA
Sample : M2704-11
Misc : 6.60G/10ML/MSVOA_W/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDD4

Manual Integrations
APPROVED

MMDadoda
6/15/2021 5:14:07 PM

Quant Time: Jun 15 01:19:29 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 15 01:16:33 2021
Response via : Initial Calibration

