

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061421\
 Data File : VW019217.D
 Acq On : 14 Jun 2021 15:57
 Operator : SY/VA
 Sample : M2704-12
 Misc : 5.58G/10ML/MSVOA_W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDD5

Manual Integrations
 APPROVED

MMDadoda
 6/15/2021 5:14:08 PM

Quant Time: Jun 15 01:19:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 15 01:16:33 2021
 Response via : Initial Calibration

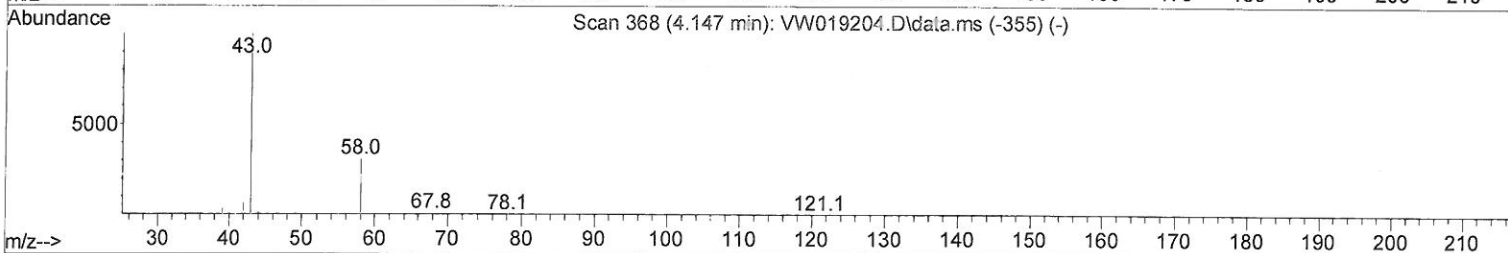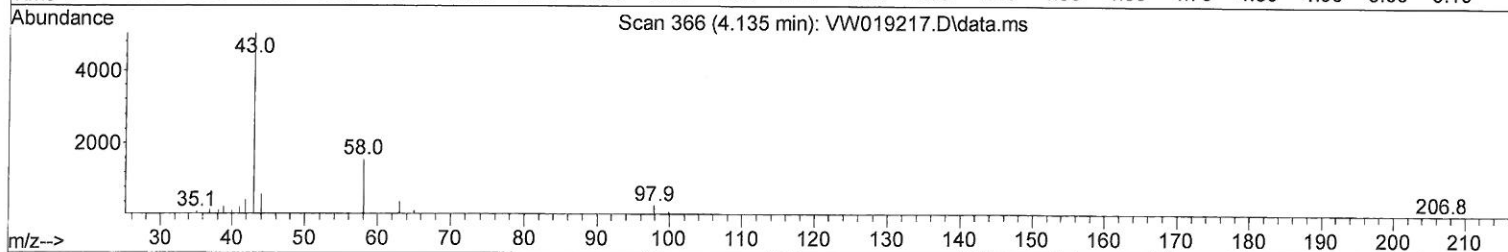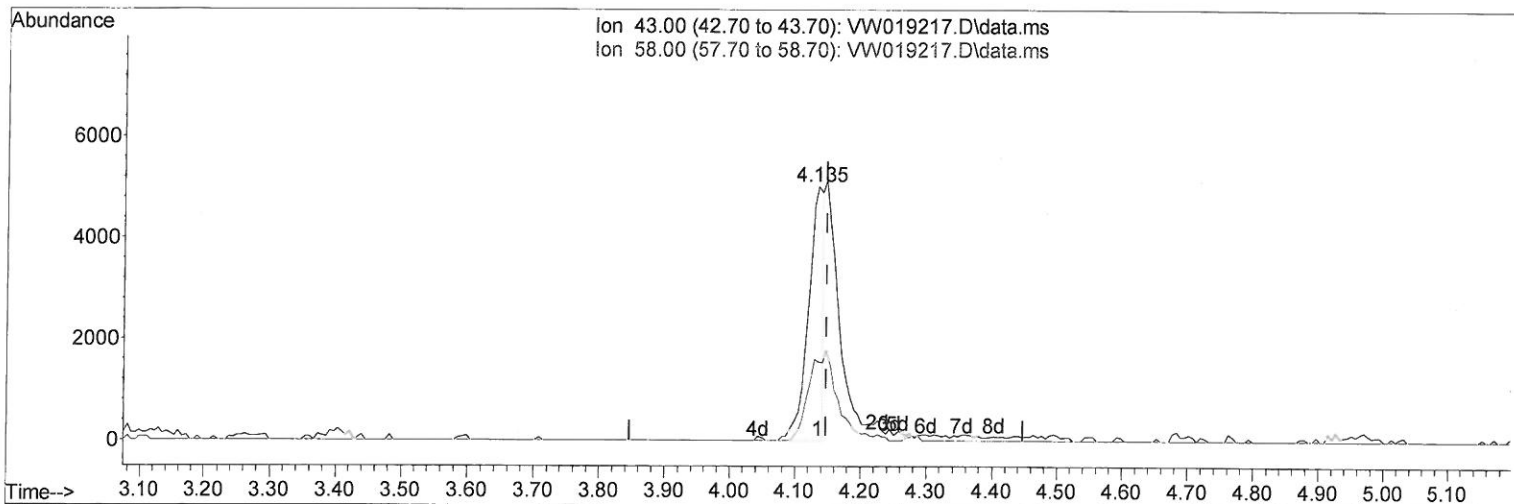

TIC: VW019217.D\data.ms

(13) Acetone (T)

4.135min (-0.013) 4.72 ug/L

response 8144

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	33.07
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061421\
 Data File : VW019217.D
 Acq On : 14 Jun 2021 15:57
 Operator : SY/VA
 Sample : M2704-12
 Misc : 5.58G/10ML/MSVOA_W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDD5

Manual Integrations
 APPROVED

MMDadoda
 6/15/2021 5:14:08 PM

Quant Time: Jun 15 01:19:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Jun 15 01:16:33 2021
 Response via : Initial Calibration

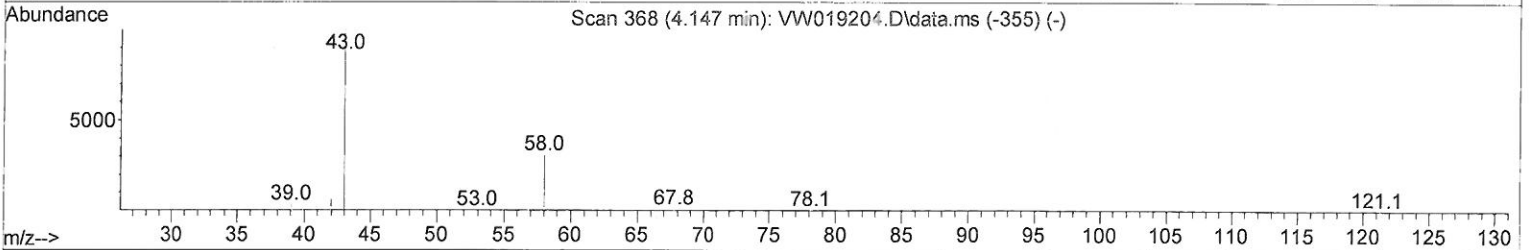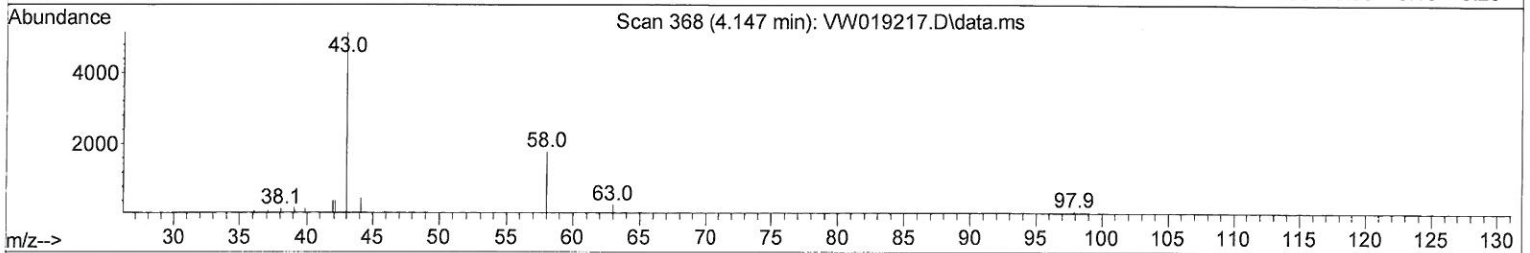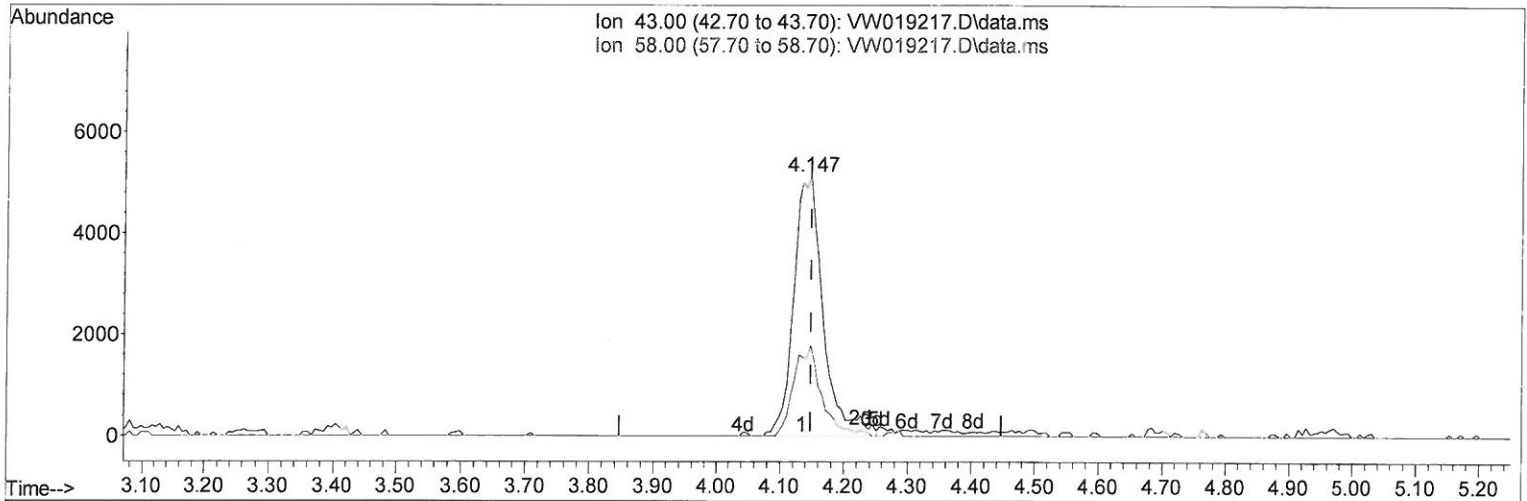

TIC: VW019217.D\data.ms

(13) Acetone (T)

4.147min (-0.000) 9.49 ug/L m

response 16374

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.90	16.45
0.00	0.00	0.00
0.00	0.00	0.00

506/16/2024

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061421\
 Data File : VW019217.D
 Acq On : 14 Jun 2021 15:57
 Operator : SY/VA
 Sample : M2704-12
 Misc : 5.58G/10ML/MSVOA_W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDD5

Manual Integrations
 APPROVED

MMDadoda
 6/15/2021 5:14:08 PM

Quant Time: Jun 15 01:19:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 Qlast Update : Tue Jun 15 01:16:33 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.847	114	562120	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.633	117	488270	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	193932	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	168995	22.735	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	90.960%	
7) Chloroethane-d5	2.897	69	139294	22.003	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	88.000%	
11) 1,1-Dichloroethene-d2	4.025	63	238812	16.171	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	64.680%	
21) 2-Butanone-d5	7.085	46	61820	31.751	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	63.500%	
24) Chloroform-d	7.652	84	342749	22.680	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	90.720%	
26) 1,2-Dichloroethane-d4	8.311	65	175512	20.704	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	82.800%	
32) Benzene-d6	8.280	84	685097	24.627	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	98.520%	
36) 1,2-Dichloropropane-d6	9.274	67	206420	24.476	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	97.920%	
41) Toluene-d8	10.329	98	604185	23.649	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	94.600%	
43) trans-1,3-Dichloroprop...	10.579	79	72696	19.903	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	79.600%	
47) 2-Hexanone-d5	10.926	63	50424	35.259	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	70.520%	
56) 1,1,2,2-Tetrachloroeth...	12.694	84	129323	18.589	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	74.360%	
66) 1,2-Dichlorobenzene-d4	13.853	152	155042	22.905	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	91.600%	
Target Compounds						
13) Acetone	4.147	43	16374m	9.490	ug/L	Qvalue 95
16) Methylene chloride	4.933	84	33981	3.258	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061421\
Data File : VW019217.D
Acq On : 14 Jun 2021 15:57
Operator : SY/VA
Sample : M2704-12
Misc : 5.58G/10ML/MSVOA_W/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDD5

Manual Integrations
APPROVED

MMDadoda
6/15/2021 5:14:08 PM

Quant Time: Jun 15 01:19:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Jun 15 01:16:33 2021
Response via : Initial Calibration

