

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061521\
 Data File : VW019224.D
 Acq On : 15 Jun 2021 12:05
 Operator : SY/VA
 Sample : M2680-17
 Misc : 4.80G/10ML/MSVOA_W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDC1

Manual Integrations
 APPROVED

MMDadoda
 6/16/2021 5:02:24 PM

Quant Time: Jun 16 01:44:12 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 16 01:01:36 2021
 Response via : Initial Calibration

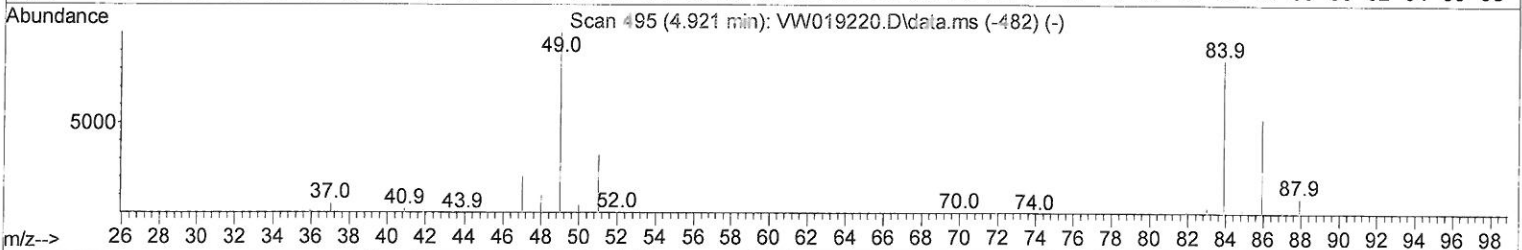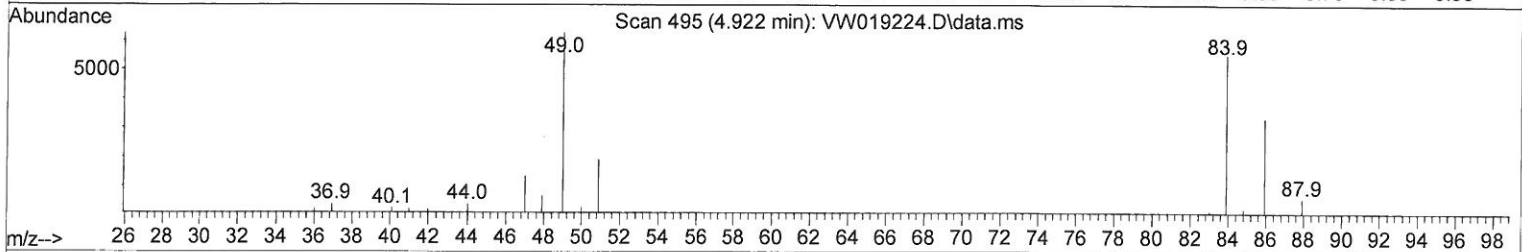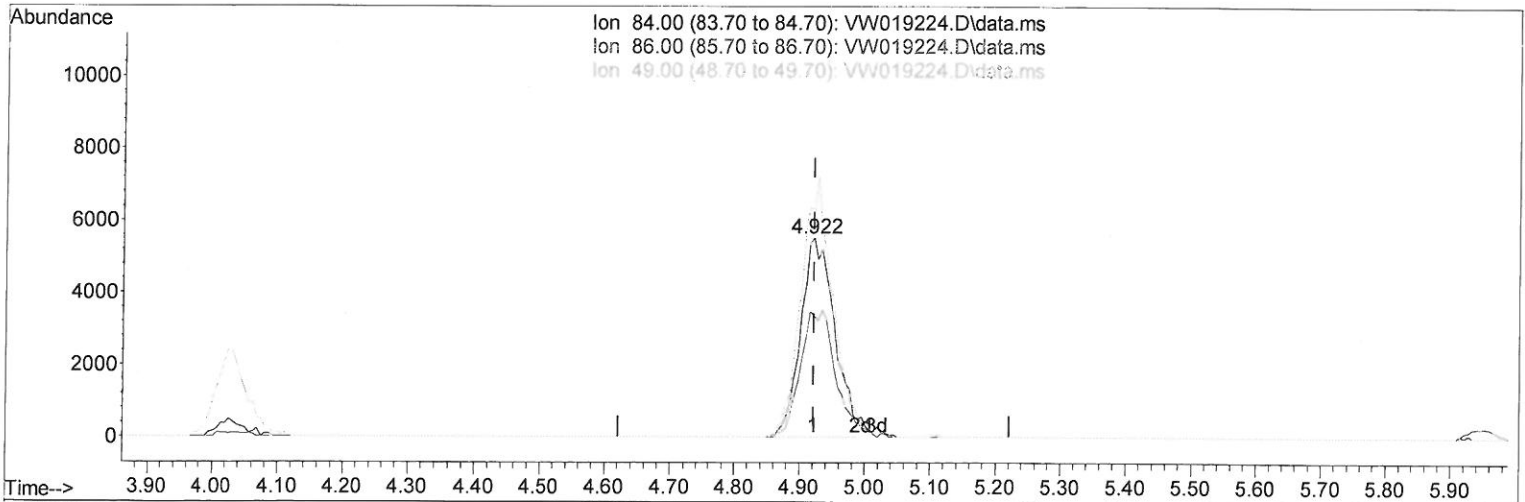

TIC: VW019224.D\data.ms

(16) Methylene chloride (T)

4.922min (+ 0.000) 1.88 ug/L

response 19784

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	60.81
49.00	123.70	113.58
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061521\
 Data File : VW019224.D
 Acq On : 15 Jun 2021 12:05
 Operator : SY/VA
 Sample : M2680-17
 Misc : 4.80G/10ML/MSVOA_W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDC1

Manual Integrations
 APPROVED

MMDadoda
 6/16/2021 5:02:24 PM

Quant Time: Jun 16 01:02:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 16 01:01:36 2021
 Response via : Initial Calibration

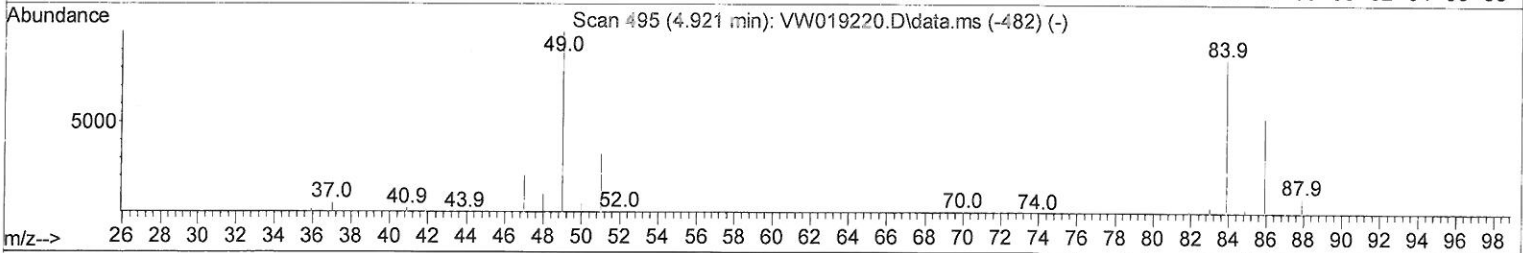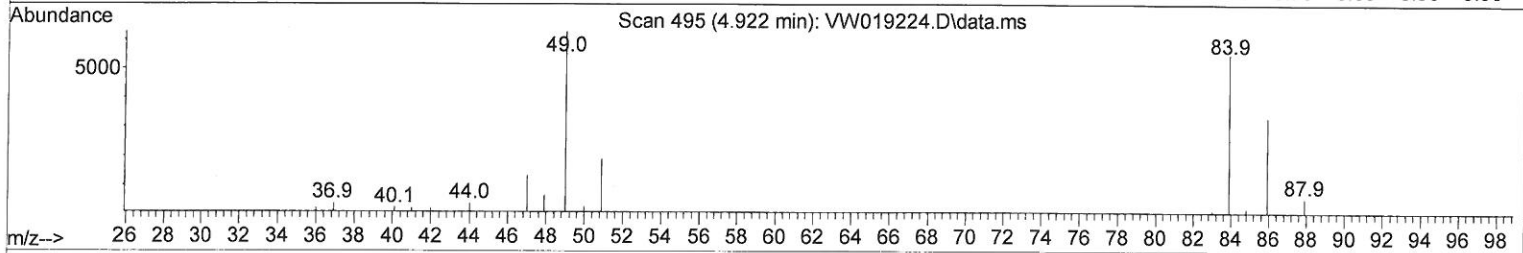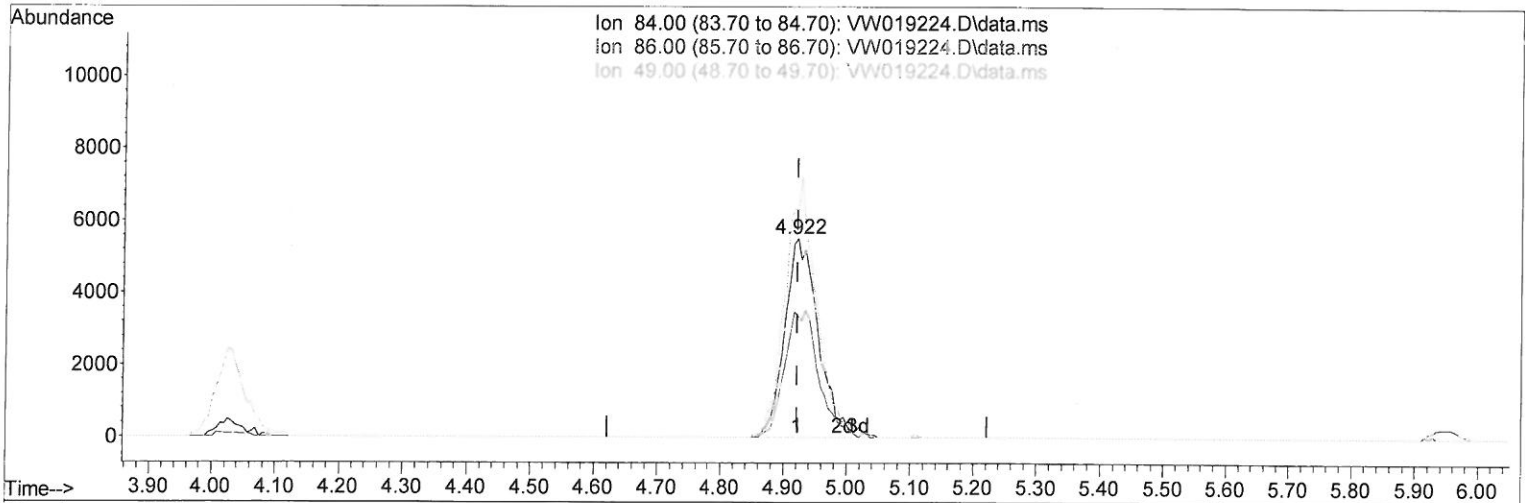

TIC: VW019224.D\data.ms

(16) Methylene chloride (T)

4.922min (+ 0.000) 1.95 ug/L m

response 20461

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	64.70	60.81
49.00	123.70	113.58
0.00	0.00	0.00

206/16/2154

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061521\
 Data File : VW019224.D
 Acq On : 15 Jun 2021 12:05
 Operator : SY/VA
 Sample : M2680-17
 Misc : 4.80G/10ML/MSVOA_W/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDC1

Manual Integrations
 APPROVED

MMDadoda
 6/16/2021 5:02:24 PM

Quant Time: Jun 16 01:02:43 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 16 01:01:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	566663	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	517189	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	207265	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	182783	24.393	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	97.560%		
7) Chloroethane-d5	2.898	69	148927	23.336	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	93.360%		
11) 1,1-Dichloroethene-d2	4.025	63	259883	17.456	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	69.840%		
21) 2-Butanone-d5	7.086	46	69495	35.406	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	70.820%		
24) Chloroform-d	7.653	84	381464	25.039	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	100.160%		
26) 1,2-Dichloroethane-d4	8.311	65	193923	22.693	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	90.760%		
32) Benzene-d6	8.281	84	766037	25.997	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	104.000%		
36) 1,2-Dichloropropane-d6	9.274	67	228110	25.536	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	102.160%		
41) Toluene-d8	10.323	98	681616	25.188	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	100.760%		
43) trans-1,3-Dichloroprop...	10.579	79	85597	22.124	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	88.480%		
47) 2-Hexanone-d5	10.927	63	56526	37.315	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	74.640%		
56) 1,1,2,2-Tetrachloroeth...	12.695	84	145013	19.679	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	78.720%		
66) 1,2-Dichlorobenzene-d4	13.853	152	186136	25.730	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	102.920%		
Target Compounds						
13) Acetone	4.141	43	19448	11.182	ug/L	91
16) Methylene chloride	4.922	84	20461m	1.946	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061521\
Data File : VW019224.D
Acq On : 15 Jun 2021 12:05
Operator : SY/VA
Sample : M2680-17
Misc : 4.80G/10ML/MSVOA_W/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDC1

Manual Integrations
APPROVED

MMDadoda
6/16/2021 5:02:24 PM

Quant Time: Jun 16 01:02:43 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 16 01:01:36 2021
Response via : Initial Calibration

