

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061521\
 Data File : VW019223.D
 Acq On : 15 Jun 2021 11:41
 Operator : SY/VA
 Sample : M2682-16RE
 Misc : 5.47G/10ML/MSVOA_W/SOIL
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDC0RE

Quant Time: Jun 16 01:02:32 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 16 01:01:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	177699	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	155190	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	57810	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	59413	25.285	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.120%
7) Chloroethane-d5	2.897	69	50214	25.091	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.360%
11) 1,1-Dichloroethene-d2	4.019	63	89336	19.135	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	76.560%
21) 2-Butanone-d5	7.086	46	19783	32.141	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	64.280%
24) Chloroform-d	7.653	84	120314	25.184	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	100.720%
26) 1,2-Dichloroethane-d4	8.311	65	66430	24.789	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.160%
32) Benzene-d6	8.281	84	238832	27.012	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	108.040%
36) 1,2-Dichloropropane-d6	9.274	67	73852	27.552	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	110.200%
41) Toluene-d8	10.323	98	201288	24.789	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	99.160%
43) trans-1,3-Dichloroprop...	10.579	79	25696	22.134	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.520%
47) 2-Hexanone-d5	10.927	63	18420	40.524	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	81.040%
56) 1,1,2,2-Tetrachloroeth...	12.694	84	47488	21.477	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.920%
66) 1,2-Dichlorobenzene-d4	13.853	152	47952	23.765	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.040%
Target Compounds						
					Qvalue	
13) Acetone	4.135	43	2686	4.925	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061521\
Data File : VW019223.D
Acq On : 15 Jun 2021 11:41
Operator : SY/VA
Sample : M2682-16RE
Misc : 5.47G/10ML/MSVOA_W/SOIL
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGDC0RE

Quant Time: Jun 16 01:02:32 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 16 01:01:36 2021
Response via : Initial Calibration

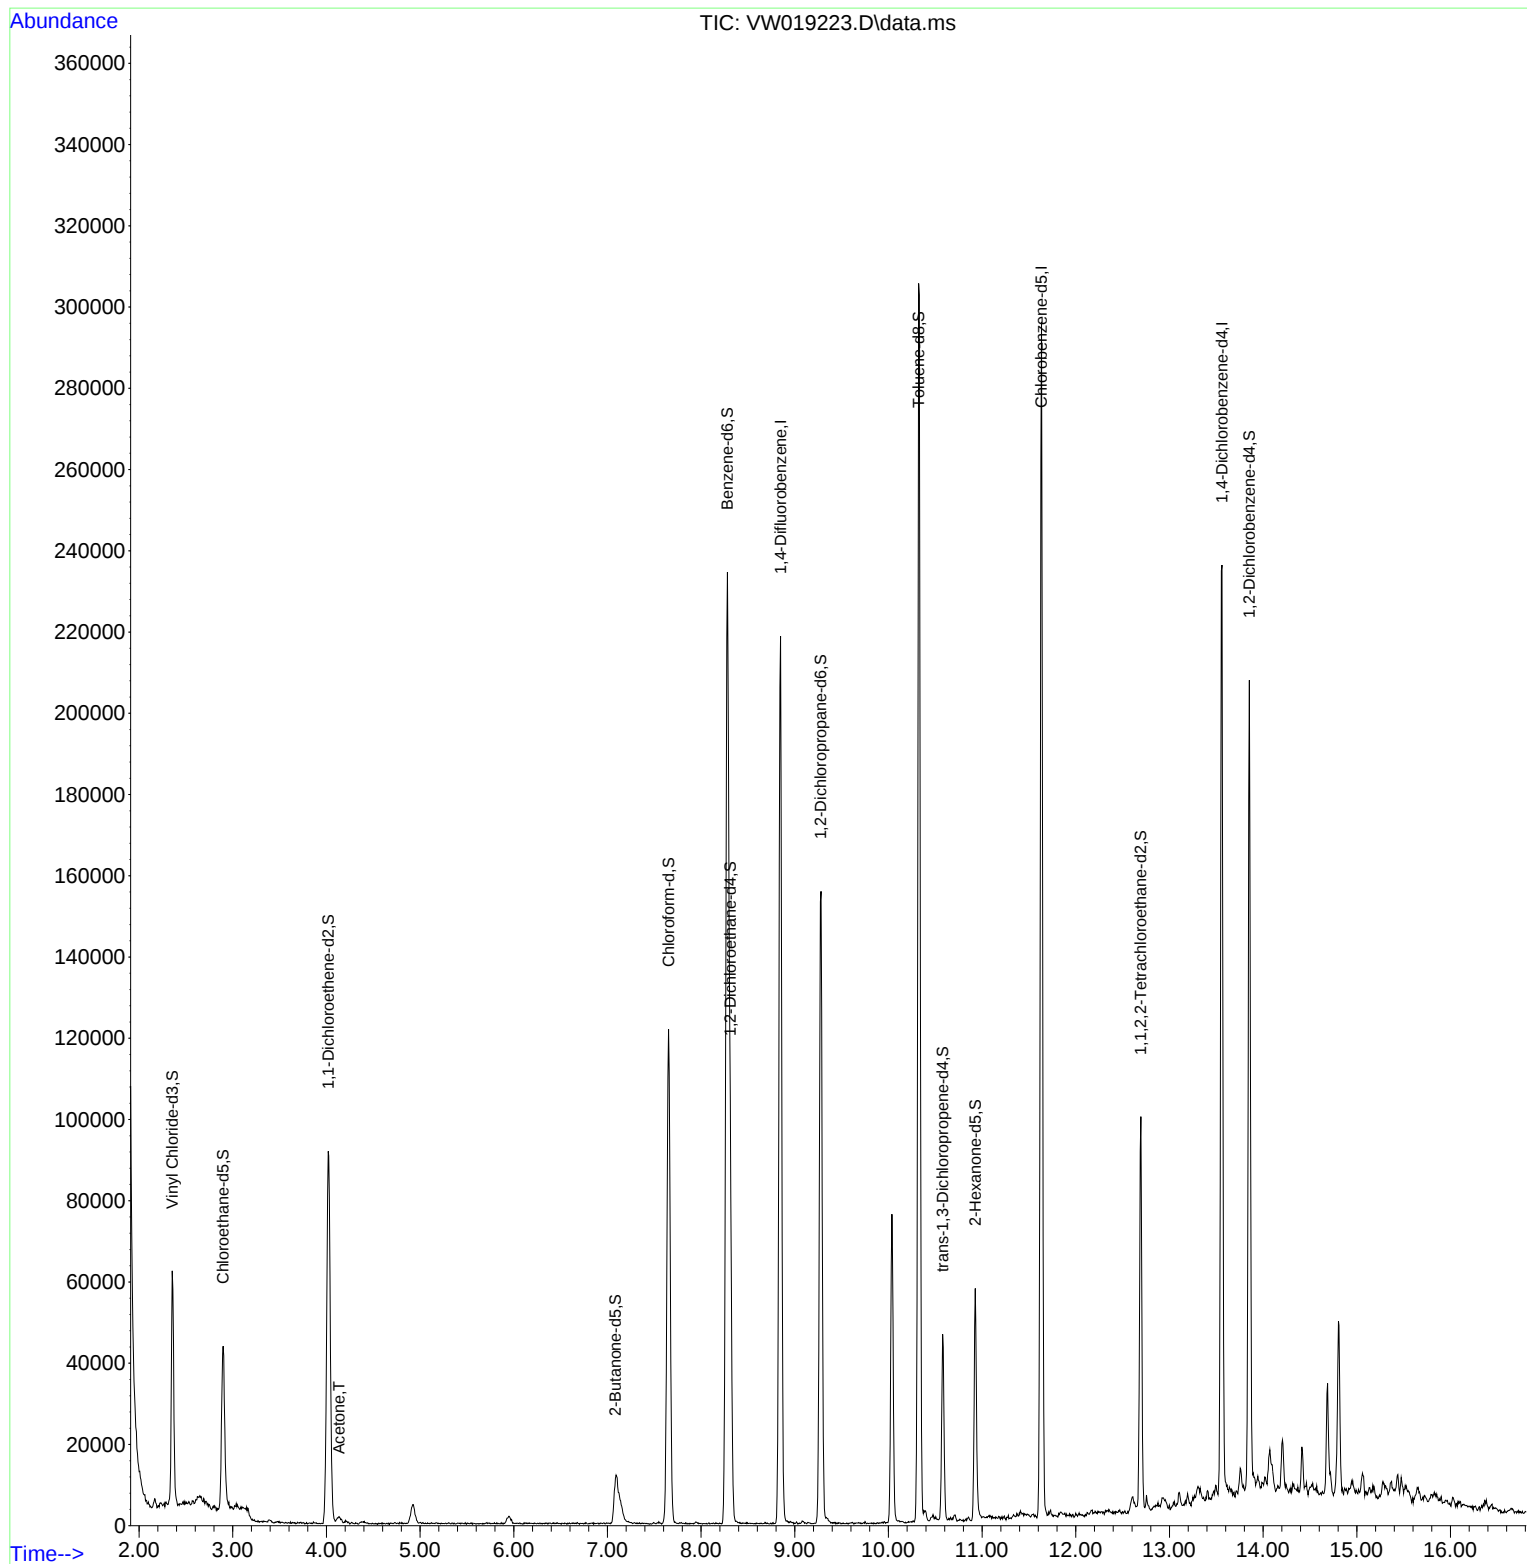

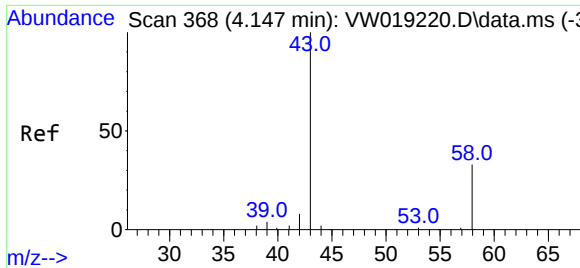

#13
 Acetone
 Concen: 4.925 ug/L
 RT: 4.135 min Scan# 366
 Delta R.T. -0.012 min
 Lab File: VW019223.D
 Acq: 15 Jun 2021 11:41

Instrument :
 MSVOA_W
 ClientSampleId :
 BGDC0RE

Tgt Ion:	43	Resp:	2686
Ion	Ratio	Lower	Upper
43	100		
58	25.7	0.0	53.8

