

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061623\
 Data File : VW026216.D
 Acq On : 16 Jun 2023 09:54
 Operator : SY/MD
 Sample : VW0616SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK519

Quant Time: Jun 16 23:59:39 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 16 23:58:43 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	692763	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	631731	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	284388	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	182673	18.744	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.960%
7) Chloroethane-d5	2.899	69	167928	23.018	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.080%
11) 1,1-Dichloroethene-d2	4.021	65	98932	20.587	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	82.360%
21) 2-Butanone-d5	7.075	46	141694	49.939	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	99.880%
24) Chloroform-d	7.648	84	445955	21.983	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	87.920%
26) 1,2-Dichloroethane-d4	8.307	65	251087	22.635	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	90.520%
32) Benzene-d6	8.276	84	883128	20.775	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	83.120%
36) 1,2-Dichloropropane-d6	9.276	67	297203	22.069	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	88.280%
41) Toluene-d8	10.319	98	745608	19.779	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	79.120%
43) trans-1,3-Dichloroprop...	10.575	79	100767	18.882	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	75.520%
47) 2-Hexanone-d5	10.922	63	91743	43.204	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.400%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	219577	22.406	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.640%
66) 1,2-Dichlorobenzene-d4	13.848	152	243827	22.400	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	89.600%
Target Compounds					Qvalue	
48) 2-Hexanone	10.922	43	12316	2.528	ug/L	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061623\
Data File : VW026216.D
Acq On : 16 Jun 2023 09:54
Operator : SY/MD
Sample : VW0616SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK519


Quant Time: Jun 16 23:59:39 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 16 23:58:43 2023
Response via : Initial Calibration

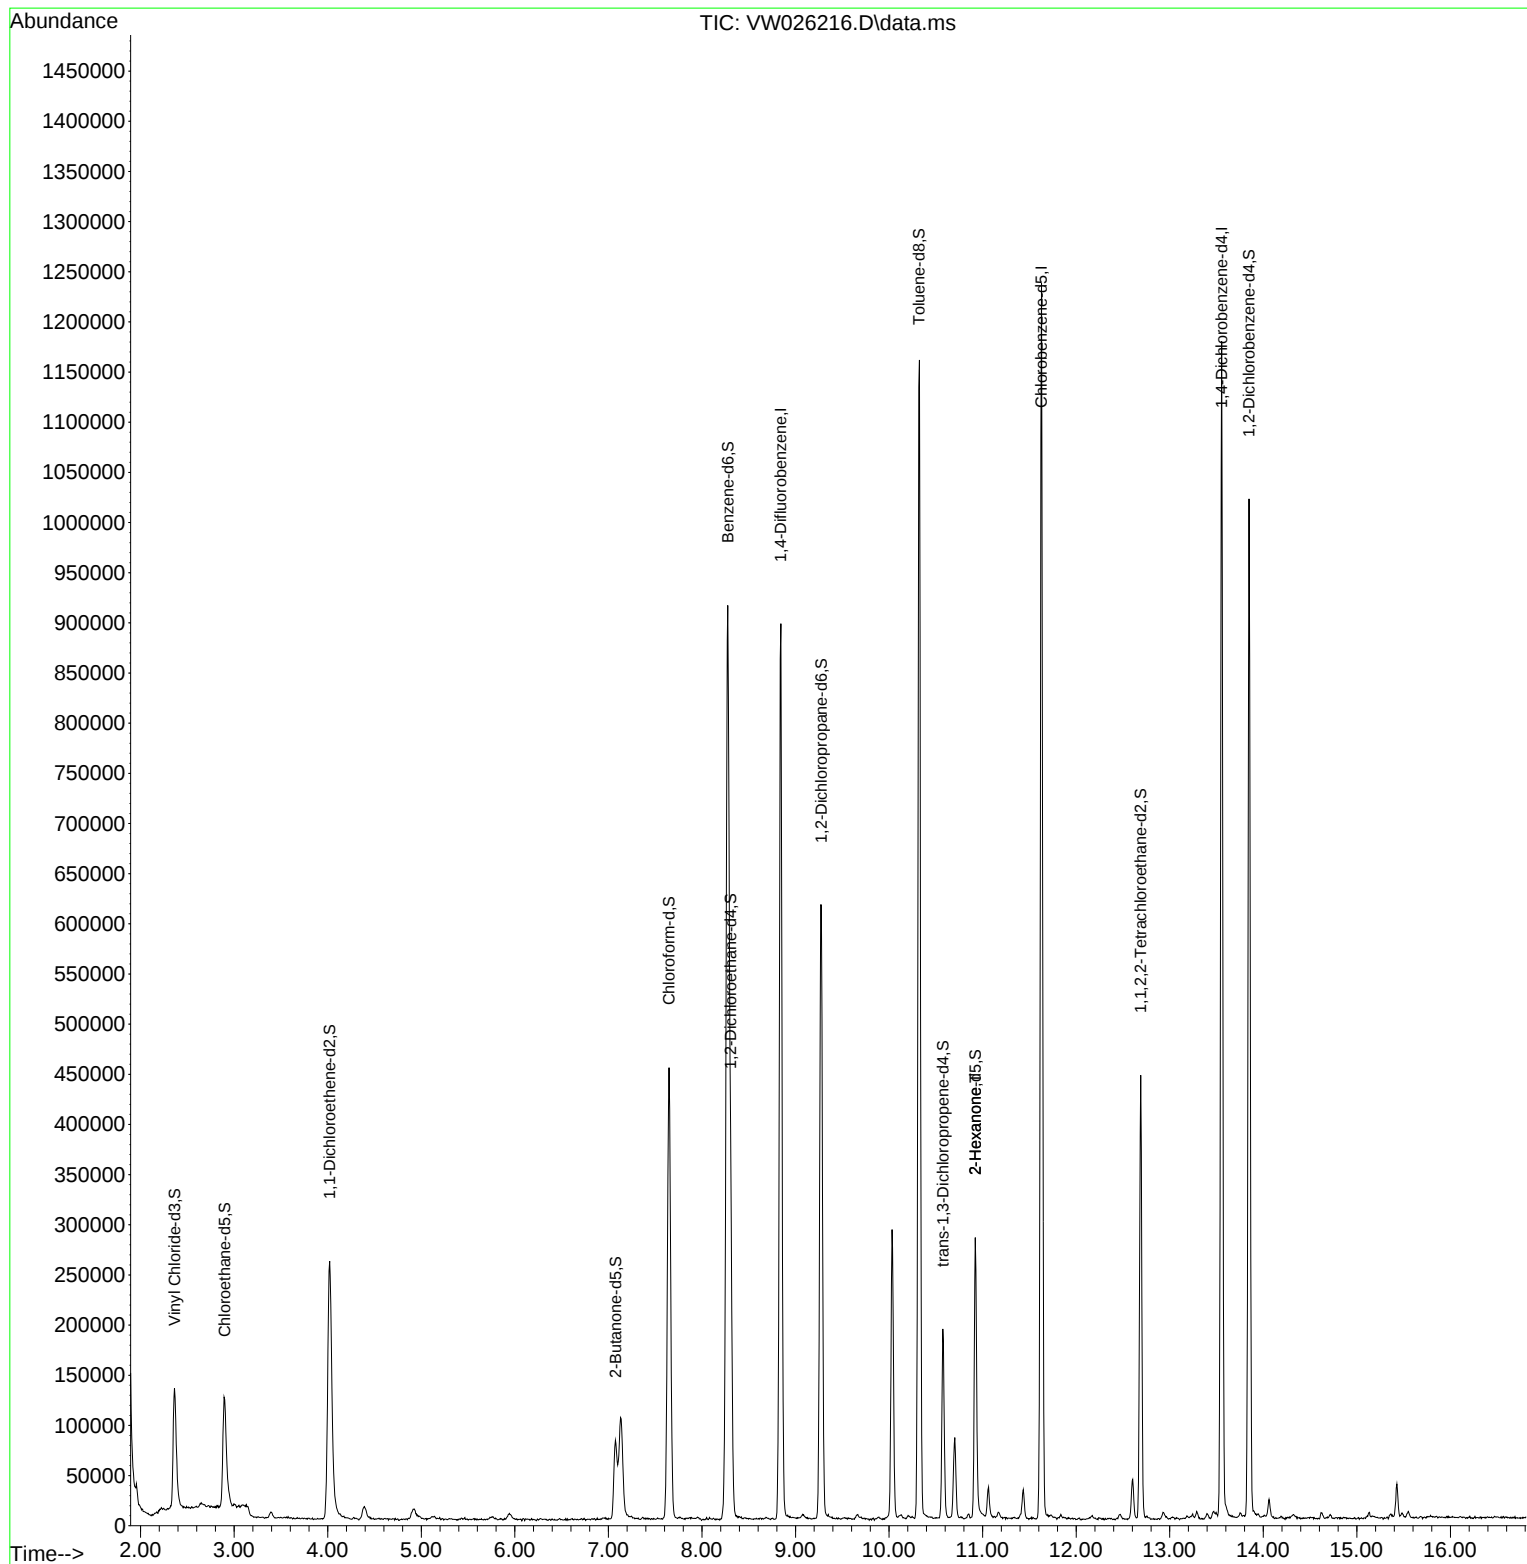

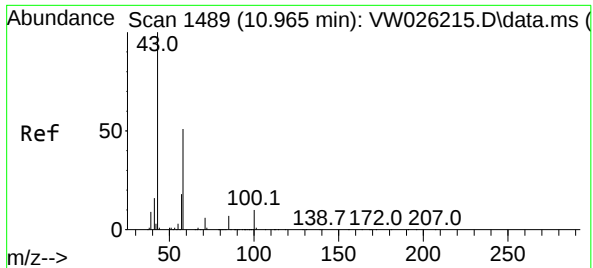

#48
 2-Hexanone
 Concen: 2.528 ug/L
 RT: 10.922 min Scan# 14
 Delta R.T. -0.043 min
 Lab File: VW026216.D
 Acq: 16 Jun 2023 09:54

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK519

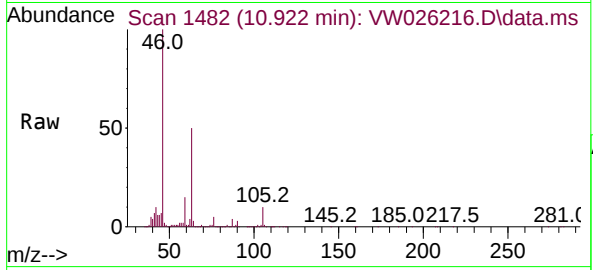

Tgt Ion: 43	Resp: 12316
Ion Ratio	Lower Upper
43 100	
58 30.8	42.2 63.2#
57 33.9	14.2 21.2#
100 2.7	8.3 12.5#

