

Data File : VW010825.D
Acq On : 17 Jun 2019 14:11
Operator : SY/VA
Sample : K3363-06
Misc : 3.62G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 05:52:48 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM061119S.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 18 05:48:46 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	91901	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	44057	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	9349	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	47552	35.53	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	142.12%
7) Chloroethane-d5	2.89	69	46649	45.96	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	183.84%#
10) 1,1-Dichloroethene-d2	4.01	63	65497	23.61	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	94.44%
20) 2-Butanone-d5	7.09	46	34319	65.35	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	130.70%
24) Chloroform-d	7.65	84	61630	32.62	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	130.48%
26) 1,2-Dichloroethane-d4	8.30	65	68786	44.71	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	178.84%#
29) Benzene-d6	8.27	84	116574	44.32	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	177.28%#
33) 1,2-Dichloropropane-d6	9.27	67	70956	84.08	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	336.32%#
37) Toluene-d8	10.32	98	73783	31.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	124.88%
38) trans-1,3-Dichloropropene-	10.58	79	18157	48.05	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	192.20%#
39) 2-Hexanone-d5	10.93	63	31905	158.24	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	316.48%#
48) 1,1,2,2-Tetrachloroethane-	12.69	84	46560	65.14	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	260.56%#
61) 1,2-Dichlorobenzene-d4	13.86	152	7808	21.94	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.76%


Target Compounds


					Qvalue
13) Acetone	4.14	43	4695	8.321 ug/L	65
16) Methylene chloride	4.92	84	9974	7.909 ug/L	98
18) trans-1,2-Dichloroethene	5.42	96	6270	5.262 ug/L	95
22) cis-1,2-Dichloroethene	7.16	96	43612	32.167 ug/L	99
25) Chloroform	7.68	83	42897	15.013 ug/L	99
35) Trichloroethene	9.09	95	842912	1213.801 ug/L	99
42) cis-1,3-Dichloropropene	10.04	75	1436	1.242 ug/L #	74
44) Toluene	10.38	91	1934	0.681 ug/L	91
45) trans-1,3-Dichloropropene	10.58	75	823	0.845 ug/L #	13
47) Tetrachloroethene	10.86	164	2383	4.579 ug/L	91
49) 2-Hexanone	10.93	43	4350	8.086 ug/L #	81
50) Dibromochloromethane	10.87	129	2400	4.028 ug/L #	11
54) m,p-Xylene	11.83	106	852	0.728 ug/L	80

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW010825.D
Acq On : 17 Jun 2019 14:11
Operator : SY/VA
Sample : K3363-06
Misc : 3.62G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jun 18 05:52:48 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM061119S.M
Quant Title : VOC Analysis
QLast Update : Tue Jun 18 05:48:46 2019
Response via : Initial Calibration

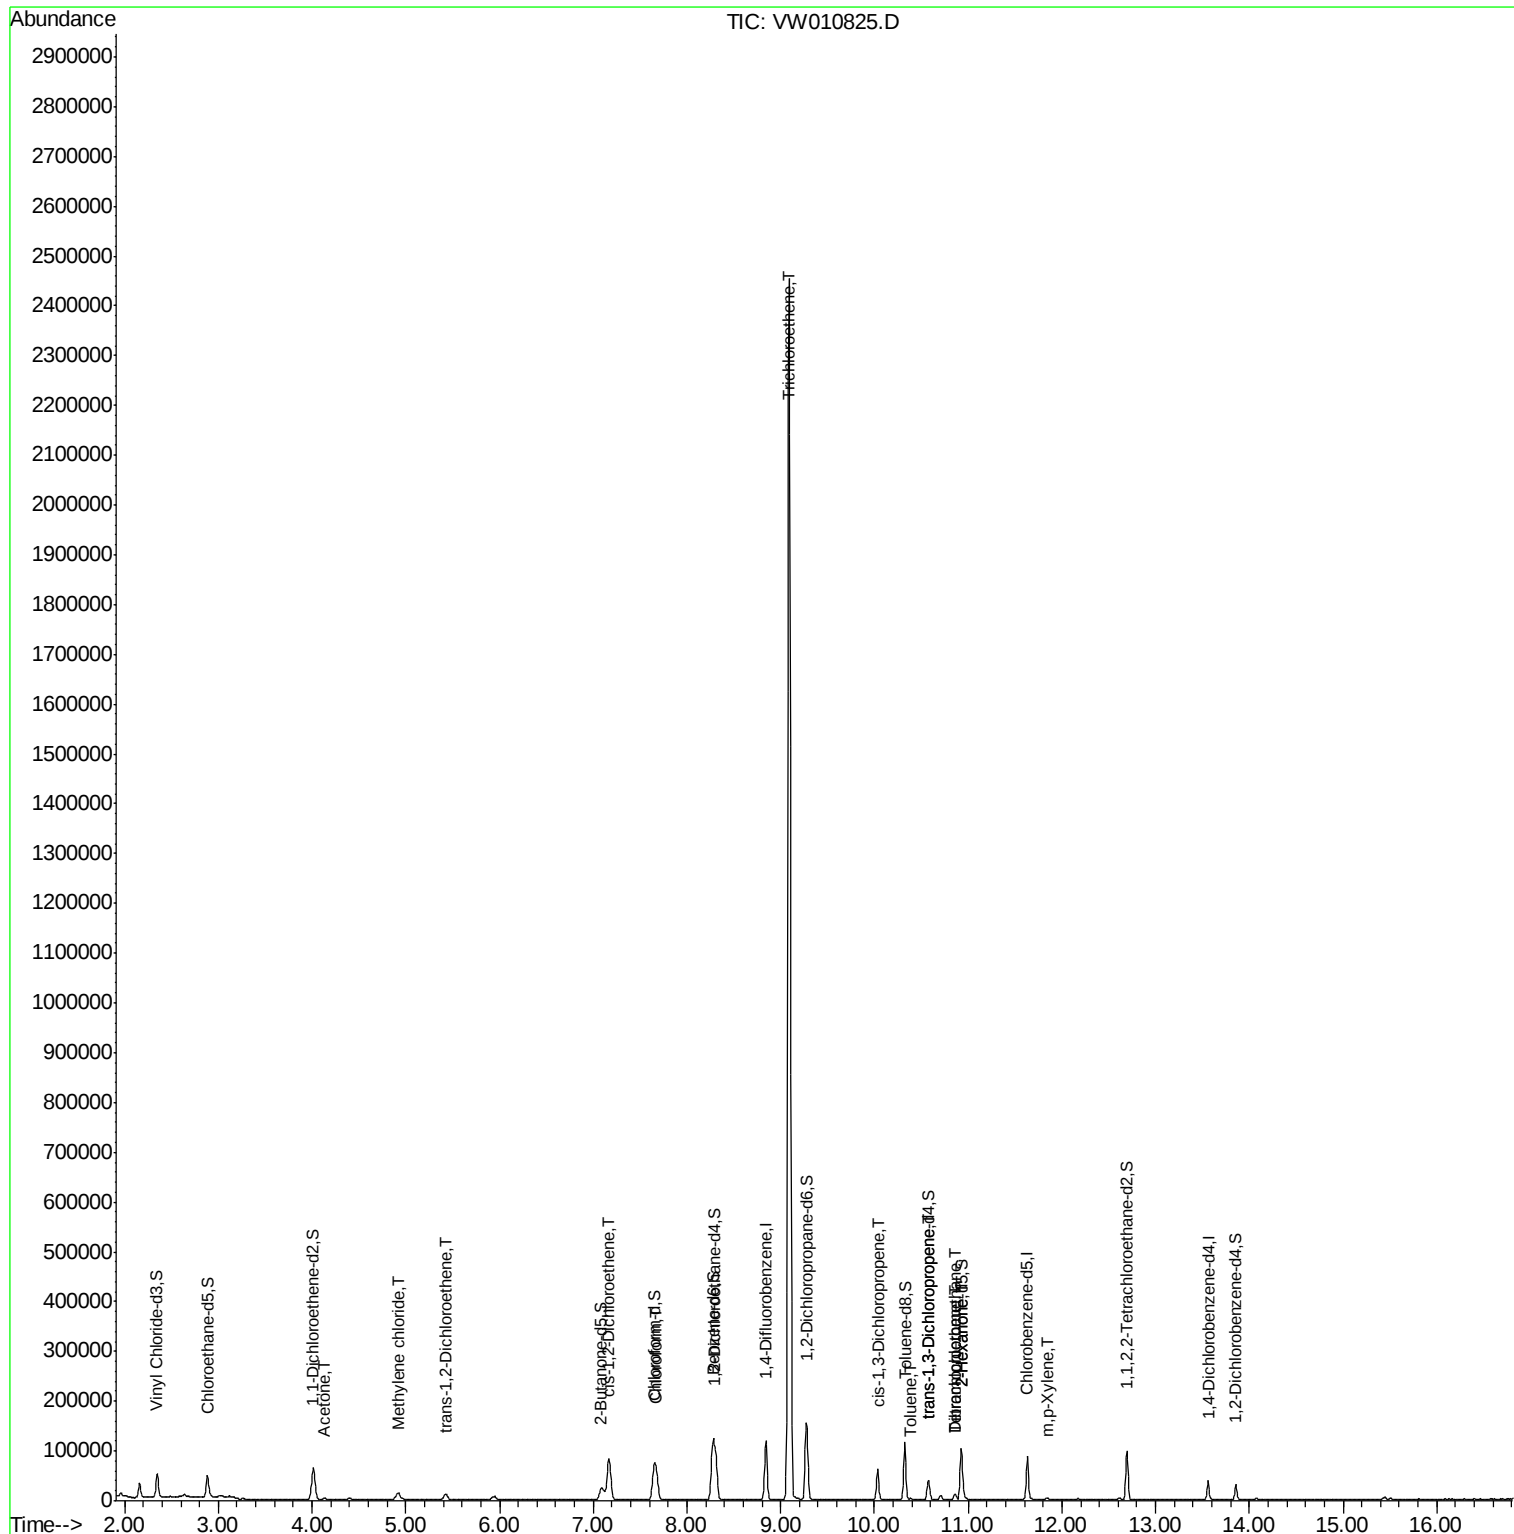

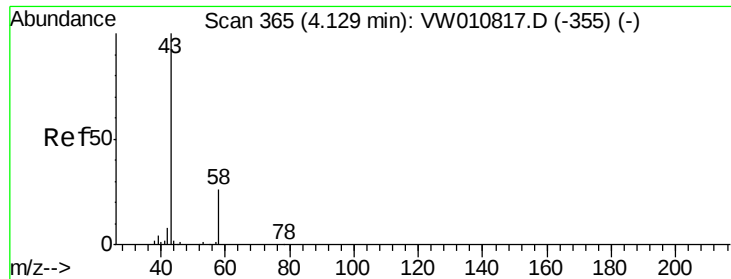

#13

Acetone

Concen: 8.321 ug/L

RT: 4.14 min Scan# 366

Delta R.T. 0.01 min

Lab File: VW010825.D





Acq: 17 Jun 2019 14:11

Tgt Ion: 43 Resp: 4695

Ion Ratio Lower Upper

43 100

58 9.3 0.0 54.6

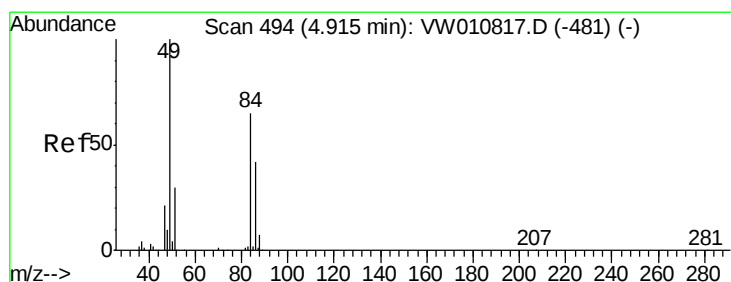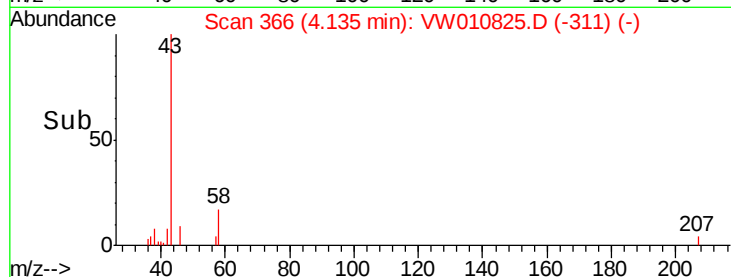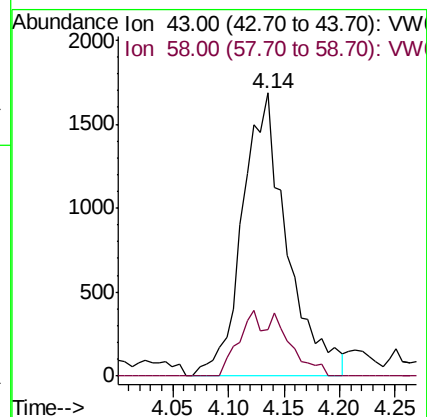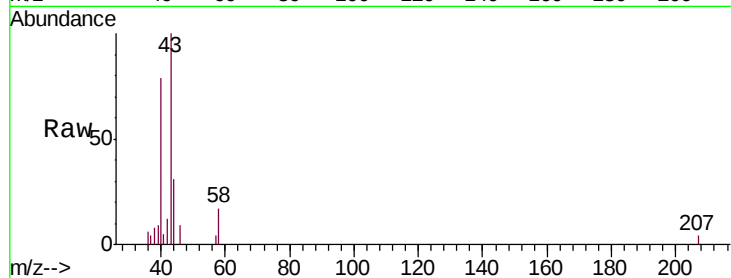

#16

Methylene chloride

Concen: 7.909 ug/L

RT: 4.92 min Scan# 495

Delta R.T. 0.01 min

Lab File: VW010825.D

Acq: 17 Jun 2019 14:11




Tgt Ion: 84 Resp: 9974


Ion Ratio Lower Upper

84 100

49 152.3 105.2 195.4

86 65.9 43.7 81.1

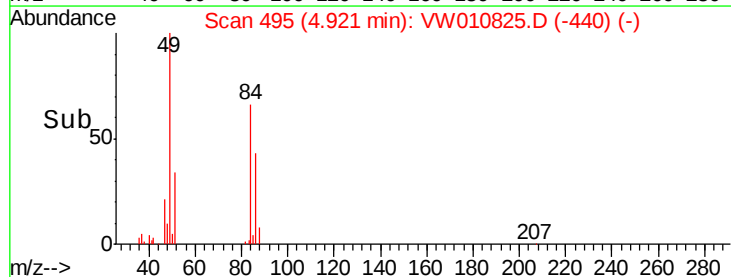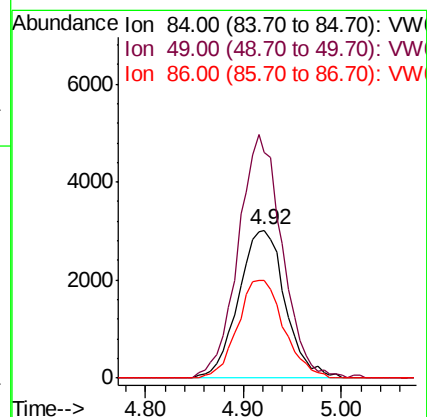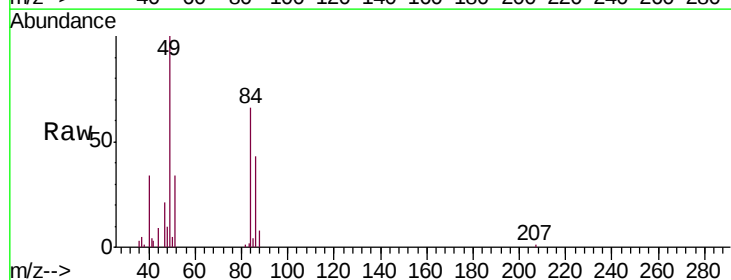

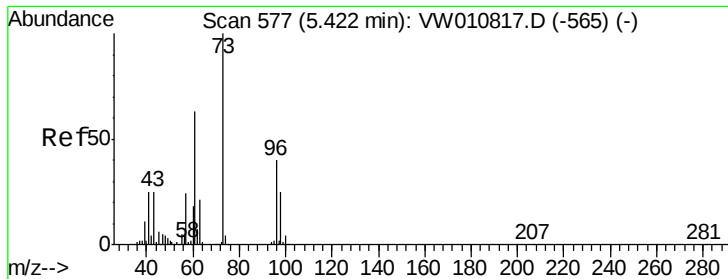

#18

trans-1,2-Dichloroethene

Concen: 5.262 ug/L

RT: 5.42 min Scan# 577

Delta R.T. -0.00 min

Lab File: VW010825.D

Acq: 17 Jun 2019 14:11


Tgt Ion: 96 Resp: 6270

Ion Ratio Lower Upper




96 100

61 165.9 111.5 207.1

98 68.1 44.1 81.9

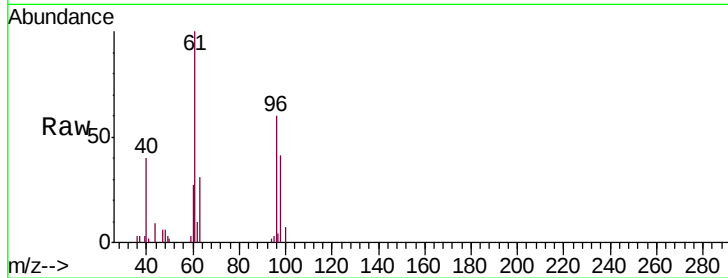

Abundance Ion 96.00 (95.70 to 96.70): VW
Ion 61.00 (60.70 to 61.70): VW
Ion 98.00 (97.70 to 98.70): VW

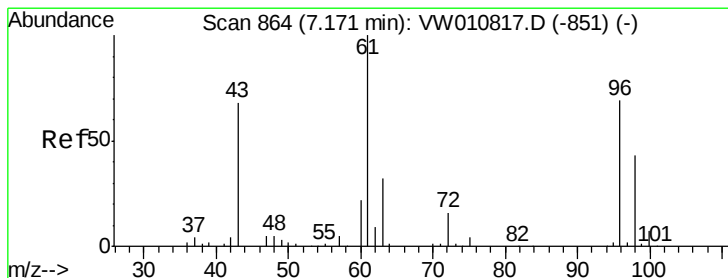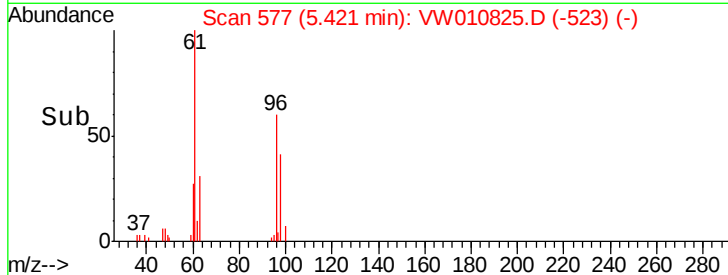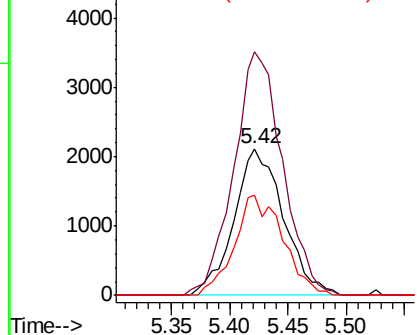

#22

cis-1,2-Dichloroethene

Concen: 32.167 ug/L

RT: 7.16 min Scan# 863

Delta R.T. -0.01 min

Lab File: VW010825.D

Acq: 17 Jun 2019 14:11


Tgt Ion: 96 Resp: 43612

Ion Ratio Lower Upper



96 100


61 149.1 105.3 195.6

98 62.0 44.6 82.8

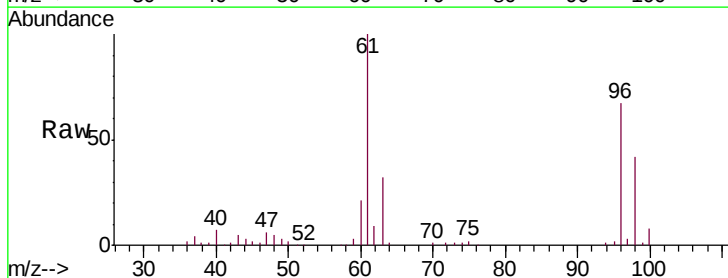

Abundance Ion 96.00 (95.70 to 96.70): VW
Ion 61.00 (60.70 to 61.70): VW
Ion 98.00 (97.70 to 98.70): VW

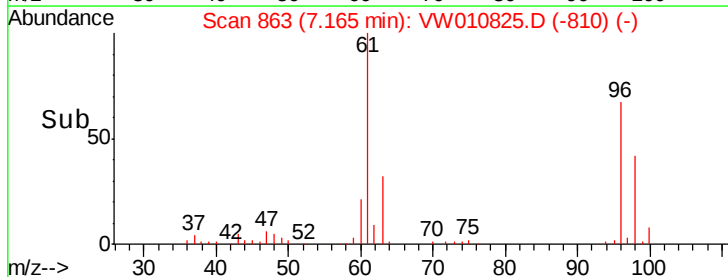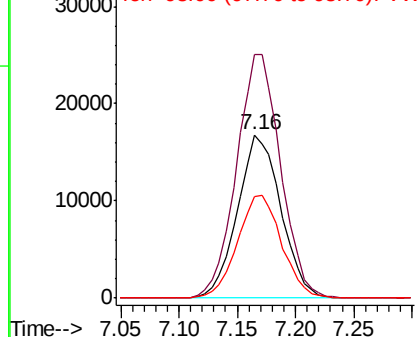

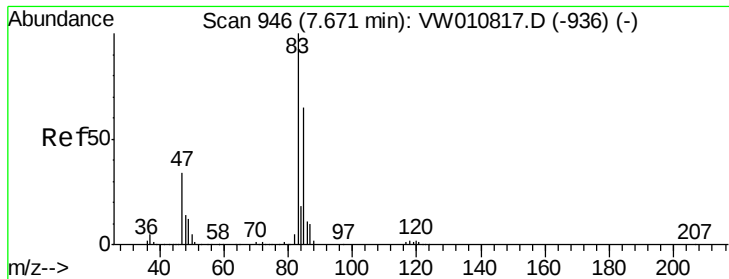

#25

Chloroform

Concen: 15.013 ug/L

RT: 7.68 min Scan# 947

Delta R.T. 0.01 min

Lab File: VW010825.D


Acq: 17 Jun 2019 14:11

Tgt Ion: 83 Resp: 42897

Ion Ratio Lower Upper




83 100

85 65.6 45.4 84.4

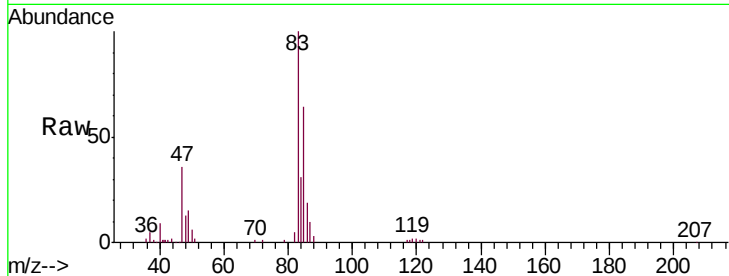

Abundance Ion 83.00 (82.70 to 83.70): VW

Ion 85.00 (84.70 to 85.70): VW

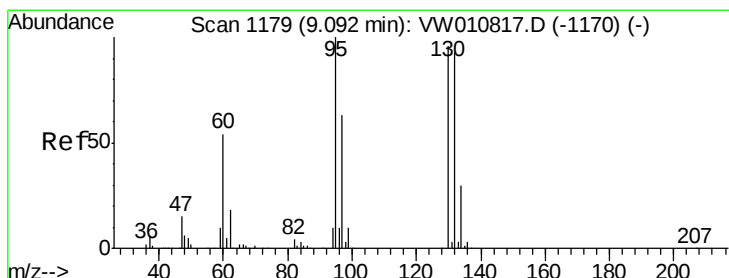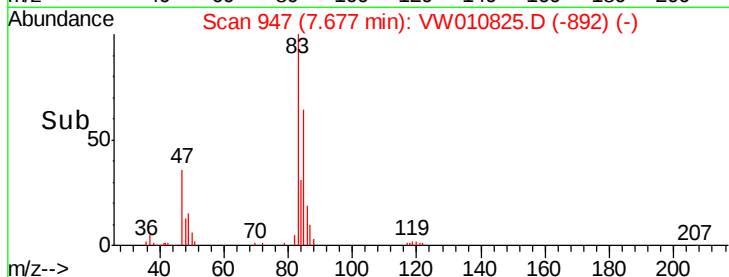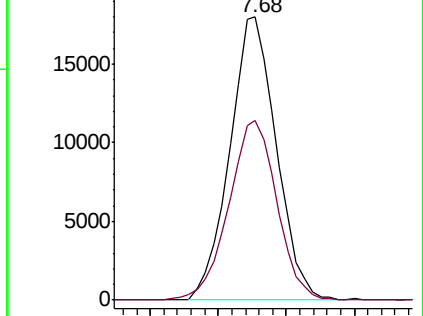

#35

Trichloroethene

Concen: 1213.801 ug/L

RT: 9.09 min Scan# 1179

Delta R.T. -0.00 min

Lab File: VW010825.D

Acq: 17 Jun 2019 14:11

Tgt Ion: 95 Resp: 842912


Ion Ratio Lower Upper

95 100

97 64.5 45.4 84.2

132 92.1 65.0 120.6

130 96.6 68.3 126.9


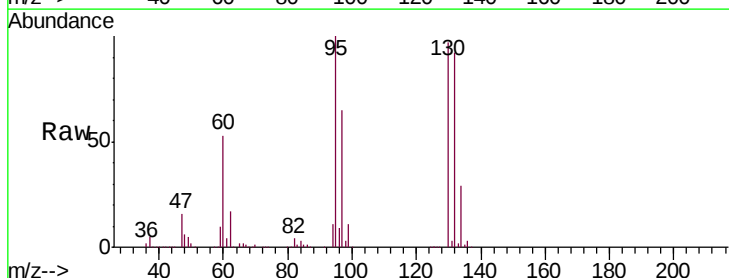



Abundance Ion 95.00 (94.70 to 95.70): VW

Ion 97.00 (96.70 to 97.70): VW

Ion 132.00 (131.70 to 132.70): V





Ion 130.00 (129.70 to 130.70): V

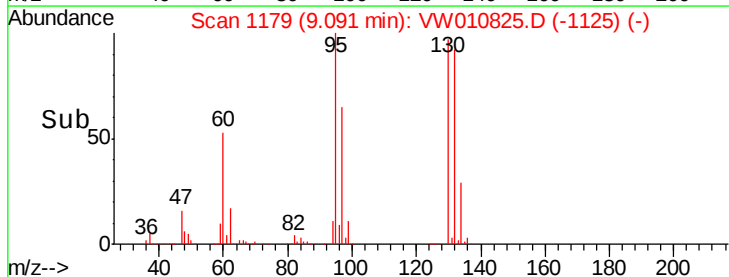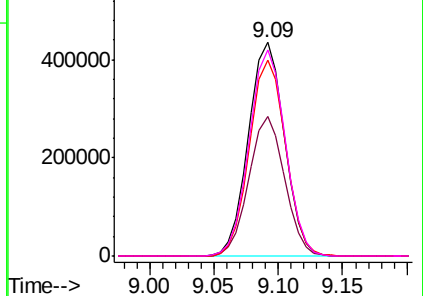

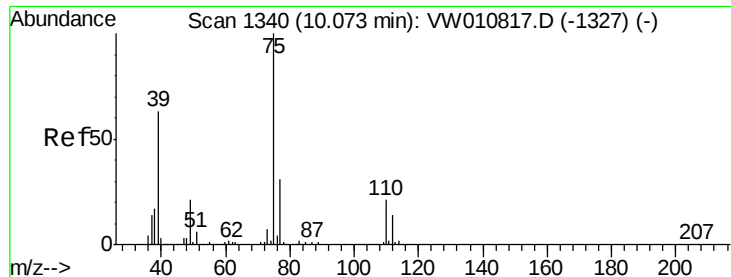




#42
 cis-1,3-Dichloropropene
 Concen: 1.242 ug/L
 RT: 10.04 min Scan# 1334
 Delta R.T. -0.04 min
 Lab File: VW010825.D
 Acq: 17 Jun 2019 14:11


Tgt Ion: 75 Resp: 1436
 Ion Ratio Lower Upper
 75 100
 77 46.0 22.0 41.0#

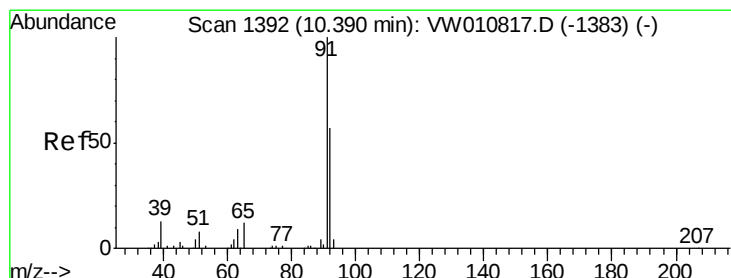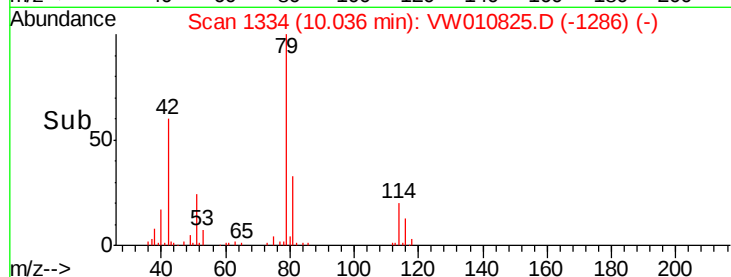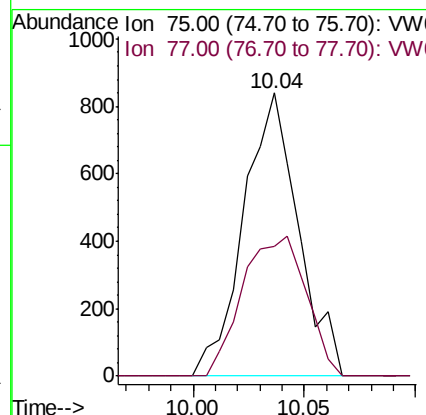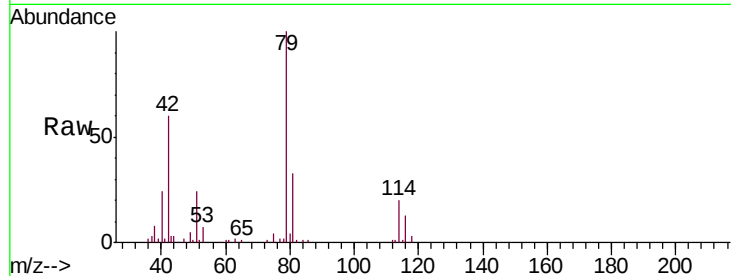

#44
 Toluene
 Concen: 0.681 ug/L
 RT: 10.38 min Scan# 1391
 Delta R.T. -0.01 min
 Lab File: VW010825.D
 Acq: 17 Jun 2019 14:11

Tgt Ion: 91 Resp: 1934
 Ion Ratio Lower Upper
 91 100
 92 52.0 41.0 76.2

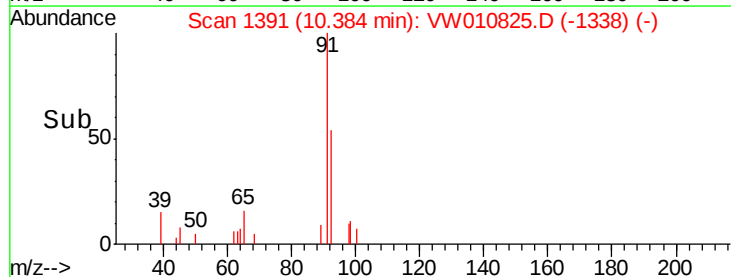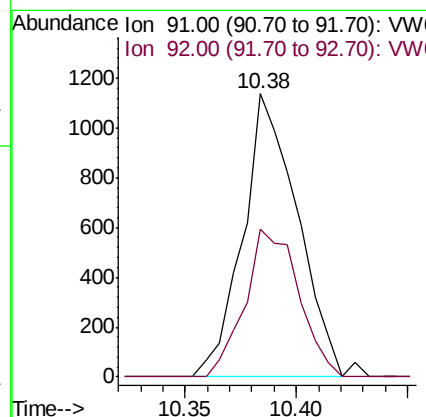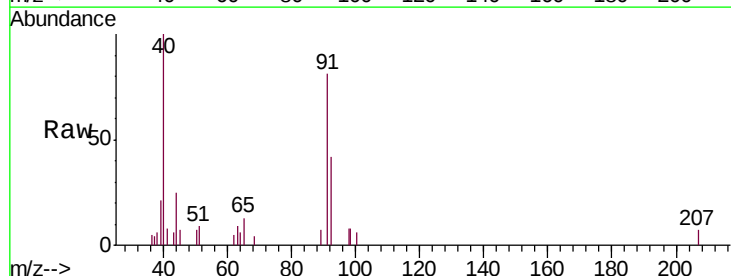

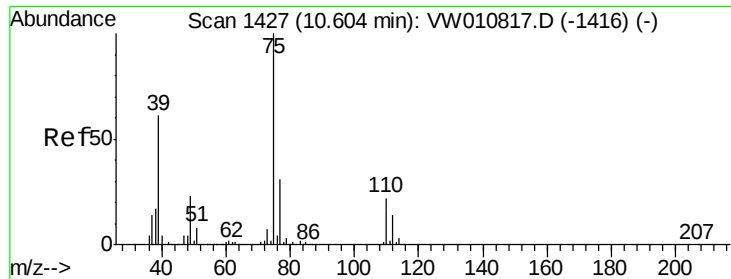

#45

trans-1,3-Dichloropropene

Concen: 0.845 ug/L

RT: 10.58 min Scan# 1423

Delta R.T. -0.02 min

Lab File: VW010825.D





Acq: 17 Jun 2019 14:11

Tgt Ion: 75 Resp: 823

Ion Ratio Lower Upper

75 100

77 80.6 22.5 41.7#

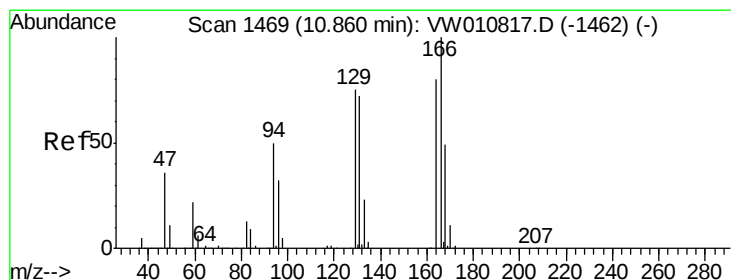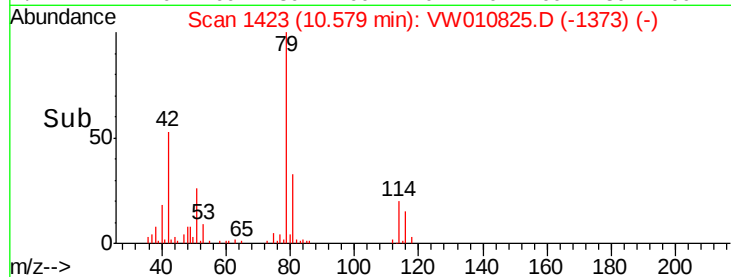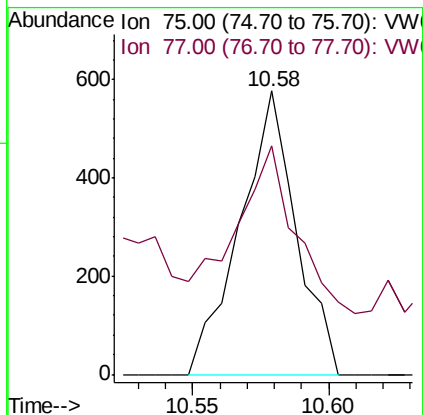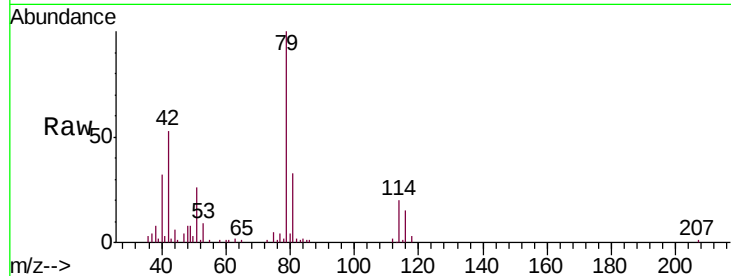

#47

Tetrachloroethene

Concen: 4.579 ug/L

RT: 10.86 min Scan# 1469

Delta R.T. -0.00 min

Lab File: VW010825.D

Acq: 17 Jun 2019 14:11

Tgt Ion: 164 Resp: 2383




Ion Ratio Lower Upper


164 100

129 93.3 64.5 119.7

131 77.3 63.6 118.0





166 110.6 85.8 159.3

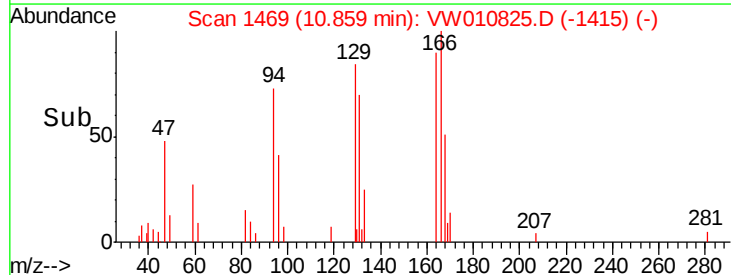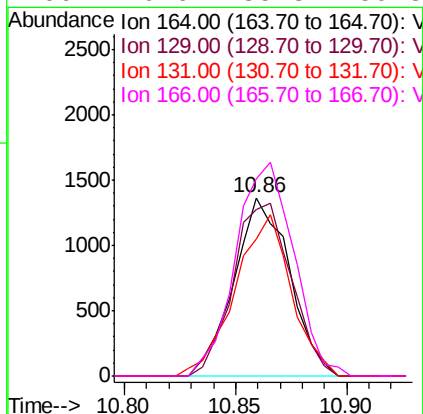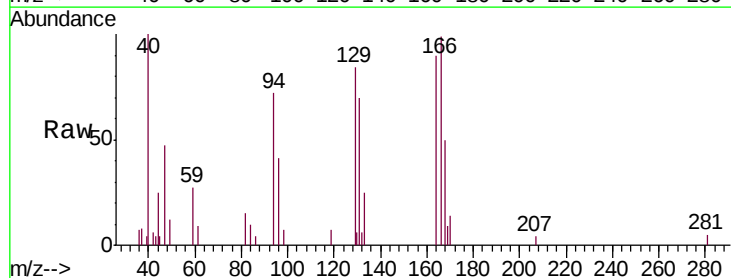

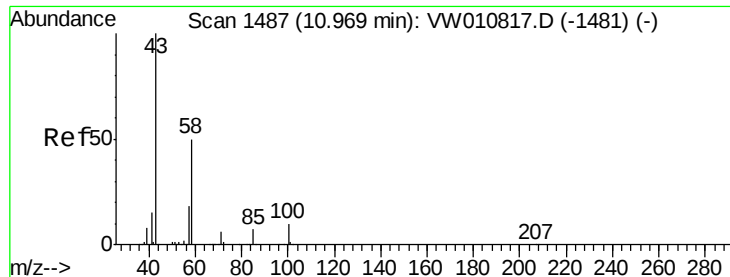




#49
2-Hexanone
Concen: 8.086 ug/L
RT: 10.93 min Scan# 1480
Delta R.T. -0.04 min
Lab File: VW010825.D
Acq: 17 Jun 2019 14:11


Tgt Ion: 43 Resp: 4350
Ion Ratio Lower Upper
43 100
58 36.5 39.5 59.3#
57 24.3 13.8 20.8#
100 0.0 7.6 11.4#

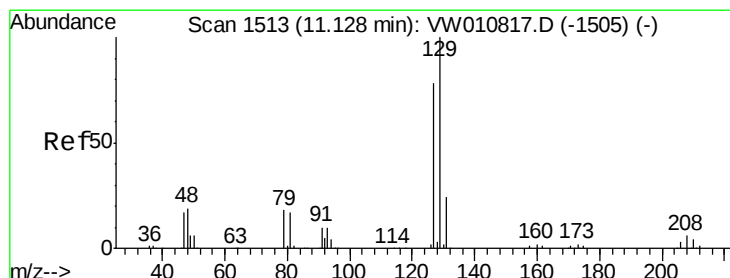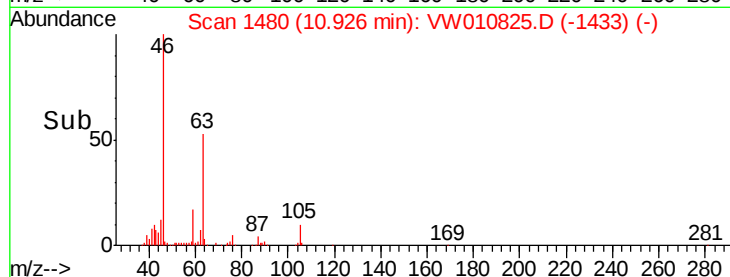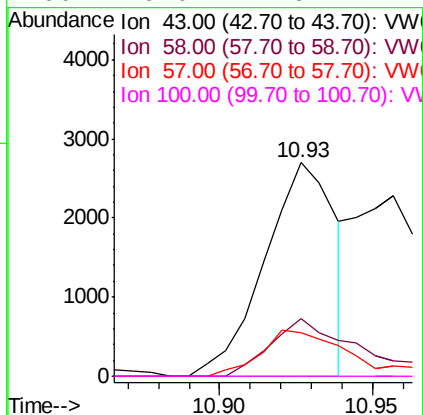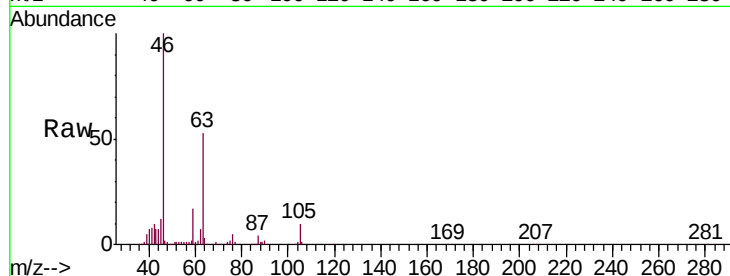

#50
Dibromochloromethane
Concen: 4.028 ug/L
RT: 10.87 min Scan# 1470
Delta R.T. -0.26 min
Lab File: VW010825.D
Acq: 17 Jun 2019 14:11


Tgt Ion: 129 Resp: 2400
Ion Ratio Lower Upper
129 100
127 0.0 53.1 98.7#

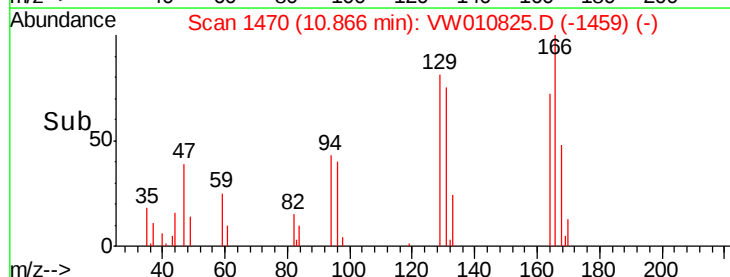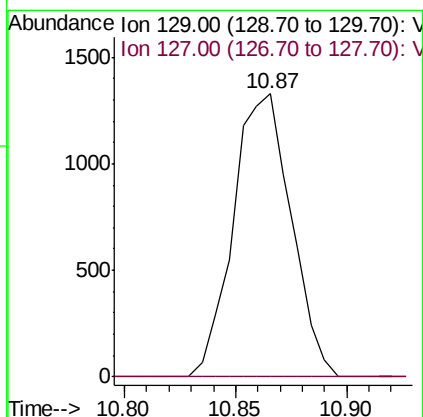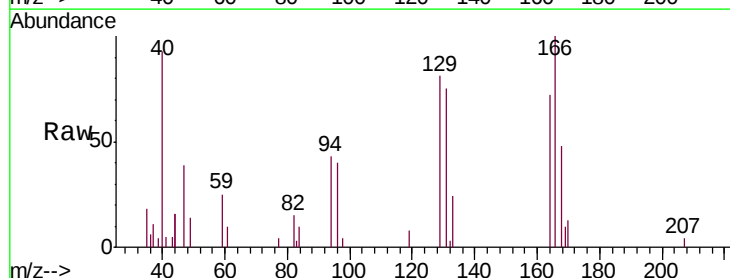

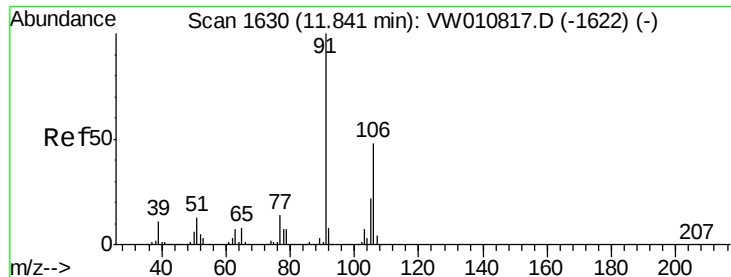

#54
 m,p-Xylene
 Concen: 0.728 ug/L
 RT: 11.83 min Scan# 1629
 Delta R.T. -0.01 min
 Lab File: VW010825.D
 Acq: 17 Jun 2019 14:11

Tgt Ion:106 Resp: 852
 Ion Ratio Lower Upper
 106 100
 91 180.4 148.7 276.1

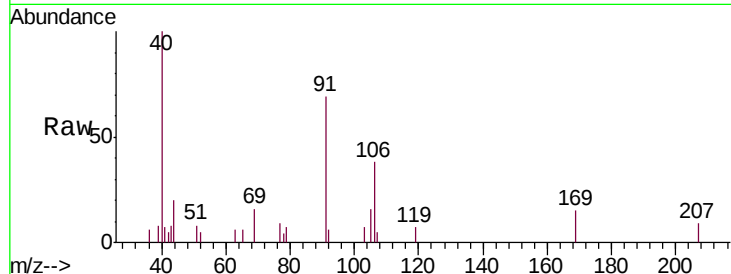

Abundance Ion 106.00 (105.70 to 106.70): V
 Ion 91.00 (90.70 to 91.70): VW

