


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW061720\
 Data File : VW015613.D
 Acq On : 17 Jun 2020 09:09
 Operator : SY/VA
 Sample : BFB11
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB11

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM052620S.M
 Title : VOC Analysis
 Last Update : Thu Jun 18 07:15:54 2020

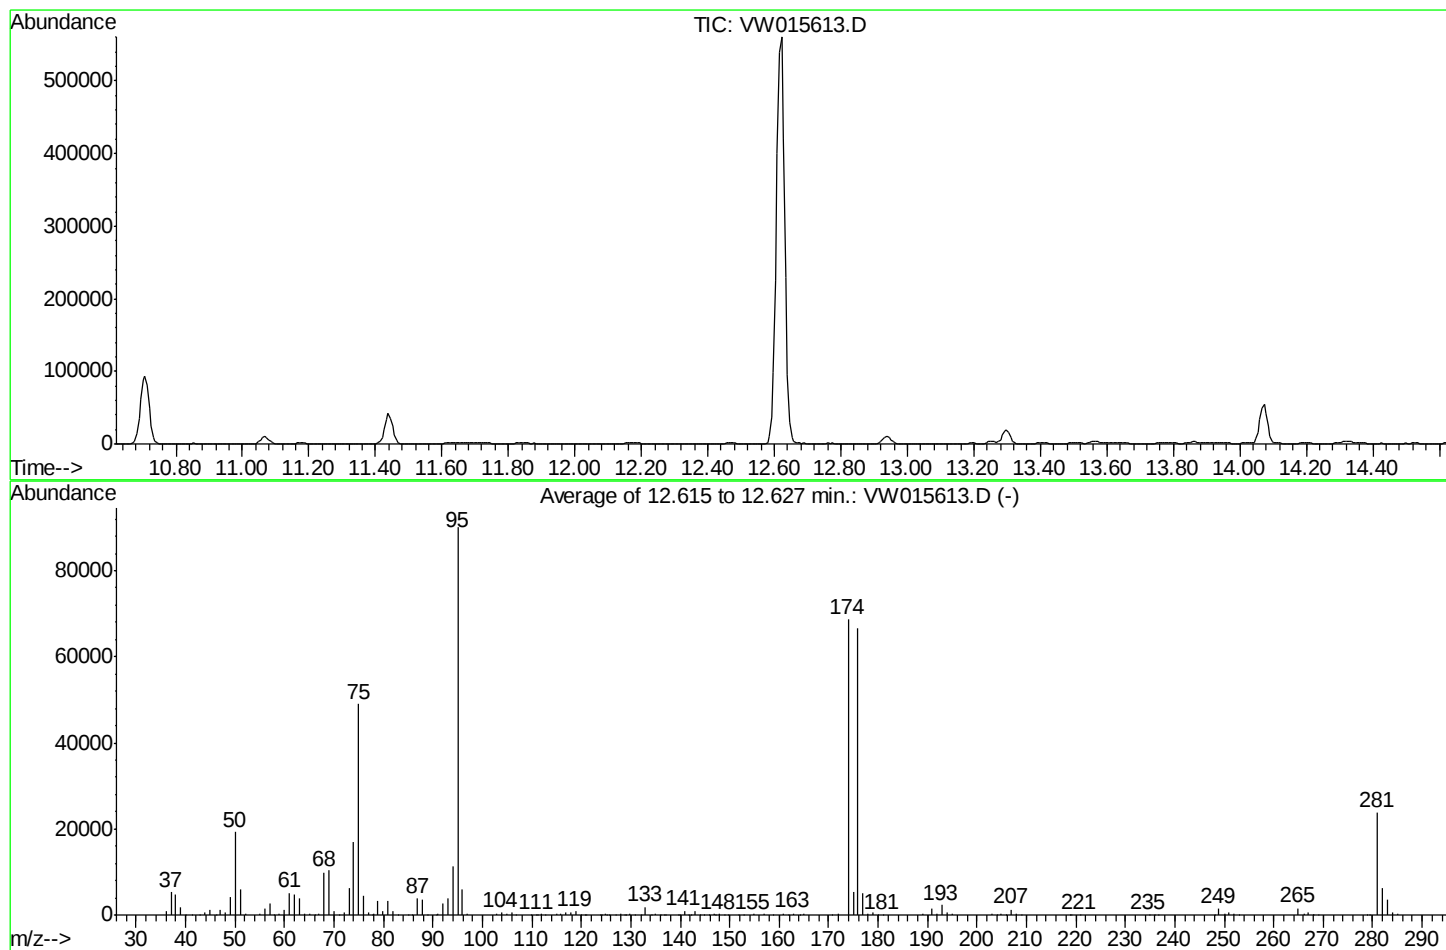

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.4	19237	PASS
75	95	30	80	54.4	48970	PASS
95	95	100	100	100.0	90072	PASS
96	95	5	9	6.6	5943	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	76.2	68664	PASS
175	174	5	9	7.9	5447	PASS
176	174	95	101	97.2	66712	PASS
177	176	5	9	7.5	5026	PASS

m/z	Abundance
36.10	982.0
37.00	5651.0
38.00	5349.0
39.00	1982.0
40.00	169.0
41.20	52.0
42.90	210.0
44.00	1007.0
45.00	1526.0
46.00	180.0
47.00	1100.0
47.90	701.0
49.00	4641.0
50.00	20664.0
51.00	6043.0
52.00	293.0
55.00	350.0
56.00	1865.0
57.00	3205.0
57.90	135.0
59.00	550.0
60.00	1048.0
61.00	5159.0
62.00	5053.0
63.00	4008.0
64.00	398.0
64.90	256.0
66.00	55.0
67.10	300.0
68.00	10189.0
69.00	10710.0
69.90	908.0
72.00	453.0
73.00	7621.0
74.00	17928.0
75.00	51136.0
76.00	4767.0
76.90	673.0
78.10	356.0
78.90	3417.0
79.90	1039.0
80.90	3568.0
81.90	719.0
82.90	149.0
84.90	68.0
85.80	153.0
86.90	3796.0
87.90	3928.0
90.80	424.0
92.00	2812.0
93.00	4293.0
94.00	11653.0
95.00	92360.0
96.00	6699.0
97.10	182.0
102.90	624.0
103.90	674.0
104.90	294.0
105.80	443.0
106.90	110.0
109.80	213.0
110.90	255.0
112.00	192.0
112.70	144.0
115.00	335.0
115.90	370.0
116.80	676.0
117.90	689.0
118.80	1021.0
119.90	116.0
120.80	113.0
123.70	84.0
124.90	908.0
125.60	330.0
127.90	349.0
128.80	187.0
129.80	405.0
130.90	142.0
132.00	132.0
133.00	2971.0
134.20	360.0
134.90	400.0
135.90	67.0
136.80	121.0
139.70	86.0
140.90	898.0
141.80	105.0
142.90	816.0
144.80	128.0
145.90	177.0
146.80	503.0
147.90	292.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

148.90	202.0
149.90	79.0
154.80	234.0
156.80	147.0
158.80	141.0
161.00	306.0
161.80	70.0
162.90	515.0
164.10	59.0
164.90	330.0
170.70	69.0
171.90	410.0
173.90	60032.0
174.90	5457.0
175.90	60352.0
176.90	5322.0
177.80	409.0
179.00	816.0
180.00	143.0
180.90	111.0
188.90	308.0
191.00	2512.0
191.90	725.0
192.90	3736.0
194.00	813.0
194.90	377.0
203.00	290.0
204.00	59.0
204.90	666.0
206.00	199.0
206.90	2106.0
207.90	348.0
208.90	224.0
218.80	73.0
220.80	136.0
234.90	251.0
235.90	112.0
236.80	52.0
248.00	93.0
248.90	2117.0
250.00	484.0
250.90	1151.0
252.00	239.0
253.00	103.0
265.00	2550.0
266.10	654.0
267.00	710.0
267.90	155.0
268.90	74.0
279.30	362.0
281.00	37840.0
282.00	9826.0
283.00	5439.0
283.90	999.0
285.00	255.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

m/z	Abundance
36.00	1143.0
37.00	6153.0
38.00	5042.0
39.00	1813.0
40.00	197.0
42.90	161.0
44.00	847.0
45.00	1240.0
46.10	152.0
46.90	1338.0
48.00	734.0
49.00	4687.0
50.00	21056.0
51.00	6763.0
52.10	292.0
54.90	333.0
56.00	1727.0
57.00	3080.0
57.90	103.0
58.90	263.0
60.00	1215.0
61.00	5863.0
62.00	5819.0
63.00	4222.0
64.00	370.0
65.00	208.0
66.90	312.0
68.00	11627.0
69.00	11711.0
70.00	1018.0
72.00	619.0
73.00	6711.0
74.00	19168.0
75.00	55008.0
76.00	4751.0
77.00	651.0
78.00	341.0
78.90	3802.0
79.90	1091.0
80.90	3761.0
81.90	971.0
83.00	115.0
85.90	140.0
86.90	4199.0
87.90	3769.0
88.80	77.0
91.00	510.0
92.00	2873.0
93.00	4532.0
94.00	12866.0
95.00	100192.0
96.00	6422.0
96.90	262.0
102.90	291.0
103.90	547.0
104.90	243.0
105.80	461.0
106.80	73.0
109.80	168.0
111.10	151.0
112.00	221.0
112.80	157.0
114.90	277.0
115.90	367.0
116.90	772.0
117.90	652.0
118.90	725.0
121.00	63.0
124.00	72.0
125.20	428.0
127.00	57.0
127.90	407.0
129.00	212.0
129.80	388.0
130.80	149.0
133.00	1774.0
134.80	293.0
136.70	177.0
139.90	129.0
140.80	1066.0
141.80	110.0
142.90	1056.0
144.00	61.0
144.90	139.0
145.90	136.0
146.80	339.0
147.90	229.0
148.80	161.0
149.80	78.0
152.90	70.0
154.90	172.0
156.80	231.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

158.90	70.0
161.00	276.0
162.90	349.0
164.90	200.0
170.80	101.0
171.90	436.0
173.90	77824.0
175.00	5961.0
175.90	76904.0
176.90	5684.0
177.90	315.0
179.00	521.0
179.90	56.0
180.90	53.0
189.00	201.0
190.90	1380.0
191.80	383.0
192.90	2314.0
193.90	506.0
195.00	214.0
203.10	189.0
205.00	386.0
205.80	100.0
207.00	1188.0
208.00	264.0
209.00	129.0
219.00	60.0
220.70	53.0
234.80	208.0
235.90	73.0
236.70	60.0
247.90	57.0
249.00	1497.0
250.00	419.0
250.90	574.0
251.90	163.0
253.00	54.0
264.90	1601.0
266.00	505.0
266.90	600.0
268.10	91.0
279.00	202.0
281.10	22448.0
282.00	5921.0
283.00	3729.0
283.90	730.0
284.90	190.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

m/z	Abundance
35.90	718.0
37.00	4252.0
38.00	3742.0
39.00	1487.0
40.00	140.0
41.10	74.0
42.90	94.0
43.90	661.0
45.00	859.0
46.00	142.0
46.90	807.0
48.00	517.0
49.00	3618.0
50.00	15993.0
51.00	4839.0
52.10	158.0
54.90	240.0
56.00	1295.0
57.00	2312.0
57.90	84.0
59.00	120.0
60.00	895.0
61.00	4300.0
62.00	3800.0
63.00	3169.0
64.00	385.0
64.90	160.0
66.90	207.0
68.00	7865.0
69.00	8778.0
70.00	778.0
71.10	77.0
72.00	435.0
73.00	4565.0
74.00	14211.0
75.00	40768.0
76.00	3702.0
77.00	436.0
77.80	301.0
78.90	2628.0
79.90	681.0
80.90	2735.0
81.90	617.0
83.00	84.0
85.70	73.0
86.90	3216.0
87.90	3012.0
88.80	119.0
90.90	353.0
92.00	2363.0
93.00	3132.0
94.00	9515.0
95.00	77664.0
96.00	4914.0
96.90	168.0
102.90	176.0
103.90	416.0
104.80	142.0
105.90	487.0
106.80	111.0
109.70	90.0
110.90	182.0
112.00	69.0
112.80	62.0
114.90	147.0
115.90	327.0
116.80	648.0
117.90	364.0
118.90	552.0
124.00	83.0
125.00	321.0
125.60	99.0
127.90	322.0
128.90	162.0
129.80	244.0
130.90	107.0
133.00	735.0
134.00	111.0
134.80	234.0
137.00	146.0
140.00	99.0
140.90	971.0
142.10	101.0
142.90	954.0
144.10	58.0
144.90	133.0
145.90	150.0
146.80	130.0
147.10	128.0
147.80	225.0
149.00	114.0
149.70	61.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

151.80	92.0
154.90	255.0
156.90	157.0
158.80	117.0
160.80	178.0
162.90	149.0
164.90	161.0
170.70	81.0
171.80	402.0
173.90	68136.0
174.90	4923.0
175.90	62880.0
176.90	4073.0
177.90	133.0
178.80	192.0
188.90	83.0
191.00	663.0
192.90	929.0
194.00	179.0
194.90	149.0
203.10	130.0
204.80	197.0
206.90	568.0
207.90	118.0
208.80	65.0
248.90	730.0
249.90	199.0
250.90	302.0
252.10	97.0
265.00	707.0
265.90	185.0
266.90	187.0
267.80	54.0
268.10	71.0
278.80	82.0
281.00	11165.0
281.90	2986.0
283.00	1678.0
283.90	329.0
285.00	105.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11

Scan 1750 (12.573 min): VW015613.D
BFB11

m/z	Abundance
39.90	147.0
43.00	56.0
44.00	271.0
57.00	71.0
73.10	65.0
95.90	68.0
280.90	71.0

Instrument :
MSVOA_W
ClientSampleId :
BFB11