

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061721\
 Data File : VW019236.D
 Acq On : 17 Jun 2021 12:17
 Operator : SY/VA
 Sample : VW0617SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK109

Manual Integrations
 APPROVED

MMDadoda
 6/18/2021 2:35:09 PM

Quant Time: Jun 18 01:03:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 18 01:02:36 2021
 Response via : Initial Calibration

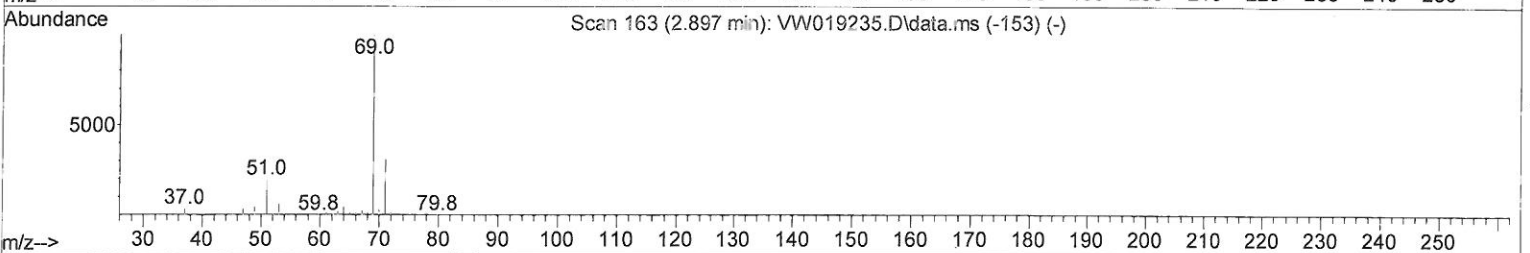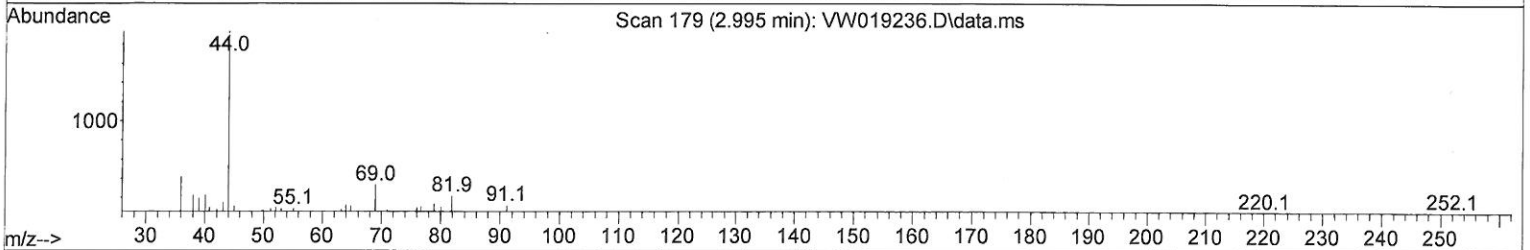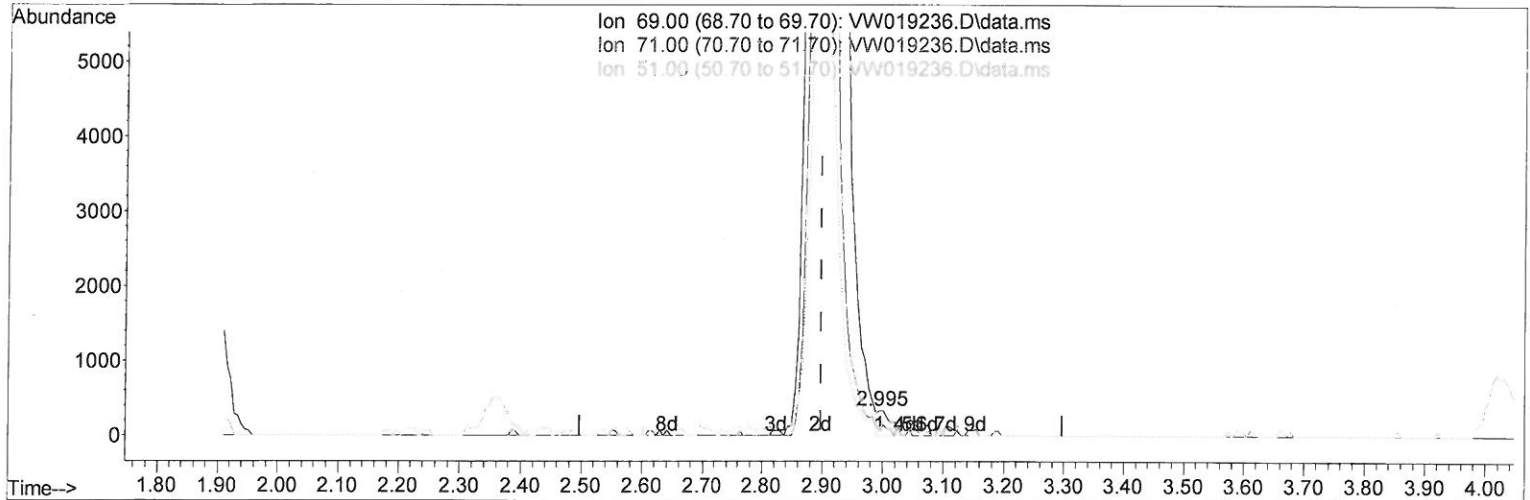

TIC: VW019236.D\data.ms

(7) Chloroethane-d5 (S)

2.995min (+ 0.098) 0.09 ug/L

response 500

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	22.60
51.00	28.40	33.80
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061721\
 Data File : VW019236.D
 Acq On : 17 Jun 2021 12:17
 Operator : SY/VA
 Sample : VW0617SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK109

Manual Integrations
 APPROVED

MMDadoda
 6/18/2021 2:35:09 PM

Quant Time: Jun 18 01:03:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 18 01:02:36 2021
 Response via : Initial Calibration

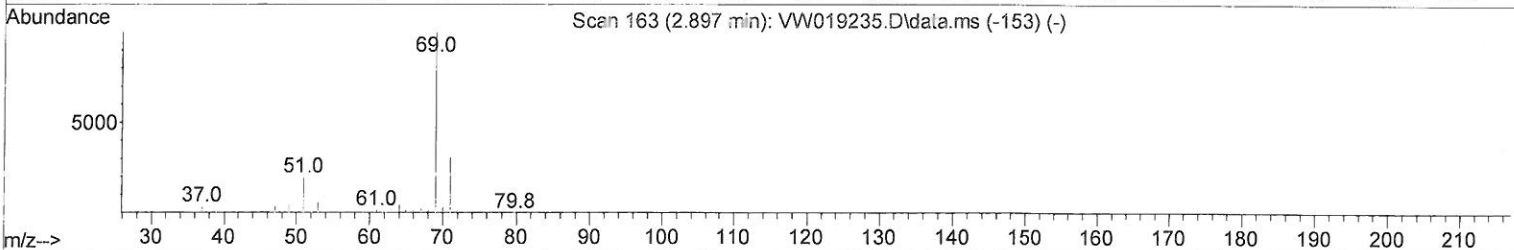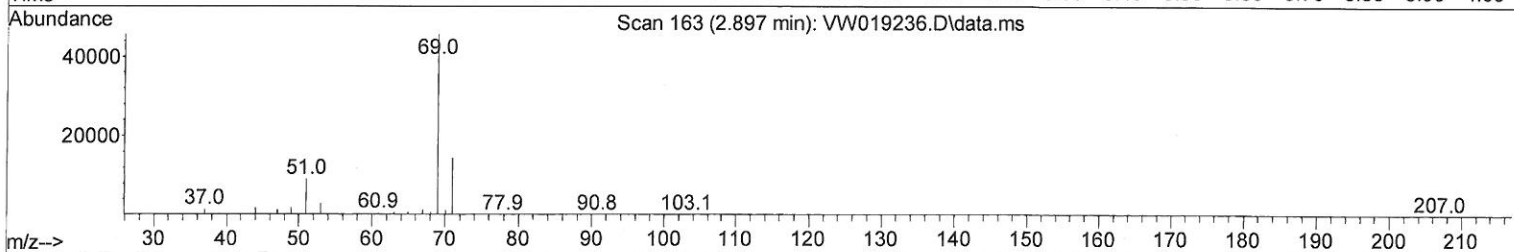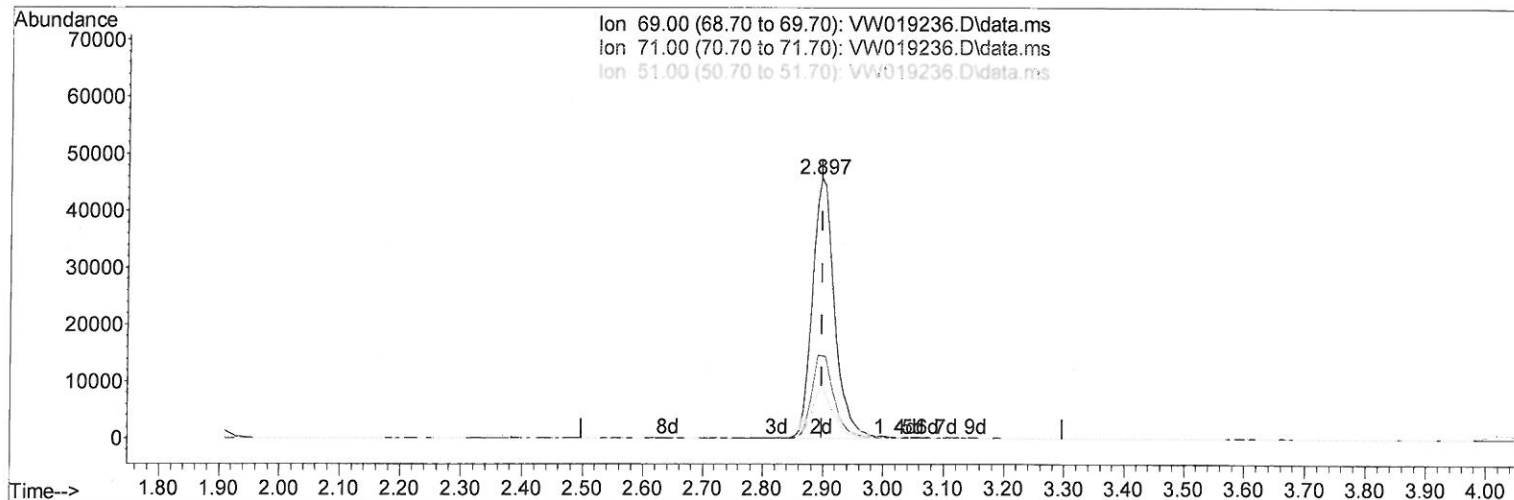

TIC: VW019236.D\data.ms

(7) Chloroethane-d5 (S)

2.897min (+ 0.000) 21.49 ug/L m

response 118359

Ion	Exp%	Act%
69.00	100.00	100.00
71.00	32.10	0.10#
51.00	28.40	0.14#
0.00	0.00	0.00

206/18/21 SY

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061721\
 Data File : VW019236.D
 Acq On : 17 Jun 2021 12:17
 Operator : SY/VA
 Sample : VW0617SBL01
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 VBLK109

Manual Integrations
 APPROVED

MMDadoda
 6/18/2021 2:35:09 PM

Quant Time: Jun 18 01:03:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
 Quant Title : SFAM01.0
 Qlast Update : Fri Jun 18 01:02:36 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.848	114	489082	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.634	117	442203	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	206722	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.361	65	126288	19.527	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 78.120%			
7) Chloroethane-d5	2.897	69	118359m	21.488	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery = 85.960%			
11) 1,1-Dichloroethene-d2	4.025	63	193806	15.083	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery = 60.320%			
21) 2-Butanone-d5	7.086	46	81802	48.287	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 96.580%			
24) Chloroform-d	7.653	84	316995	24.108	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery = 96.440%			
26) 1,2-Dichloroethane-d4	8.311	65	177118	24.014	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery = 96.040%			
32) Benzene-d6	8.281	84	624890	24.803	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery = 99.200%			
36) 1,2-Dichloropropane-d6	9.274	67	196891	25.778	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery = 103.120%			
41) Toluene-d8	10.323	98	553489	23.921	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery = 95.680%			
43) trans-1,3-Dichloroprop...	10.579	79	74060	22.389	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery = 89.560%			
47) 2-Hexanone-d5	10.927	63	63688	49.173	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery = 98.340%			
56) 1,1,2,2-Tetrachloroeth...	12.695	84	158200	25.109	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery = 100.440%			
66) 1,2-Dichlorobenzene-d4	13.853	152	184796	25.612	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery = 102.440%			
Target Compounds						
16) Methylene chloride	4.928	84	21540	2.374	ug/L	96
42) Toluene	10.390	91	11588	0.370	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

06/18/21 dy

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW061721\
Data File : VW019236.D
Acq On : 17 Jun 2021 12:17
Operator : SY/VA
Sample : VW0617SBL01
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK109

Manual Integrations
APPROVED

MMDadoda
6/18/2021 2:35:09 PM

Quant Time: Jun 18 01:03:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM060221SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 18 01:02:36 2021
Response via : Initial Calibration

