


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW061820\
 Data File : VW015625.D
 Acq On : 18 Jun 2020 08:35
 Operator : SY/VA
 Sample : BFB12
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB12

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM052620S.M
 Title : VOC Analysis
 Last Update : Fri Jun 19 07:30:11 2020

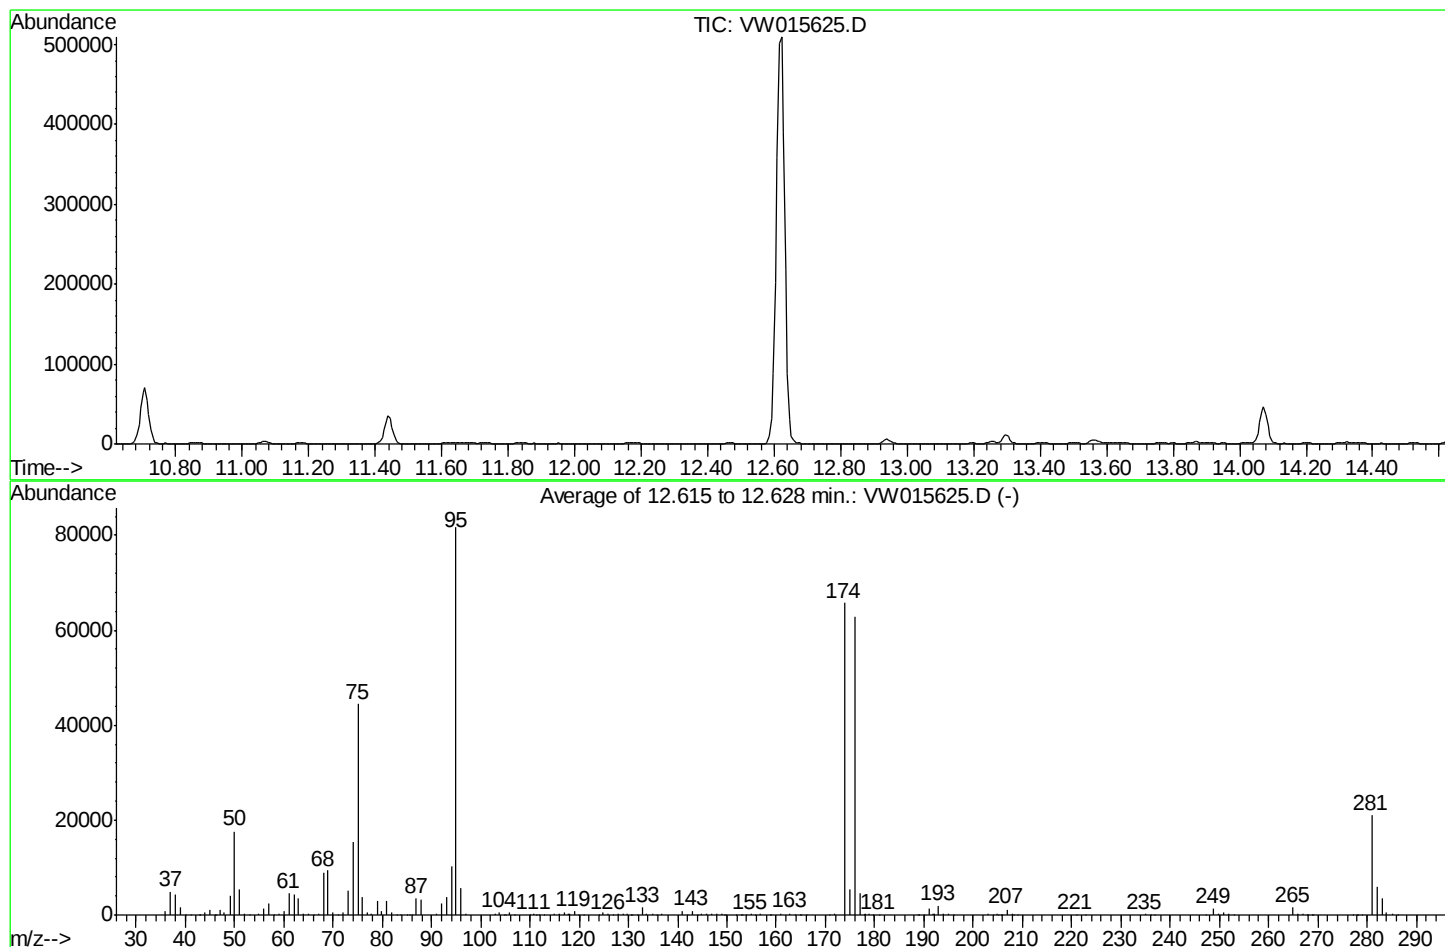

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.5	17584	PASS
75	95	30	80	54.4	44432	PASS
95	95	100	100	100.0	81682	PASS
96	95	5	9	6.8	5563	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	80.5	65792	PASS
175	174	5	9	8.1	5343	PASS
176	174	95	101	95.3	62730	PASS
177	176	5	9	7.4	4662	PASS

m/z	Abundance
36.00	986.0
37.00	5218.0
38.00	4841.0
39.00	1782.0
39.90	228.0
42.80	220.0
44.00	844.0
45.00	1277.0
46.00	108.0
47.00	1181.0
47.90	631.0
49.00	4371.0
50.00	18800.0
51.00	5914.0
52.00	253.0
55.00	235.0
56.00	1389.0
56.90	2812.0
58.10	100.0
58.90	413.0
60.00	1048.0
61.00	4990.0
62.00	4872.0
63.00	3688.0
64.00	489.0
65.10	308.0
66.10	60.0
66.90	298.0
68.00	9781.0
69.00	10163.0
69.90	761.0
71.10	89.0
72.00	643.0
73.00	6122.0
74.00	16346.0
75.00	46256.0
76.00	4135.0
76.90	575.0
77.80	413.0
78.90	3191.0
79.90	956.0
80.90	3171.0
81.80	731.0
83.00	108.0
83.80	105.0
84.90	55.0
85.90	121.0
86.90	3363.0
88.00	3277.0
91.00	409.0
92.00	2555.0
92.90	3542.0
94.00	10566.0
95.00	84920.0
96.00	5765.0
97.10	259.0
102.90	526.0
103.80	595.0
104.80	217.0
105.90	386.0
106.90	115.0
110.00	157.0
110.90	328.0
111.80	153.0
113.00	80.0
115.00	307.0
115.90	356.0
116.90	700.0
117.80	550.0
118.90	917.0
121.00	113.0
124.00	102.0
124.90	757.0
125.90	239.0
127.80	249.0
128.90	164.0
129.80	291.0
130.90	157.0
131.90	63.0
132.90	2651.0
133.80	462.0
134.80	385.0
135.80	58.0
136.70	170.0
140.90	758.0
142.90	857.0
144.00	64.0
144.90	285.0
145.90	145.0
146.90	446.0
147.80	201.0
148.90	232.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

149.60	100.0
152.80	65.0
153.90	90.0
154.90	273.0
156.80	186.0
158.80	157.0
160.90	236.0
162.90	458.0
163.90	122.0
164.80	321.0
166.00	57.0
172.00	387.0
173.90	63800.0
174.90	4889.0
175.90	58336.0
176.90	4838.0
177.90	367.0
178.80	471.0
179.70	133.0
180.90	70.0
188.70	220.0
190.00	105.0
190.90	2230.0
191.80	564.0
192.90	3110.0
193.90	513.0
194.90	372.0
196.00	53.0
203.00	302.0
204.00	64.0
204.90	665.0
206.00	121.0
206.90	1798.0
207.90	403.0
208.90	169.0
221.00	159.0
222.90	59.0
234.90	361.0
236.00	88.0
236.70	68.0
247.20	61.0
248.90	2068.0
249.90	619.0
251.00	880.0
252.10	203.0
253.00	109.0
264.90	2196.0
265.90	546.0
266.90	592.0
268.00	131.0
268.90	70.0
277.00	50.0
277.90	78.0
280.90	31720.0
282.00	8088.0
283.00	5404.0
284.00	991.0
285.10	256.0
286.10	70.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

m/z	Abundance
36.00	979.0
37.00	5538.0
38.00	4603.0
39.00	1915.0
39.90	219.0
41.00	55.0
43.00	129.0
43.90	926.0
44.90	1027.0
45.90	105.0
47.00	1113.0
48.00	645.0
49.00	4501.0
50.00	19944.0
51.00	5951.0
52.00	250.0
54.90	294.0
56.00	1687.0
57.00	2829.0
58.00	157.0
59.00	223.0
59.90	1060.0
61.00	4898.0
62.00	4785.0
63.00	3846.0
64.00	435.0
65.00	211.0
67.00	300.0
68.00	10138.0
69.00	10251.0
70.00	764.0
71.00	51.0
71.90	576.0
73.00	5708.0
74.00	16800.0
75.00	49896.0
76.00	4175.0
76.90	555.0
77.90	409.0
78.90	3114.0
79.90	950.0
80.90	3339.0
81.90	667.0
83.00	89.0
86.00	159.0
86.90	3831.0
87.90	3354.0
91.00	381.0
92.00	2906.0
93.00	4364.0
94.00	11661.0
95.00	90496.0
96.00	6084.0
97.00	176.0
103.00	395.0
103.90	451.0
105.00	204.0
105.90	437.0
106.80	75.0
110.00	150.0
110.80	172.0
111.30	92.0
111.90	126.0
112.80	108.0
114.90	214.0
115.90	346.0
117.00	692.0
118.00	543.0
118.90	732.0
119.80	51.0
124.00	101.0
124.90	441.0
125.80	212.0
126.80	74.0
127.90	325.0
128.90	208.0
129.70	330.0
130.60	163.0
131.90	51.0
133.00	1452.0
133.60	442.0
134.90	294.0
136.80	277.0
140.90	913.0
142.00	118.0
142.90	977.0
144.80	172.0
145.90	203.0
146.90	208.0
147.90	215.0
148.80	163.0
149.80	118.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

152.80	85.0
153.90	94.0
154.80	188.0
155.70	68.0
156.80	172.0
159.00	136.0
160.80	202.0
162.80	288.0
165.00	239.0
170.90	110.0
171.90	389.0
173.90	70096.0
174.90	6216.0
175.90	69136.0
176.90	5304.0
178.00	285.0
178.90	419.0
179.80	92.0
189.00	179.0
191.00	1550.0
192.00	321.0
192.90	1695.0
194.00	378.0
194.80	209.0
202.90	186.0
204.80	459.0
205.70	58.0
206.90	1262.0
207.80	219.0
208.10	189.0
209.00	137.0
220.90	112.0
234.90	192.0
236.00	59.0
248.80	1406.0
249.90	352.0
250.90	574.0
251.90	181.0
265.00	1614.0
265.90	367.0
266.80	372.0
267.70	61.0
269.10	66.0
278.20	66.0
278.90	117.0
281.00	20944.0
282.00	6302.0
283.00	3852.0
284.00	631.0
285.00	217.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

m/z	Abundance
36.00	794.0
37.00	3890.0
38.00	3505.0
39.00	1212.0
39.90	182.0
41.10	75.0
43.00	103.0
44.00	772.0
45.00	695.0
46.20	104.0
47.00	752.0
47.90	412.0
49.00	3152.0
50.00	14009.0
51.00	4391.0
52.10	194.0
53.10	62.0
55.00	227.0
56.00	1238.0
57.00	2043.0
57.90	78.0
59.00	98.0
59.90	745.0
61.00	3536.0
62.00	3695.0
63.00	2772.0
64.00	217.0
64.90	304.0
66.90	204.0
68.00	7209.0
69.00	7974.0
69.90	524.0
71.00	82.0
72.00	429.0
73.00	3888.0
74.00	13038.0
75.00	37144.0
76.00	3118.0
76.80	277.0
77.80	293.0
78.90	2696.0
79.90	740.0
80.90	2629.0
81.90	519.0
85.60	81.0
87.00	2991.0
87.80	2749.0
91.00	305.0
91.90	2201.0
92.90	3529.0
94.00	8268.0
95.00	69632.0
96.00	4842.0
97.00	146.0
102.80	162.0
103.80	479.0
104.90	130.0
105.80	513.0
107.00	110.0
109.80	68.0
110.70	143.0
111.80	109.0
112.80	80.0
114.90	136.0
115.90	311.0
116.80	499.0
117.90	321.0
119.00	560.0
123.90	77.0
124.90	296.0
126.00	53.0
126.90	53.0
127.80	270.0
128.70	143.0
129.70	335.0
130.80	132.0
133.00	730.0
134.80	161.0
136.70	157.0
140.90	814.0
142.90	789.0
144.00	52.0
144.80	156.0
145.90	110.0
146.80	218.0
147.80	160.0
149.00	73.0
149.80	111.0
151.90	61.0
153.00	52.0
154.90	139.0
155.70	66.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

156.80	176.0
158.90	84.0
160.80	116.0
162.80	158.0
164.70	63.0
170.80	69.0
171.90	395.0
173.90	63480.0
175.00	4925.0
175.90	60720.0
176.90	3846.0
177.70	153.0
178.90	192.0
189.00	61.0
190.90	620.0
192.00	181.0
193.00	1118.0
194.00	117.0
194.80	77.0
202.90	91.0
205.10	216.0
207.00	571.0
207.90	141.0
208.90	80.0
235.00	74.0
249.00	541.0
249.80	175.0
250.80	399.0
251.90	80.0
264.90	840.0
265.90	234.0
267.00	142.0
278.80	81.0
281.00	10312.0
282.00	3204.0
282.90	1690.0
283.90	321.0
285.20	106.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12

Scan 1749 (12.567 min): VW015625.D
BFB12

m/z	Abundance
39.90	112.0
43.90	328.0
55.10	68.0

Instrument :
MSVOA_W
ClientSampleId :
BFB12