

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW061919\
 Data File : VW010880.D
 Acq On : 20 Jun 2019 07:08
 Operator : SY/VA
 Sample : K3447-08
 Misc : 4.99G/5ML/MSVOA W/SOIL
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DISPENSER-2

Quant Time: Jun 20 07:36:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W060419S.M
 Quant Title : SW846 8260
 QLast Update : Wed Jun 05 03:21:19 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	184157	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.84	114	339242	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	282040	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	108737	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.30	65	144054	66.37	ug/l	0.00
Spiked Amount 50.000			Recovery	=	132.74%	
35) Dibromofluoromethane	7.88	113	90315	49.05	ug/l	0.00
Spiked Amount 50.000			Recovery	=	98.10%	
50) Toluene-d8	10.32	98	375771	46.54	ug/l	0.00
Spiked Amount 50.000			Recovery	=	93.08%	
62) 4-Bromofluorobenzene	12.62	95	138884	47.27	ug/l	0.00
Spiked Amount 50.000			Recovery	=	94.54%	
Target Compounds						
16) Acetone	4.13	43	17846	30.684	ug/l	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW061919\
Data File : VW010880.D
Acq On : 20 Jun 2019 07:08
Operator : SY/VA
Sample : K3447-08
Misc : 4.99G/5ML/MSVOA W/SOIL
ALS Vial : 42 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DISPENSER-2

Quant Time: Jun 20 07:36:17 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W060419S.M
Quant Title : SW846 8260
QLast Update : Wed Jun 05 03:21:19 2019
Response via : Initial Calibration

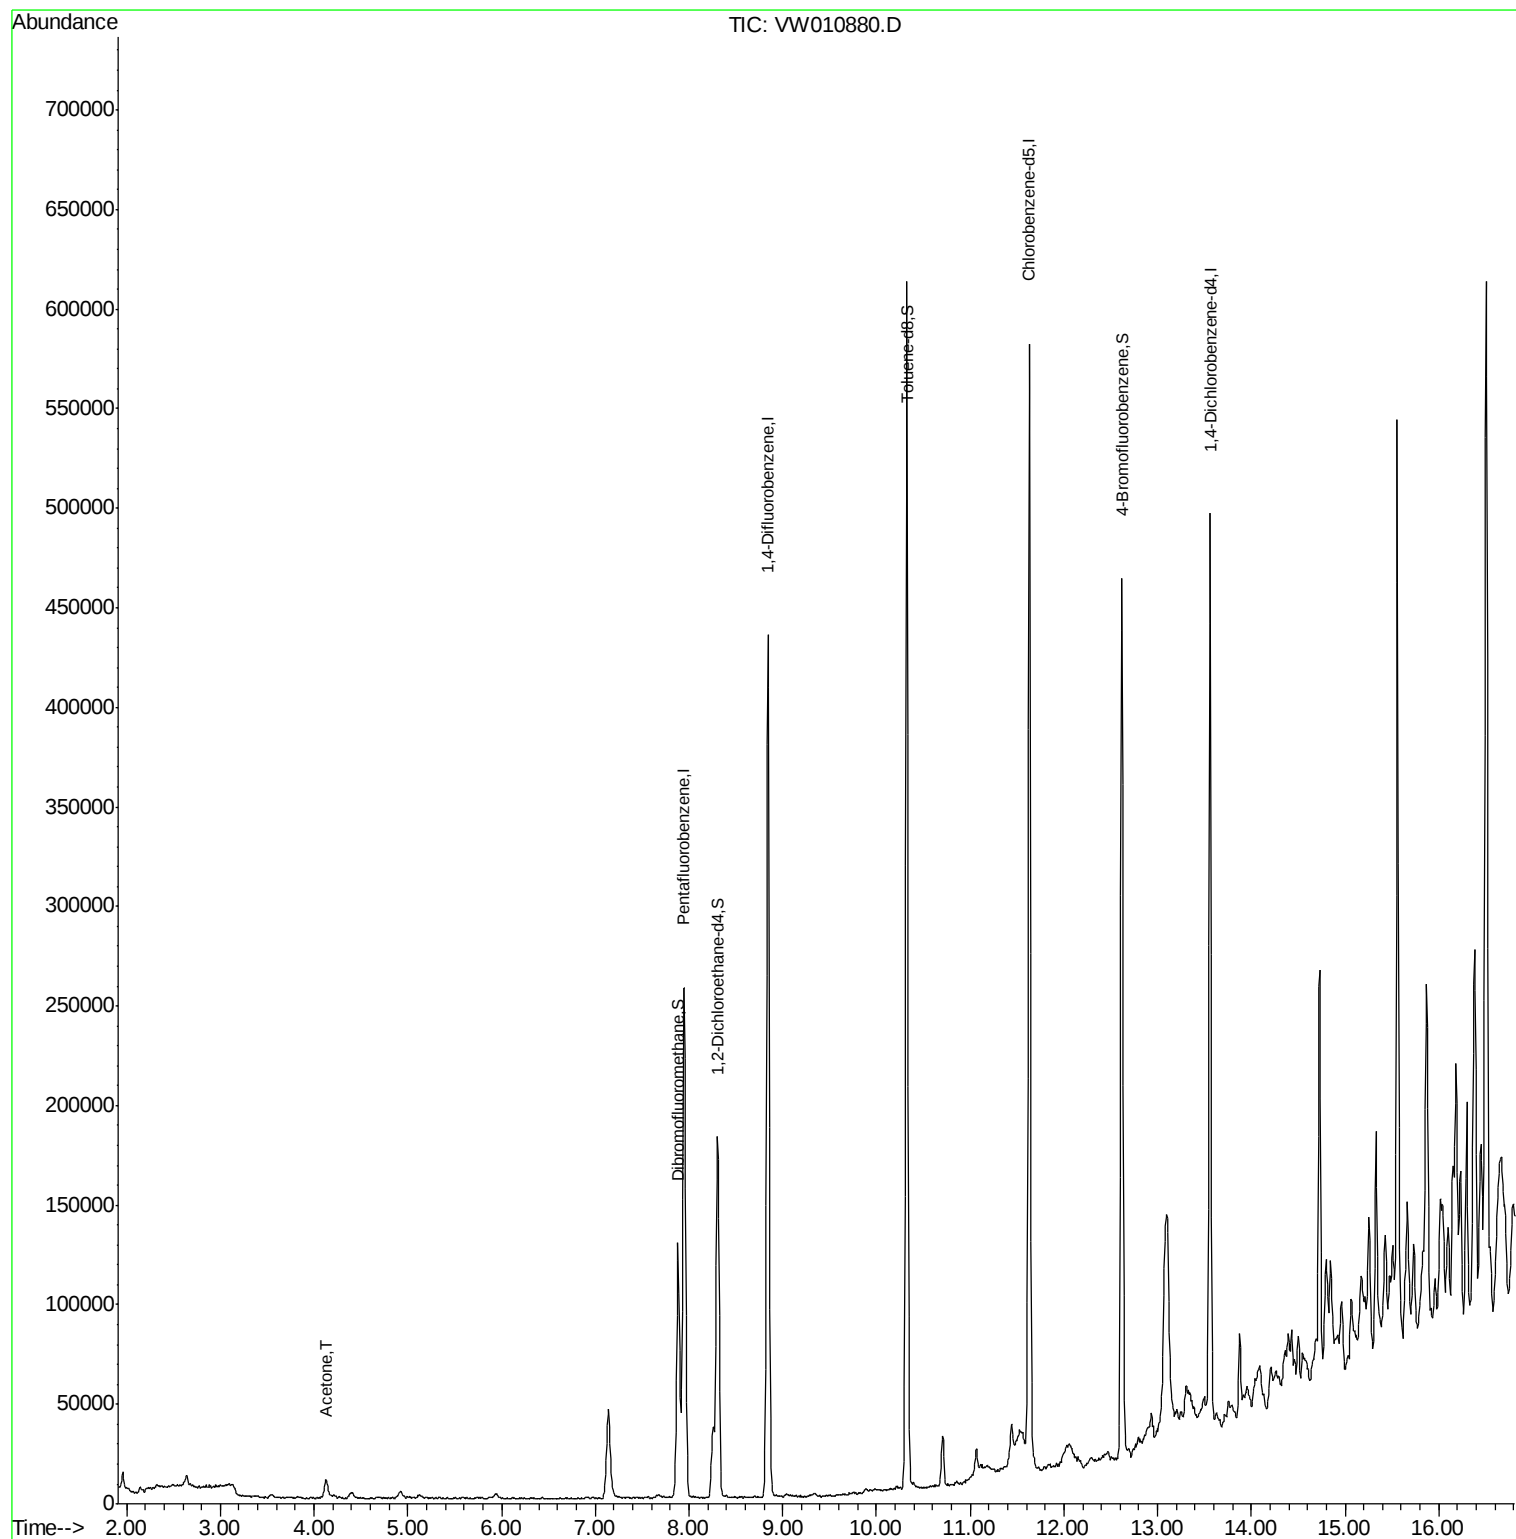

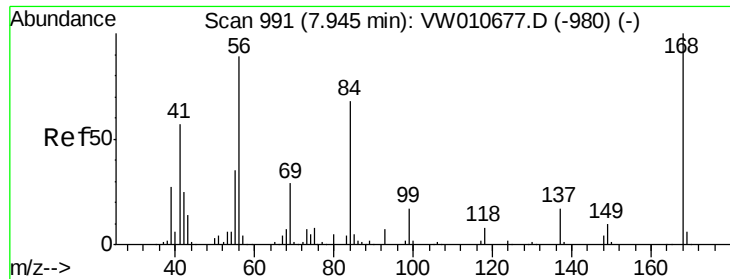

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. 0.01 min

Lab File: VW010880.D

Acq: 20 Jun 2019 07:08

Instrument :

MSVOA_W

ClientSampleId :


DISPENSER-2

Tot Ion:168 Resp: 184157

Ion Ratio Lower Upper




168 100

99 60.6 47.7 71.5

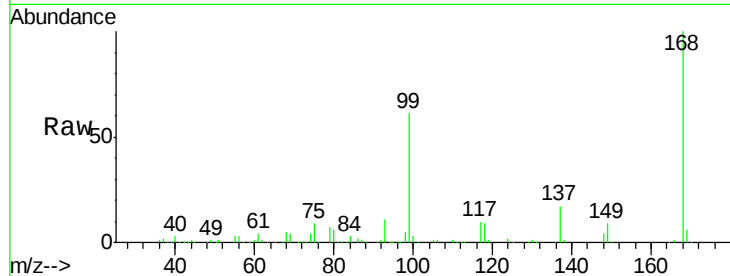

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VW

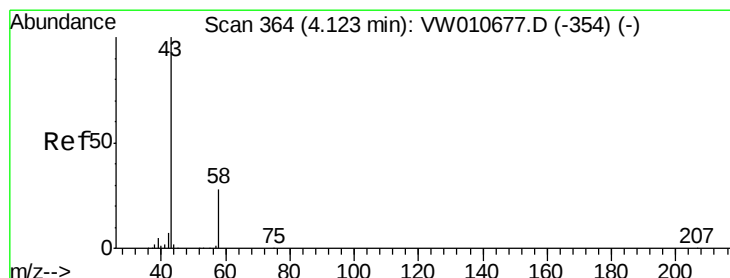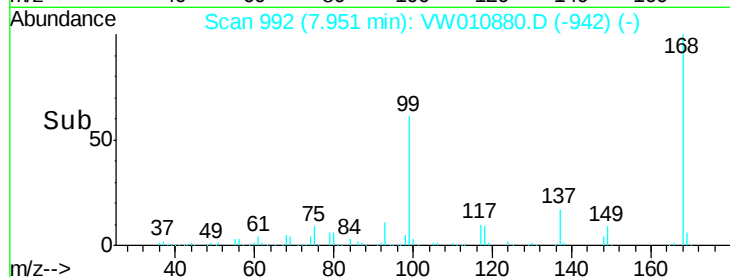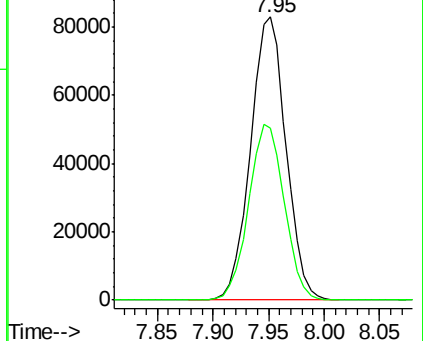

#16

Acetone

Concen: 30.684 ug/l

RT: 4.13 min Scan# 365

Delta R.T. 0.01 min

Lab File: VW010880.D


Acq: 20 Jun 2019 07:08

Tgt Ion: 43 Resp: 17846

Ion Ratio Lower Upper



43 100


58 30.1 22.1 33.1

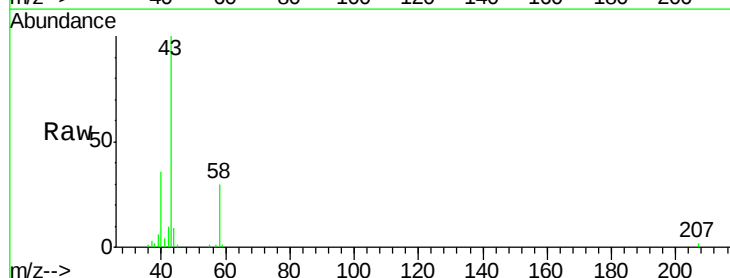

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

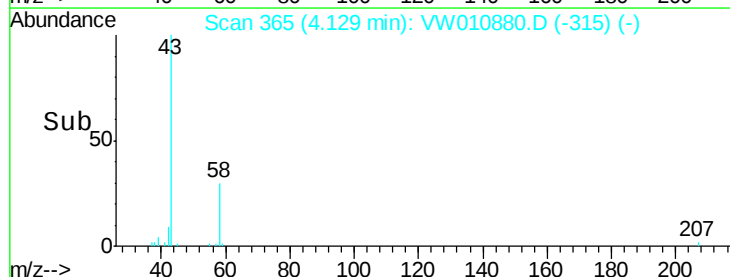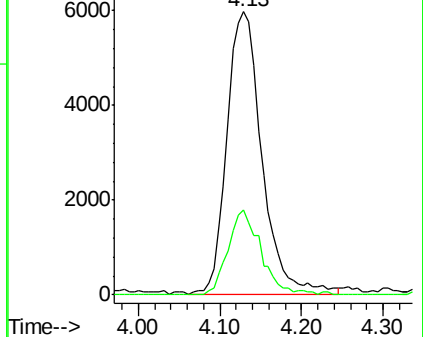

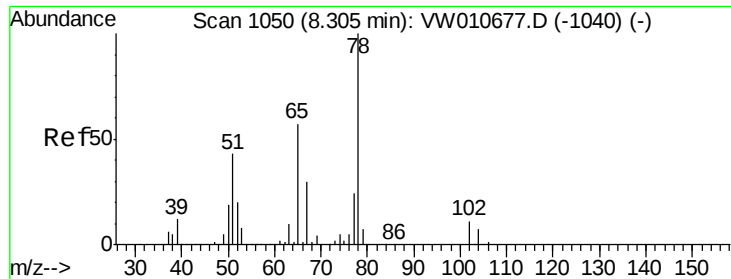

#33

1,2-Dichloroethane-d4

Concen: 66.366 ug/l

RT: 8.30 min Scan# 1050

Delta R.T. -0.00 min

Lab File: VW010880.D

Acq: 20 Jun 2019 07:08

Instrument :

MSVOA_W

ClientSampleId :





DISPENSER-2

Tot Ion: 65 Resp: 144054

Ion Ratio Lower Upper

65 100

67 51.5 0.0 102.6

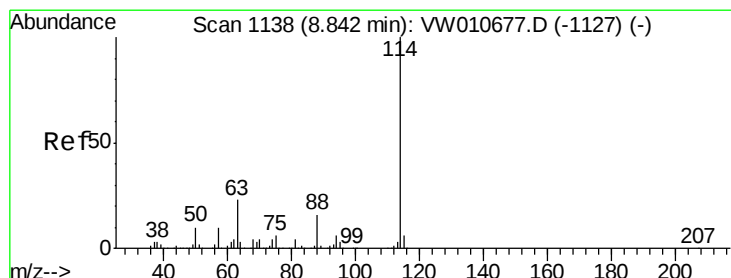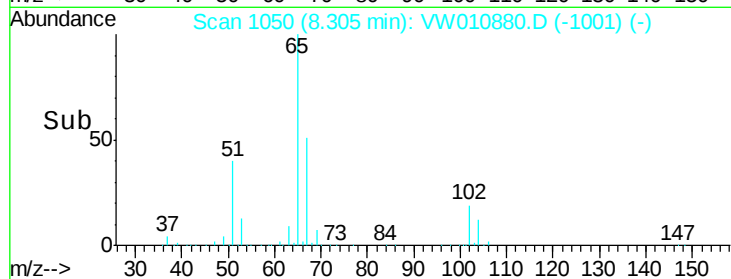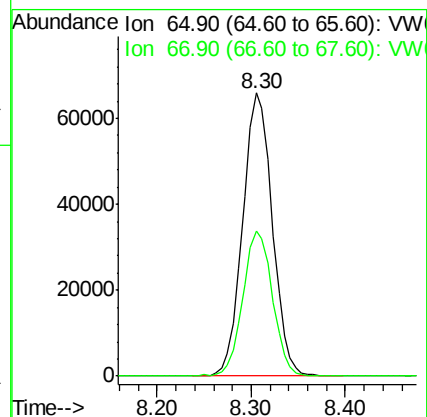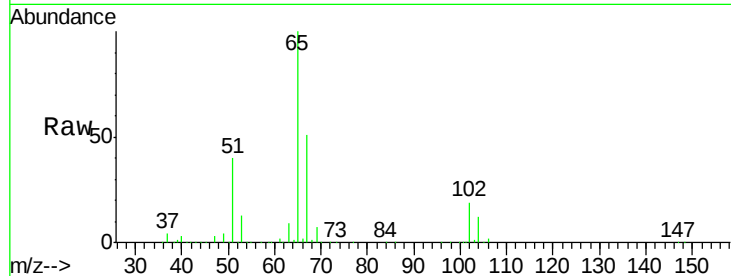

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.84 min Scan# 1138

Delta R.T. -0.00 min

Lab File: VW010880.D

Acq: 20 Jun 2019 07:08




Tgt Ion: 114 Resp: 339242


Ion Ratio Lower Upper

114 100

63 25.5 0.0 46.4

88 17.1 0.0 32.2

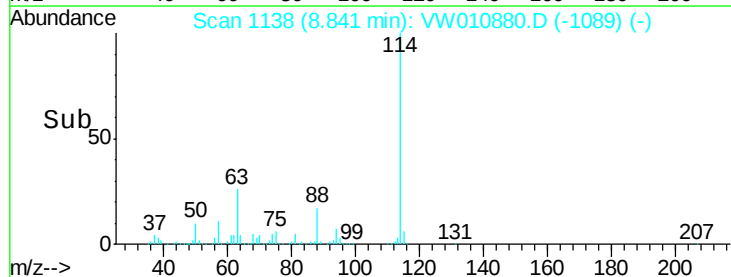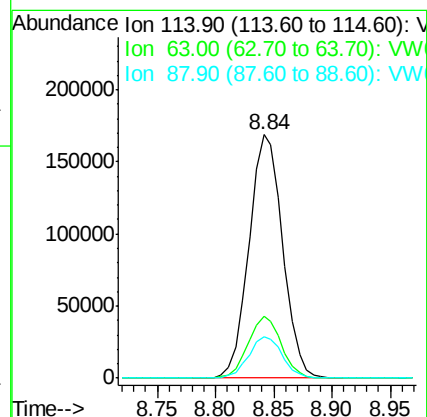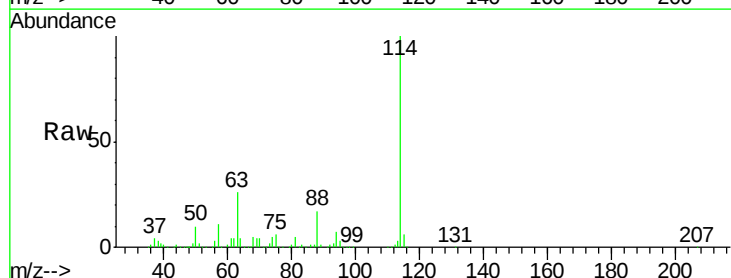


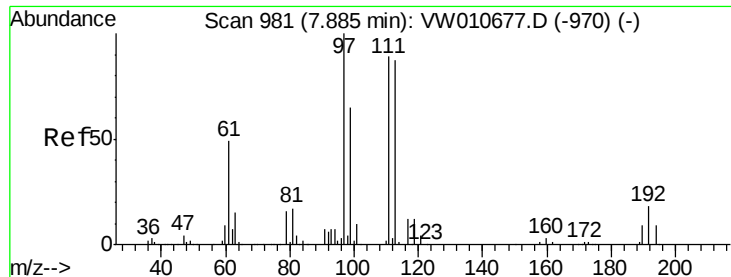




#35
 Dibromofluoromethane
 Concen: 49.049 ug/l
 RT: 7.88 min Scan# 981
 Delta R.T. -0.00 min
 Lab File: VW010880.D
 Acq: 20 Jun 2019 07:08

Instrument :
 MSVOA_W
 ClientSampleId :
 DISPENSER-2

Tot Ion	Ratio	Lower	Upper
113	100		
111	104.0	82.6	123.8
192	19.6	16.4	24.6

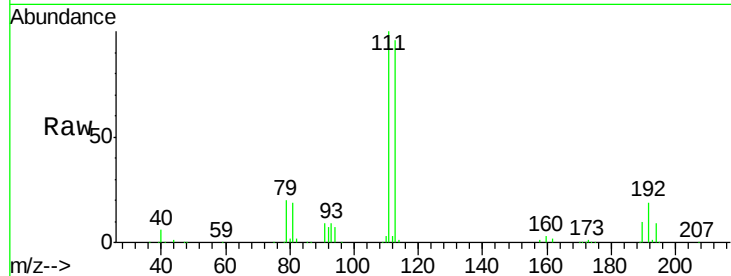


Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

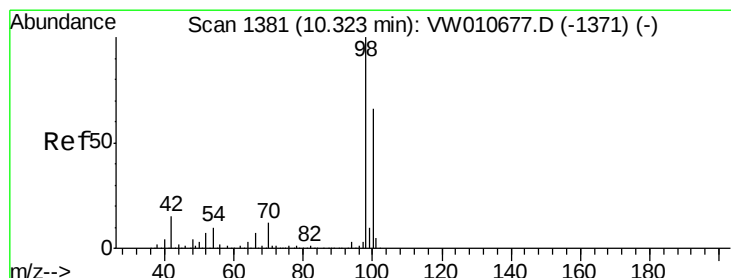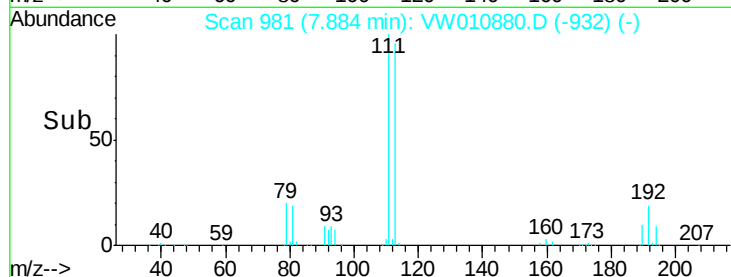
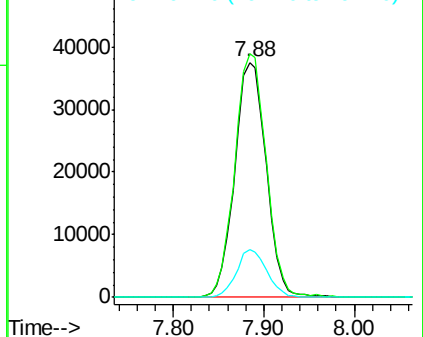



#50
 Toluene-d8
 Concen: 46.538 ug/l
 RT: 10.32 min Scan# 1381
 Delta R.T. -0.00 min
 Lab File: VW010880.D
 Acq: 20 Jun 2019 07:08

Tgt Ion	Ratio	Lower	Upper
98	100		
100	65.3	53.0	79.6

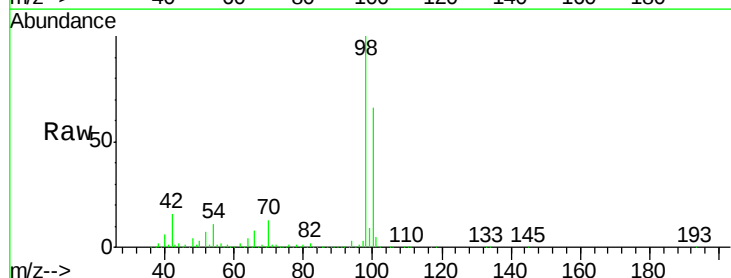

Abundance Ion 98.00 (97.70 to 98.70): VW
 Ion 100.00 (99.70 to 100.70): VW



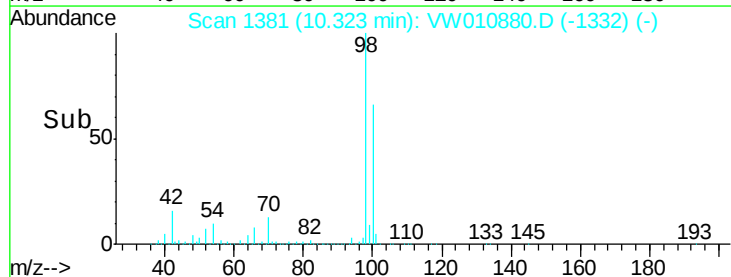
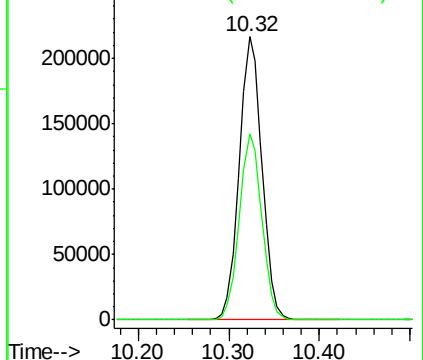


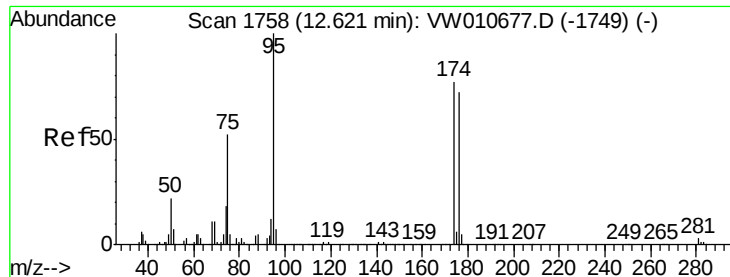

#62
4-Bromofluorobenzene
Concen: 47.269 ug/l
RT: 12.62 min Scan# 1758
Delta R.T. -0.00 min
Lab File: VW010880.D
Acq: 20 Jun 2019 07:08




Instrument :
MSVOA_W
ClientSampleId :
DISPENSER-2


Tot Ion: 95 Resp: 138884
Ion Ratio Lower Upper
95 100
174 73.2 0.0 150.4
176 70.4 0.0 144.8

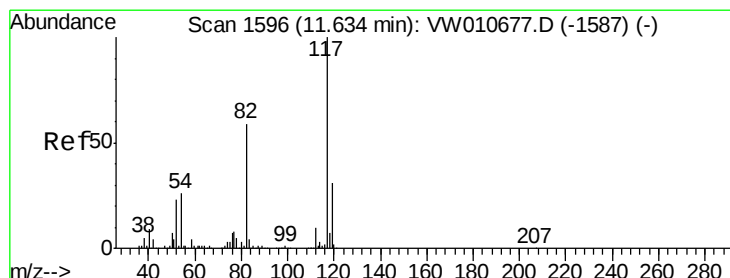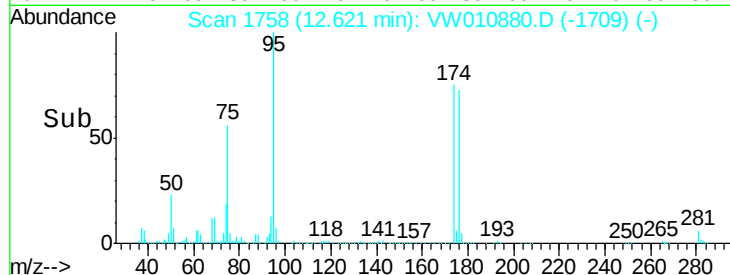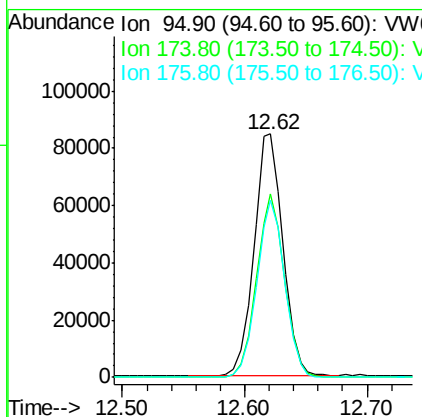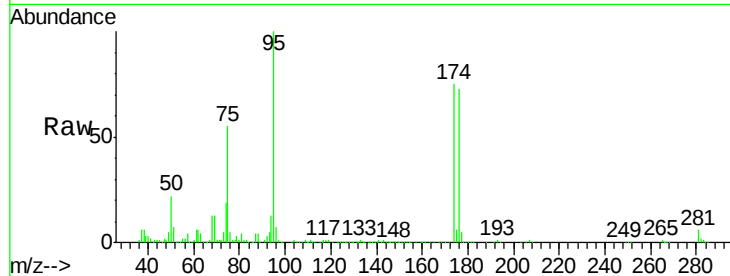

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. -0.00 min
Lab File: VW010880.D
Acq: 20 Jun 2019 07:08

Tgt Ion: 117 Resp: 282040
Ion Ratio Lower Upper
117 100
82 60.3 47.0 70.4
119 32.3 25.1 37.7

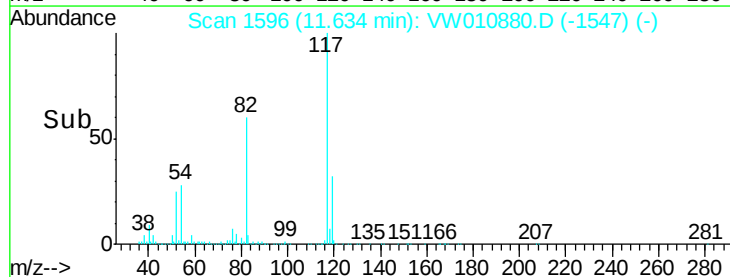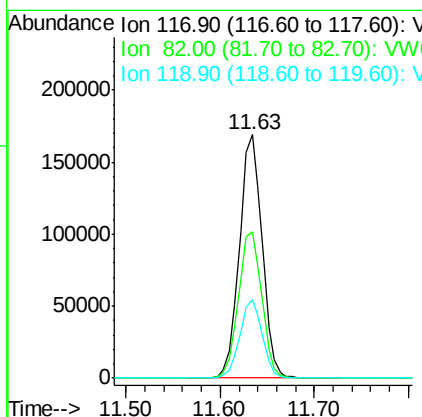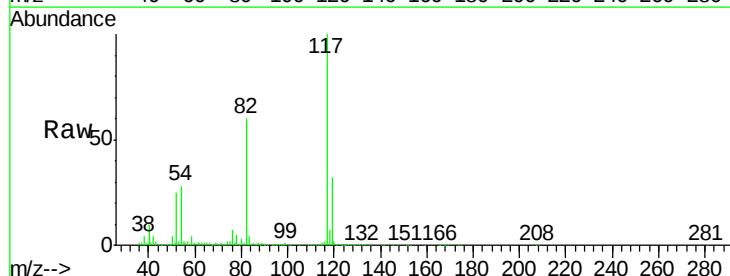

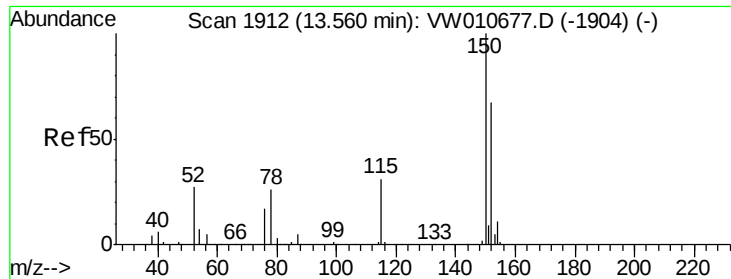

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. -0.00 min

Lab File: VW010880.D

Acq: 20 Jun 2019 07:08

Instrument :

MSVOA_W

ClientSampleId :

DISPENSER-2


Tot Ion:152 Resp: 108737

Ion Ratio Lower Upper

152 100

115 61.0 29.8 89.3

150 159.0 0.0 345.0

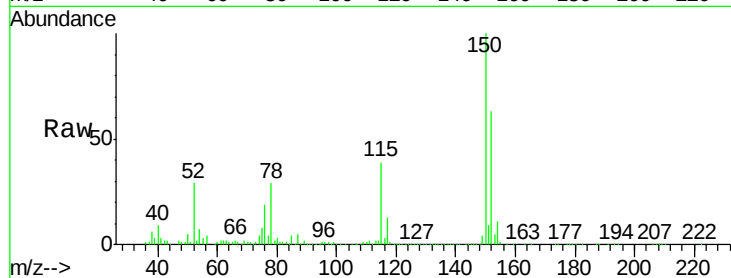

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

