


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW061919\  
Data File : VW010845.D  
Acq On : 19 Jun 2019 10:28  
Operator : SY/VA  
Sample : BFB  
Misc : 5.00G/5ML/MSVOA W/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_W  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA\_W\METHOD\82W060419S.M  
Title : SW846 8260  
Last Update : Wed Jun 05 03:21:19 2019

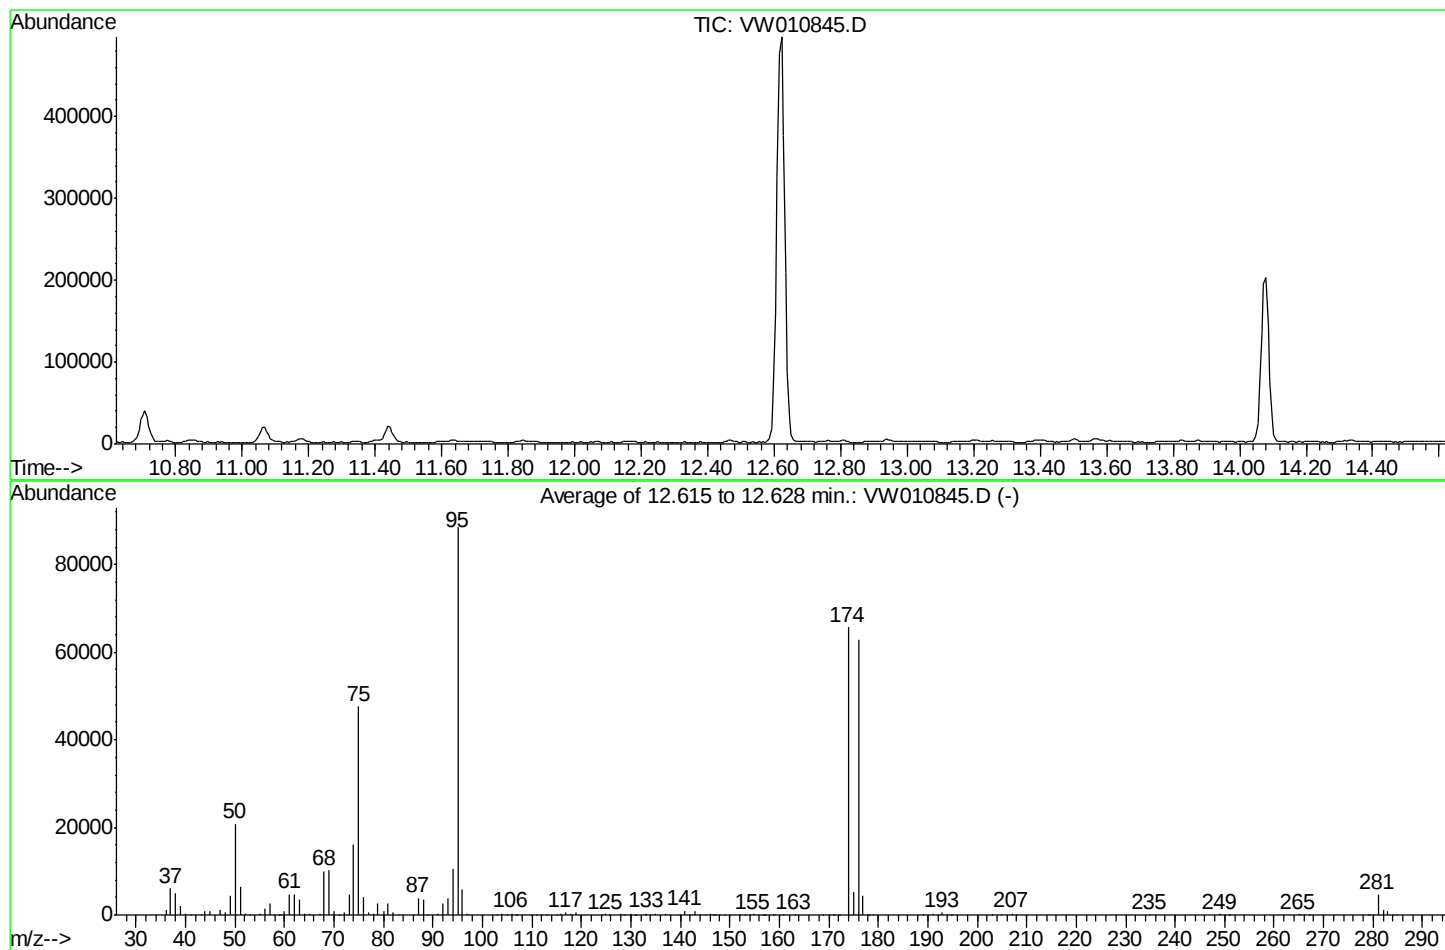

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 50          | 95           | 15           | 40           | 23.6      | 20872   | PASS             |
| 75          | 95           | 30           | 60           | 53.7      | 47552   | PASS             |
| 95          | 95           | 100          | 100          | 100.0     | 88504   | PASS             |
| 96          | 95           | 5            | 9            | 6.6       | 5817    | PASS             |
| 173         | 174          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 174         | 95           | 50           | 100          | 74.3      | 65730   | PASS             |
| 175         | 174          | 5            | 9            | 8.0       | 5241    | PASS             |
| 176         | 174          | 95           | 101          | 95.5      | 62794   | PASS             |
| 177         | 176          | 5            | 9            | 7.0       | 4423    | PASS             |