


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW061919\
 Data File : VW010865.D
 Acq On : 19 Jun 2019 22:40
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W060419S.M
 Title : SW846 8260
 Last Update : Wed Jun 05 03:21:19 2019

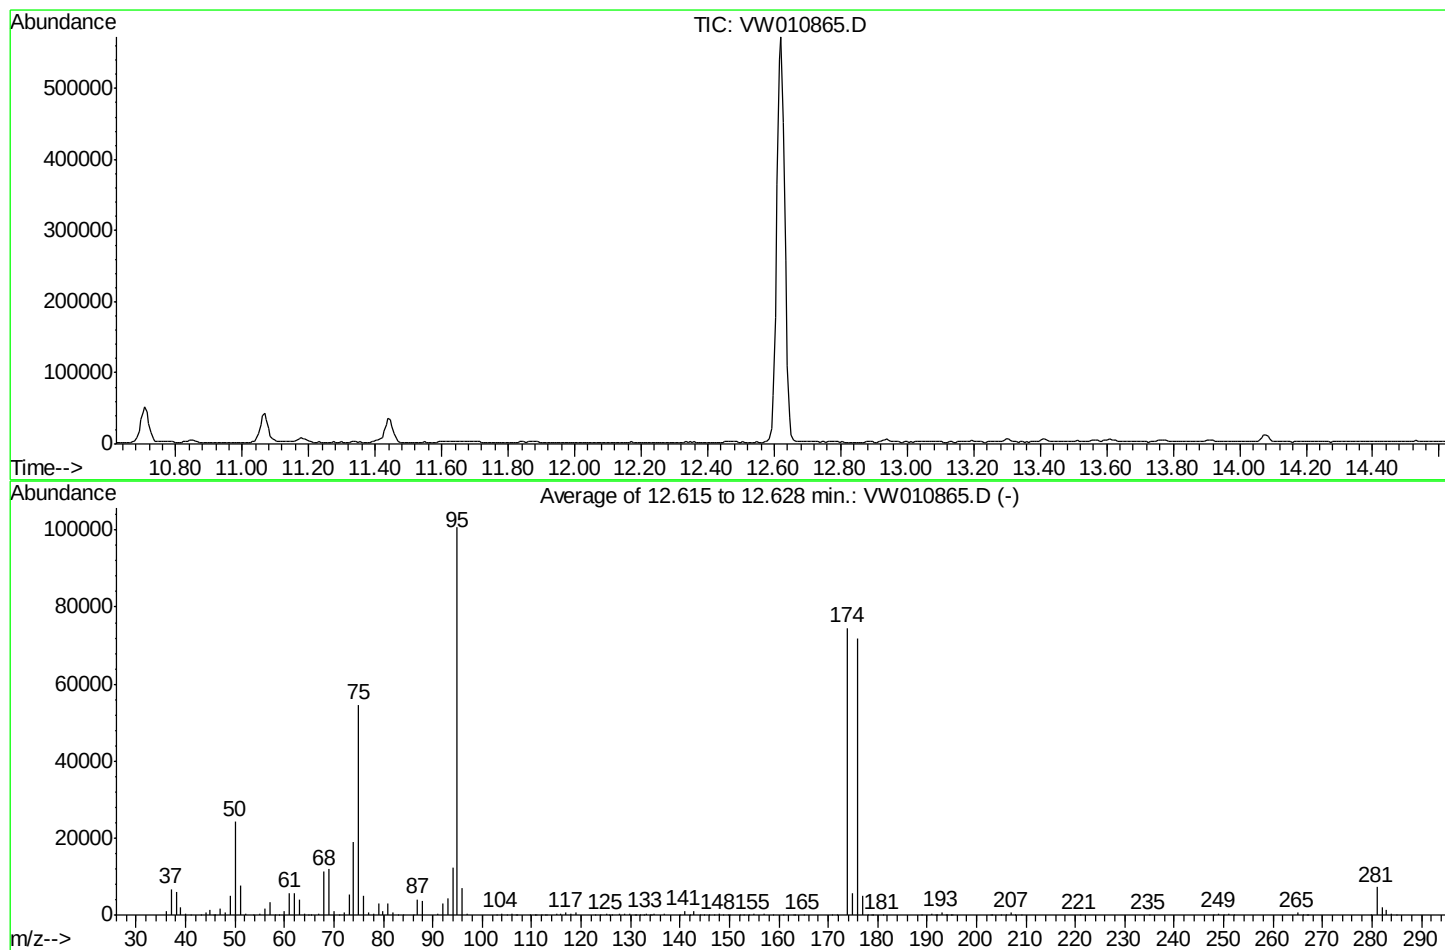

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.0	24186	PASS
75	95	30	60	54.2	54560	PASS
95	95	100	100	100.0	100728	PASS
96	95	5	9	7.0	7049	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.1	74666	PASS
175	174	5	9	7.8	5818	PASS
176	174	95	101	96.2	71842	PASS
177	176	5	9	6.8	4918	PASS