

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW062018\
 Data File : VW003356.D
 Acq On : 20 Jun 2018 16:49
 Operator : SY/AP
 Sample : J3568-07
 Misc : 5.57G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DAXS0

Quant Time: Jun 21 04:21:58 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 21 04:12:02 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	362026	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	334486	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	139320	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	118426	24.12	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.48%
7) Chloroethane-d5	2.89	69	94631	23.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	92.40%
10) 1,1-Dichloroethene-d2	4.01	63	171521	17.59	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.36%
20) 2-Butanone-d5	7.09	46	78066	50.46	ug/L	-0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.92%
24) Chloroform-d	7.65	84	222122	23.32	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.28%
26) 1,2-Dichloroethane-d4	8.31	65	140537	24.83	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.32%
29) Benzene-d6	8.28	84	426172	24.01	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	96.04%
33) 1,2-Dichloropropane-d6	9.28	67	138406	24.64	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.56%
37) Toluene-d8	10.33	98	402923	23.75	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.00%
38) trans-1,3-Dichloropropene-	10.58	79	62604	23.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.96%
39) 2-Hexanone-d5	10.93	63	61414	53.48	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	106.96%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	126687	24.24	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	96.96%
61) 1,2-Dichlorobenzene-d4	13.87	152	130526	24.81	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.24%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	4.14	43	4615	2.798	ug/L	54


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW062018\
Data File : VW003356.D
Acq On : 20 Jun 2018 16:49
Operator : SY/AP
Sample : J3568-07
Misc : 5.57G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DAXS0

Quant Time: Jun 21 04:21:58 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 21 04:12:02 2018
Response via : Initial Calibration

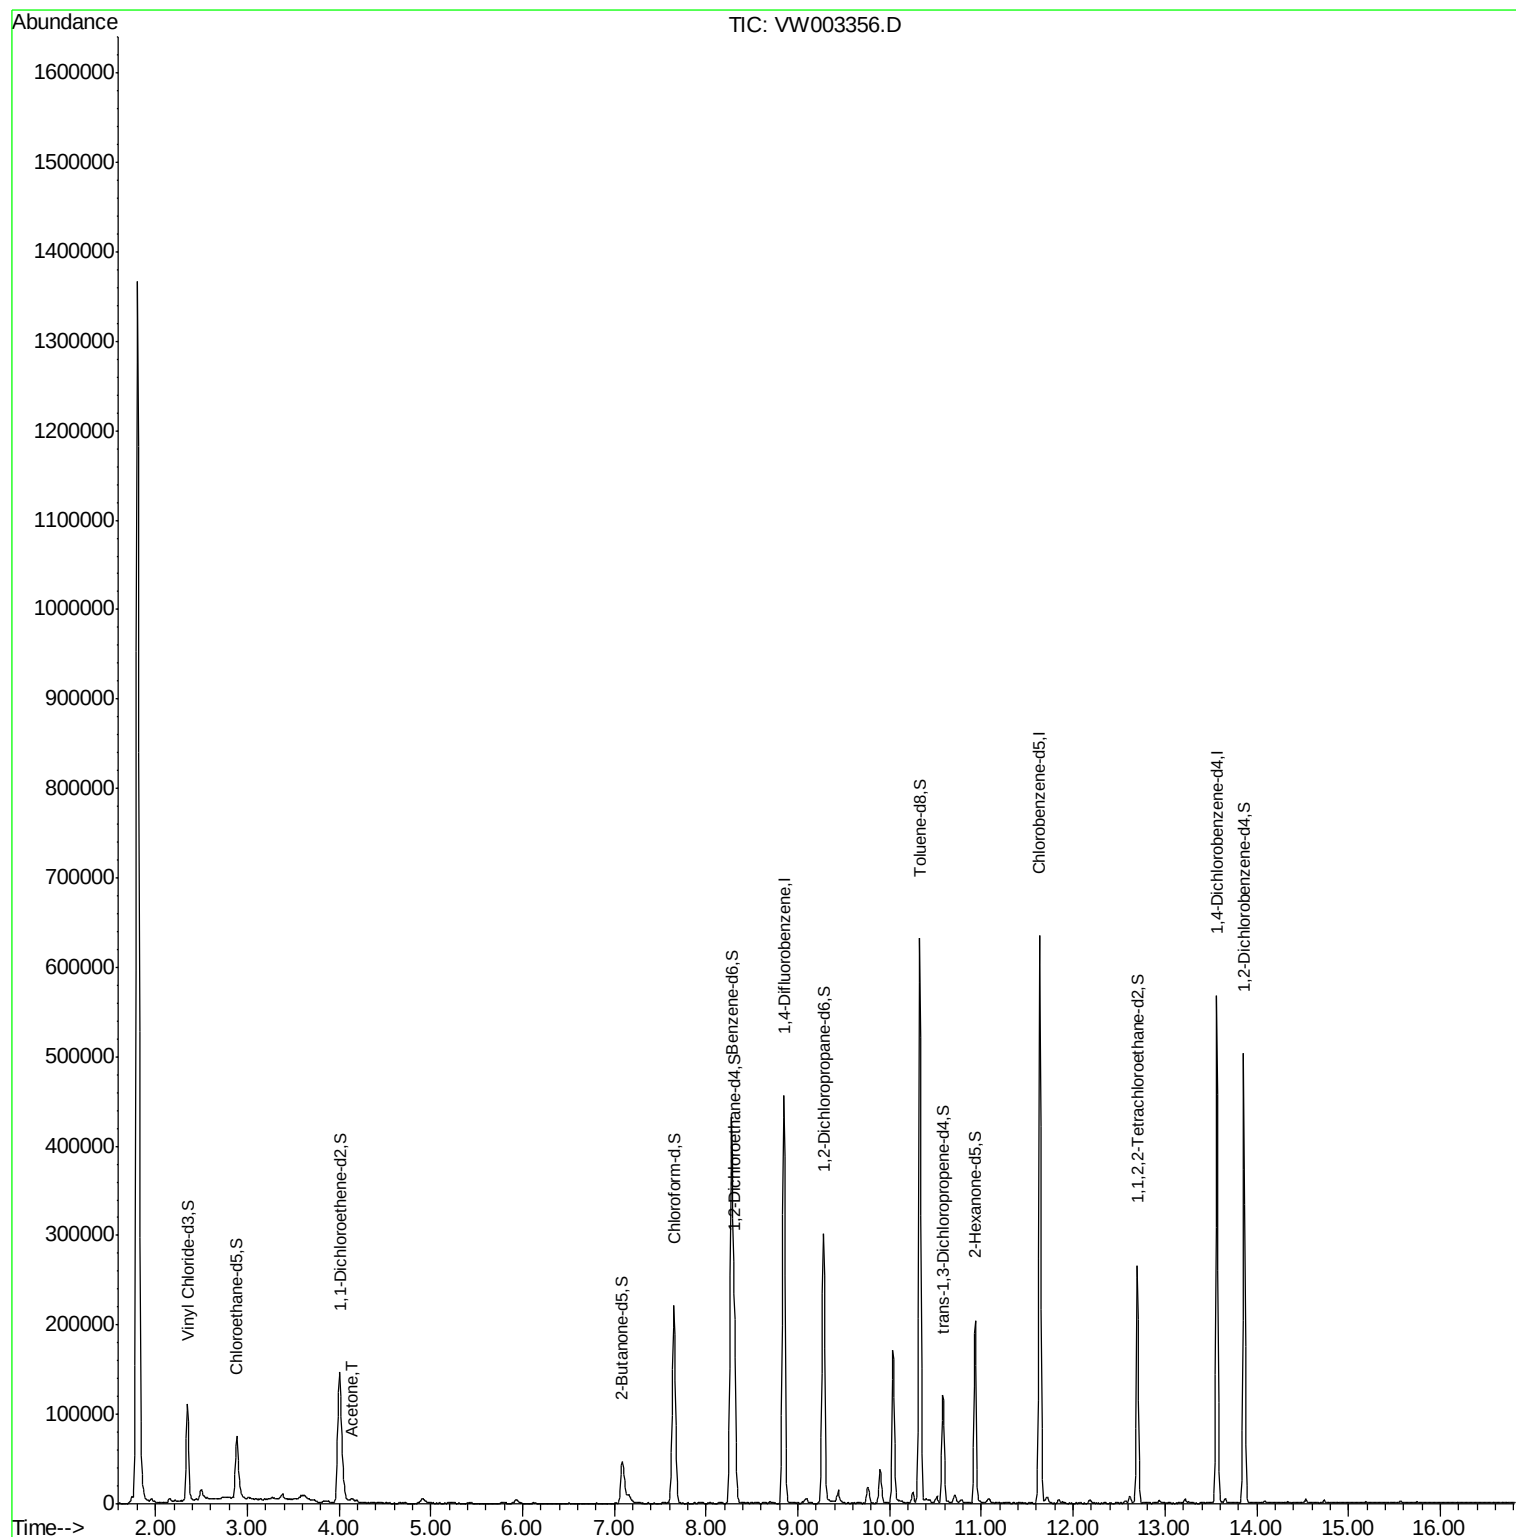

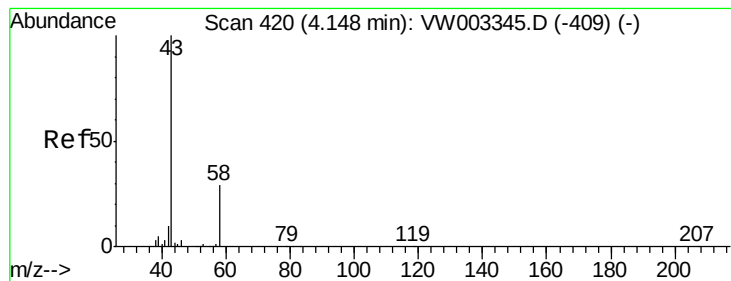

#13
 Acetone
 Concen: 2.798 ug/L
 RT: 4.14 min Scan# 418
 Delta R.T. -0.01 min
 Lab File: VW003356.D
 Acq: 20 Jun 2018 16:49

Instrument :
 MSVOA_W
 ClientSampleId :
 DAXS0

Tgt Ion: 43 Resp: 4615
 Ion Ratio Lower Upper
 43 100
 58 4.5 0.0 58.6

