

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW062018\
 Data File : VW003359.D
 Acq On : 20 Jun 2018 18:17
 Operator : SY/AP
 Sample : VW0620SBL02
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK87

Quant Time: Jun 21 05:05:11 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 21 05:02:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	318009	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	304976	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	140466	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	112533	26.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	104.36%
7) Chloroethane-d5	2.89	69	88609	24.62	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.48%
10) 1,1-Dichloroethene-d2	4.00	63	157453	18.39	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	73.56%
20) 2-Butanone-d5	7.09	46	81769	60.17	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	120.34%
24) Chloroform-d	7.65	84	196874	23.53	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.12%
26) 1,2-Dichloroethane-d4	8.31	65	127522	25.65	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	102.60%
29) Benzene-d6	8.27	84	382288	23.62	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.48%
33) 1,2-Dichloropropane-d6	9.27	67	121898	23.80	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.20%
37) Toluene-d8	10.33	98	359456	23.23	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.92%
38) trans-1,3-Dichloropropene-	10.58	79	56249	23.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.56%
39) 2-Hexanone-d5	10.93	63	61786	59.01	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	118.02%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	120644	25.31	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	101.24%
61) 1,2-Dichlorobenzene-d4	13.86	152	132641	25.00	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.00%


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
13) Acetone	4.15	43	3497	2.414	ug/L	51


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW062018\
Data File : VW003359.D
Acq On : 20 Jun 2018 18:17
Operator : SY/AP
Sample : VW0620SBL02
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK87

Quant Time: Jun 21 05:05:11 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 21 05:02:42 2018
Response via : Initial Calibration

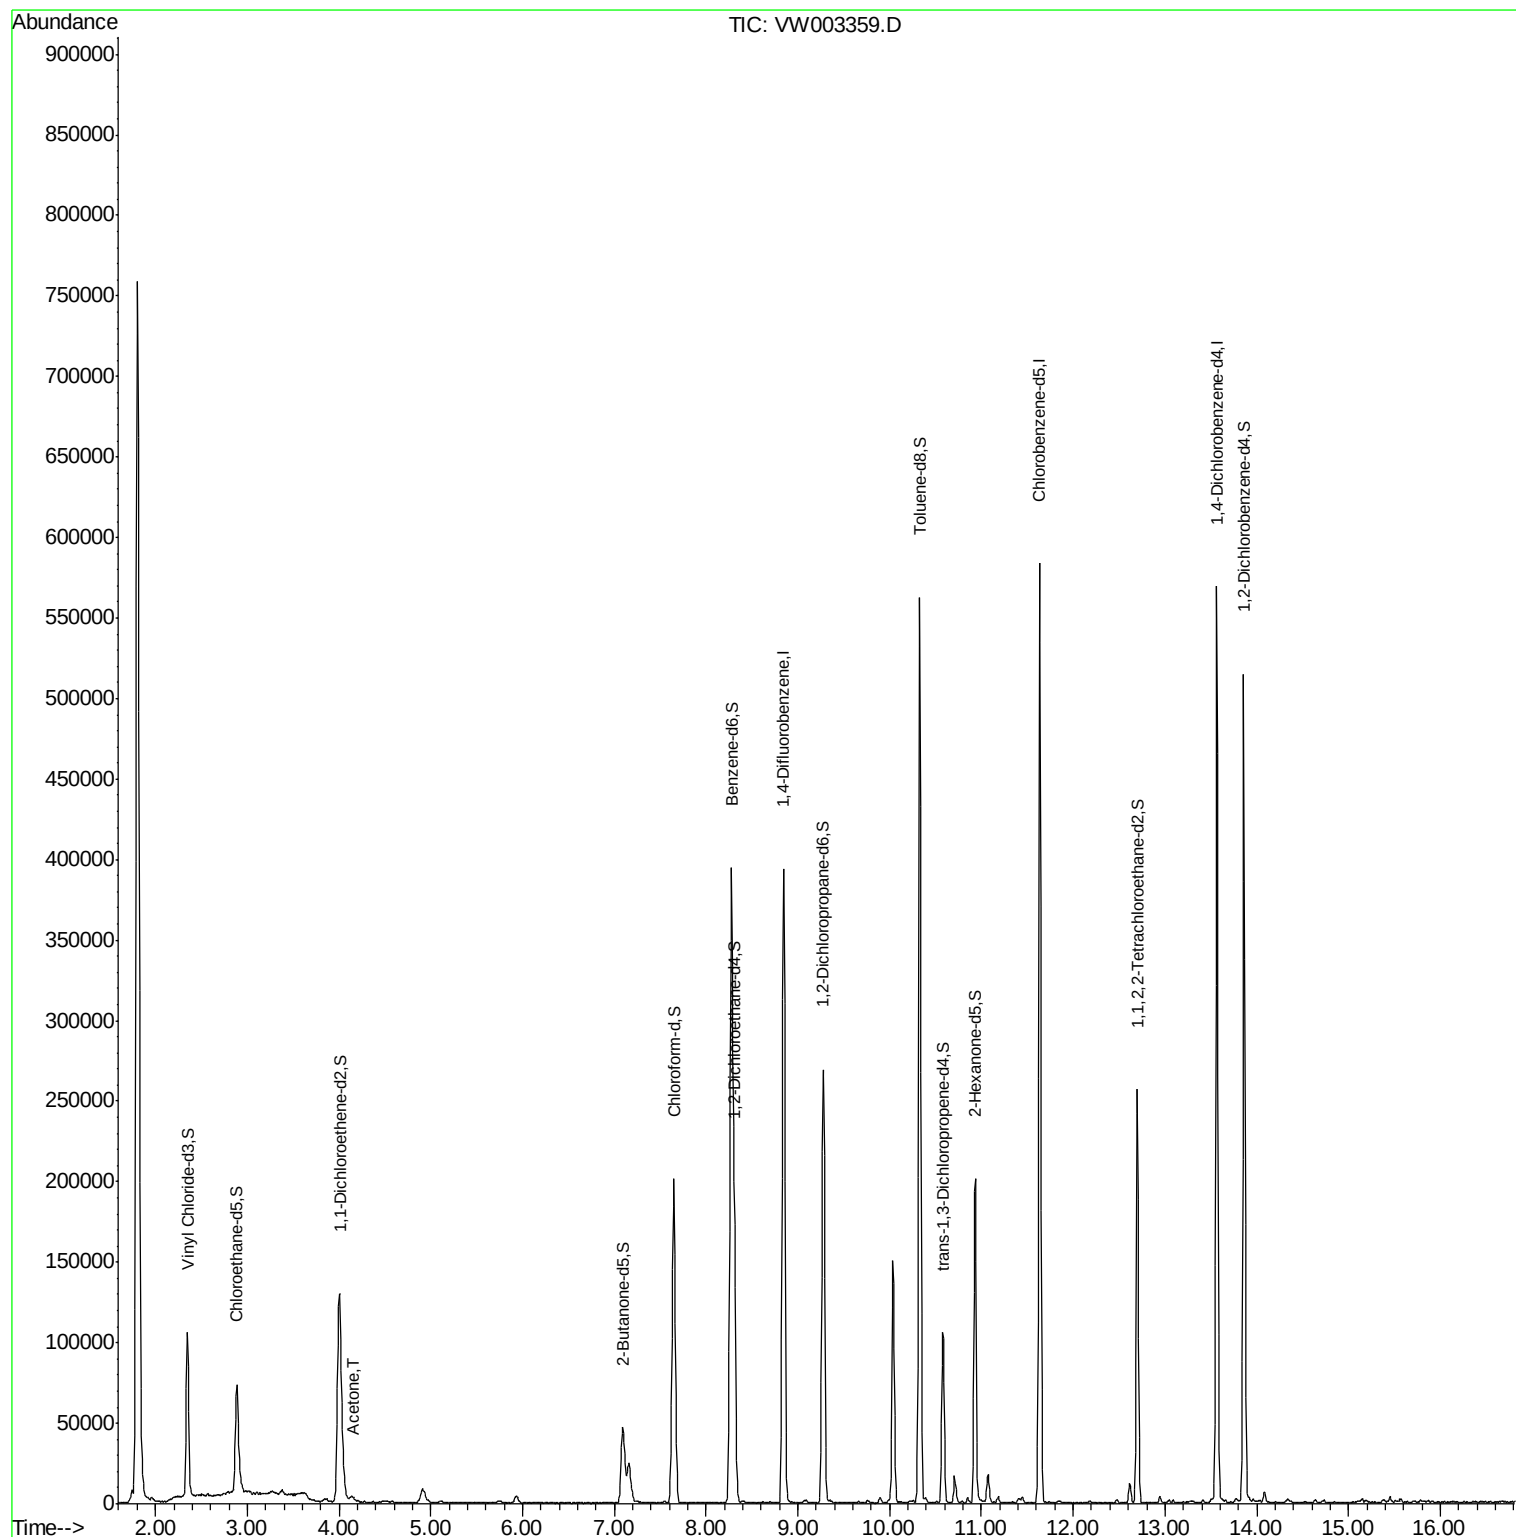

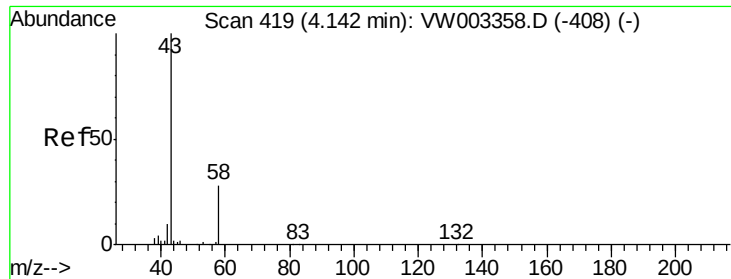

#13

Acetone

Concen: 2.414 ug/L

RT: 4.15 min Scan# 421

Delta R.T. 0.01 min

Lab File: VW003359.D

Acq: 20 Jun 2018 18:17

Instrument :

MSVOA_W

ClientSampleId :

VBLK87

Tgt Ion: 43 Resp: 3497

Ion Ratio Lower Upper

43 100

58 3.0 0.0 58.6

