

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062018\
 Data File : VW003360.D
 Acq On : 20 Jun 2018 18:53
 Operator : SY/AP
 Sample : J3568-06
 Misc : 6.57G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DAXR6

Quant Time: Jun 21 05:05:16 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 21 05:02:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	303141	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	276238	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	105799	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	113600	27.63	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	110.52%
7) Chloroethane-d5	2.89	69	92590	26.99	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.96%
10) 1,1-Dichloroethene-d2	4.00	63	161294	19.76	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	79.04%
20) 2-Butanone-d5	7.09	46	78527	60.62	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	121.24%
24) Chloroform-d	7.65	84	216501	27.15	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	108.60%
26) 1,2-Dichloroethane-d4	8.31	65	141565	29.88	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	119.52%
29) Benzene-d6	8.27	84	411972	28.11	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	112.44%
33) 1,2-Dichloropropane-d6	9.27	67	134744	29.04	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	116.16%
37) Toluene-d8	10.33	98	372865	26.61	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	106.44%
38) trans-1,3-Dichloropropene-	10.58	79	58245	26.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	106.96%
39) 2-Hexanone-d5	10.93	63	59949	63.22	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	126.44%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	123593	28.63	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	114.52%
61) 1,2-Dichlorobenzene-d4	13.87	152	115236	28.84	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	115.36%


Target Compounds					Ovalue
13) Acetone	4.15	43	11847	8.58 ug/L	69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW062018\
Data File : VW003360.D
Acq On : 20 Jun 2018 18:53
Operator : SY/AP
Sample : J3568-06
Misc : 6.57G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DAXR6

Quant Time: Jun 21 05:05:16 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 21 05:02:42 2018
Response via : Initial Calibration

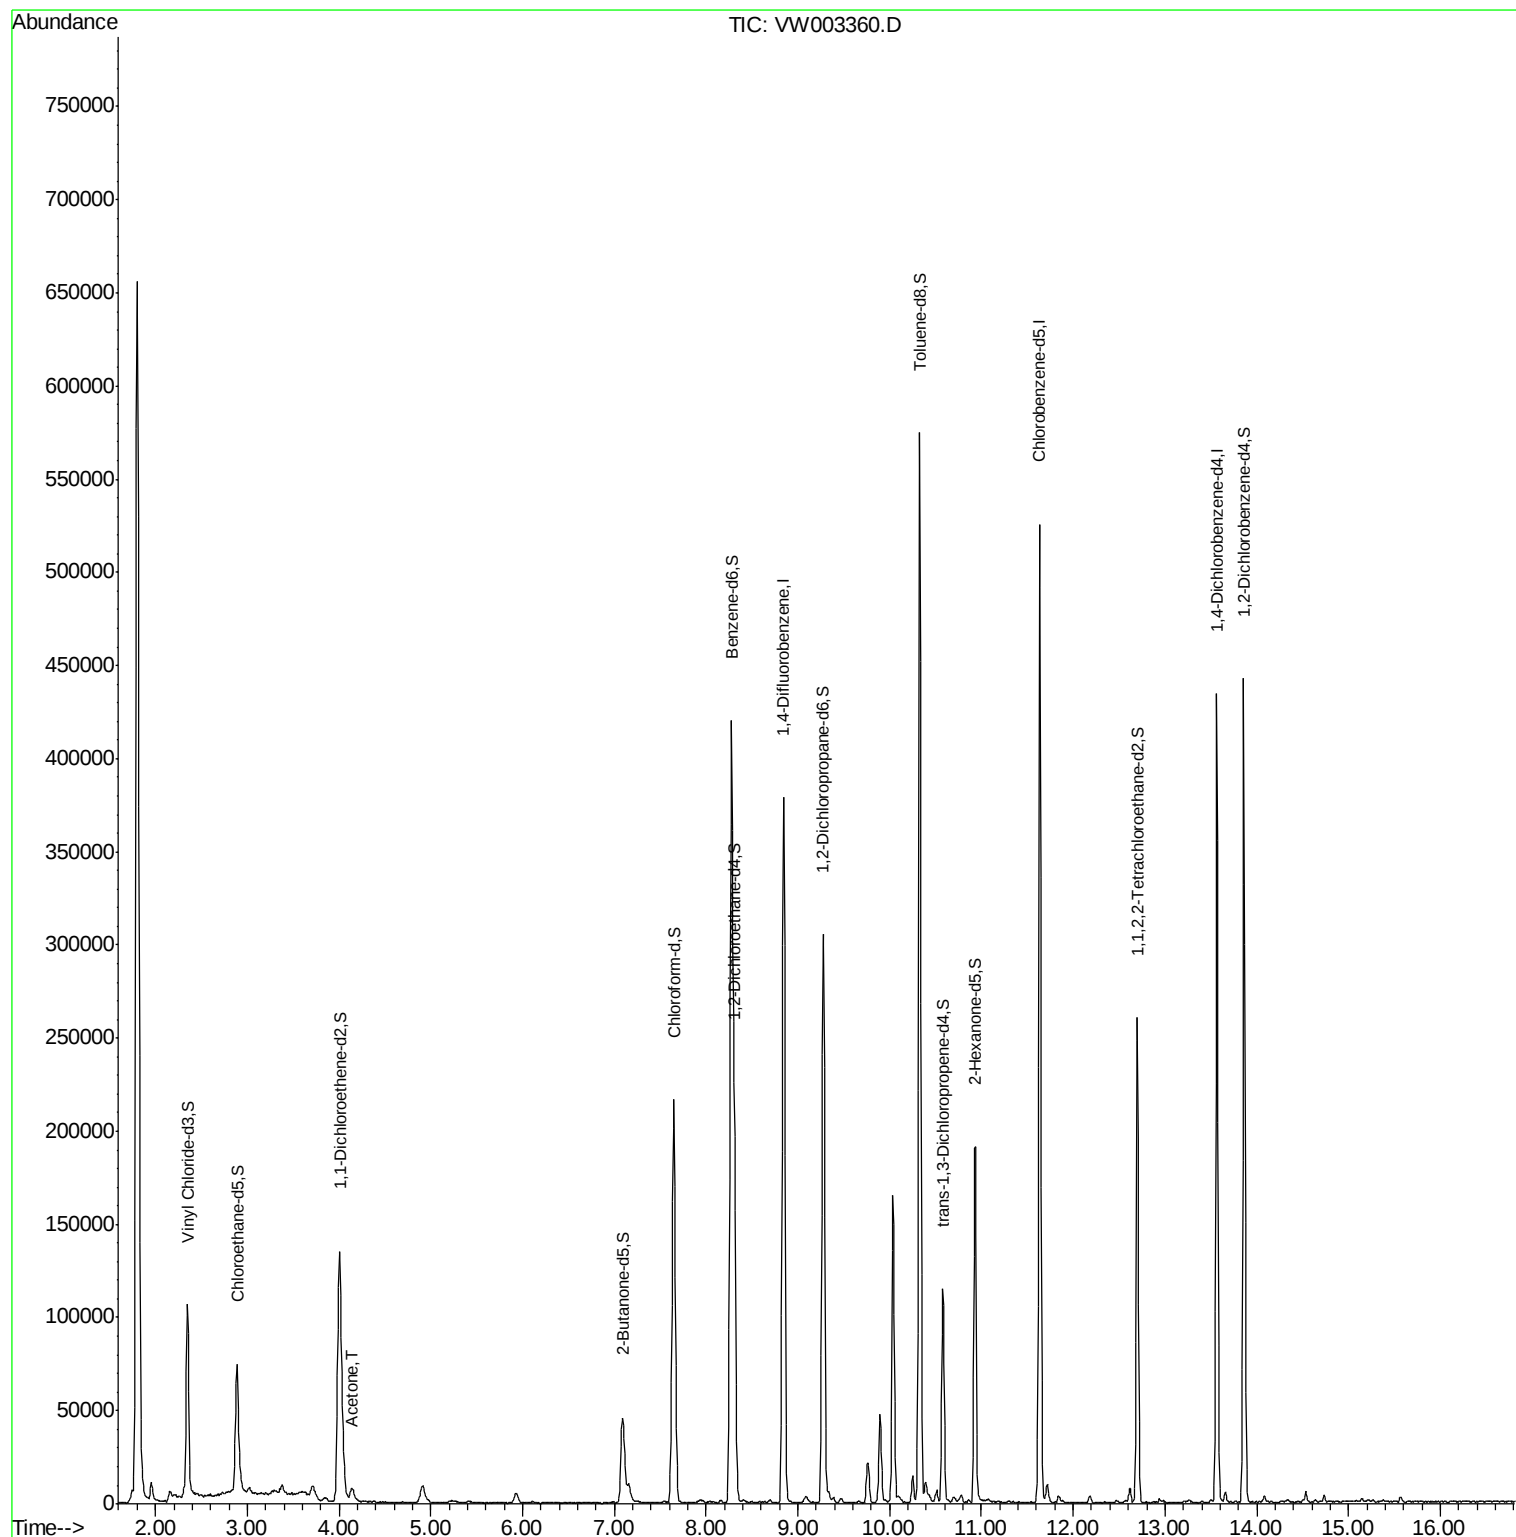

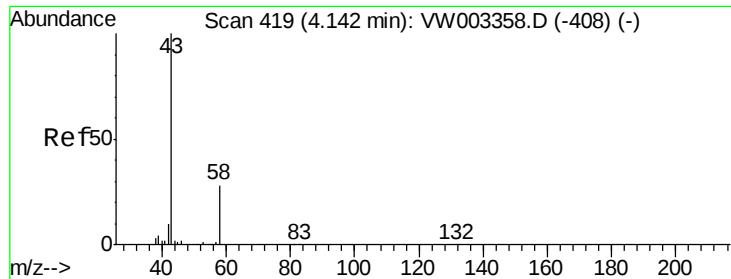

#13

Acetone

Concen: 8.58 ug/L

RT: 4.15 min Scan# 420

Delta R.T. 0.01 min

Lab File: VW003360.D

Acq: 20 Jun 2018 18:53

Instrument :
MSVOA_W
ClientSampleId :
DAXR6

Tot Ion: 43 Resp: 11847

Ion Ratio Lower Upper

43 100

58 12.6 0.0 58.6

