

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062018\
 Data File : VW003371.D
 Acq On : 20 Jun 2018 23:38
 Operator : SY/AP
 Sample : J3569-18
 Misc : 6.09G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DAXT1

Manual Integrations
 APPROVED

MMDadoda
 6/22/2018 4:56:06 PM

Quant Time: Jun 21 06:48:19 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 21 05:02:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	280662	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	190413	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	47030	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	110273	28.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	115.88%
7) Chloroethane-d5	2.89	69	91944	28.95	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	115.80%
10) 1,1-Dichloroethene-d2	4.00	63	150381	19.90	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	79.60%
20) 2-Butanone-d5	7.09	46	45081	37.59	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	75.18%
24) Chloroform-d	7.65	84	186997	25.33	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	101.32%
26) 1,2-Dichloroethane-d4	8.31	65	106209	24.21	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.84%
29) Benzene-d6	8.28	84	360555	35.69	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	142.76%#
33) 1,2-Dichloropropane-d6	9.28	67	109983	34.39	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	137.56%#
37) Toluene-d8	10.33	98	276065	28.58	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	114.32%
38) trans-1,3-Dichloropropene-	10.58	79	34747	23.14	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.56%
39) 2-Hexanone-d5	10.93	63	32863	50.27	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	100.54%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	54898	18.45	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	73.80%
61) 1,2-Dichlorobenzene-d4	13.87	152	44777	25.21	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.84%

Target Compounds

						Ovalue
13) Acetone	4.13	43	108033	84.50	ug/L	86
14) Carbon disulfide	4.36	76	81465	7.20	ug/L	99
16) Methylene chloride	4.91	84	13455m	3.48	ug/L	
21) 2-Butanone	7.18	43	56734	37.76	ug/L	99
44) Toluene	10.39	91	88114	7.48	ug/L	96
54) m,p-Xylene	11.84	106	10052	2.05	ug/L	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062018\
Data File : VW003371.D
Acq On : 20 Jun 2018 23:38
Operator : SY/AP
Sample : J3569-18
Misc : 6.09G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
DAXT1

Manual Integrations
APPROVED

MMDadoda
6/22/2018 4:56:06 PM

Quant Time: Jun 21 06:48:19 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 21 05:02:42 2018
Response via : Initial Calibration

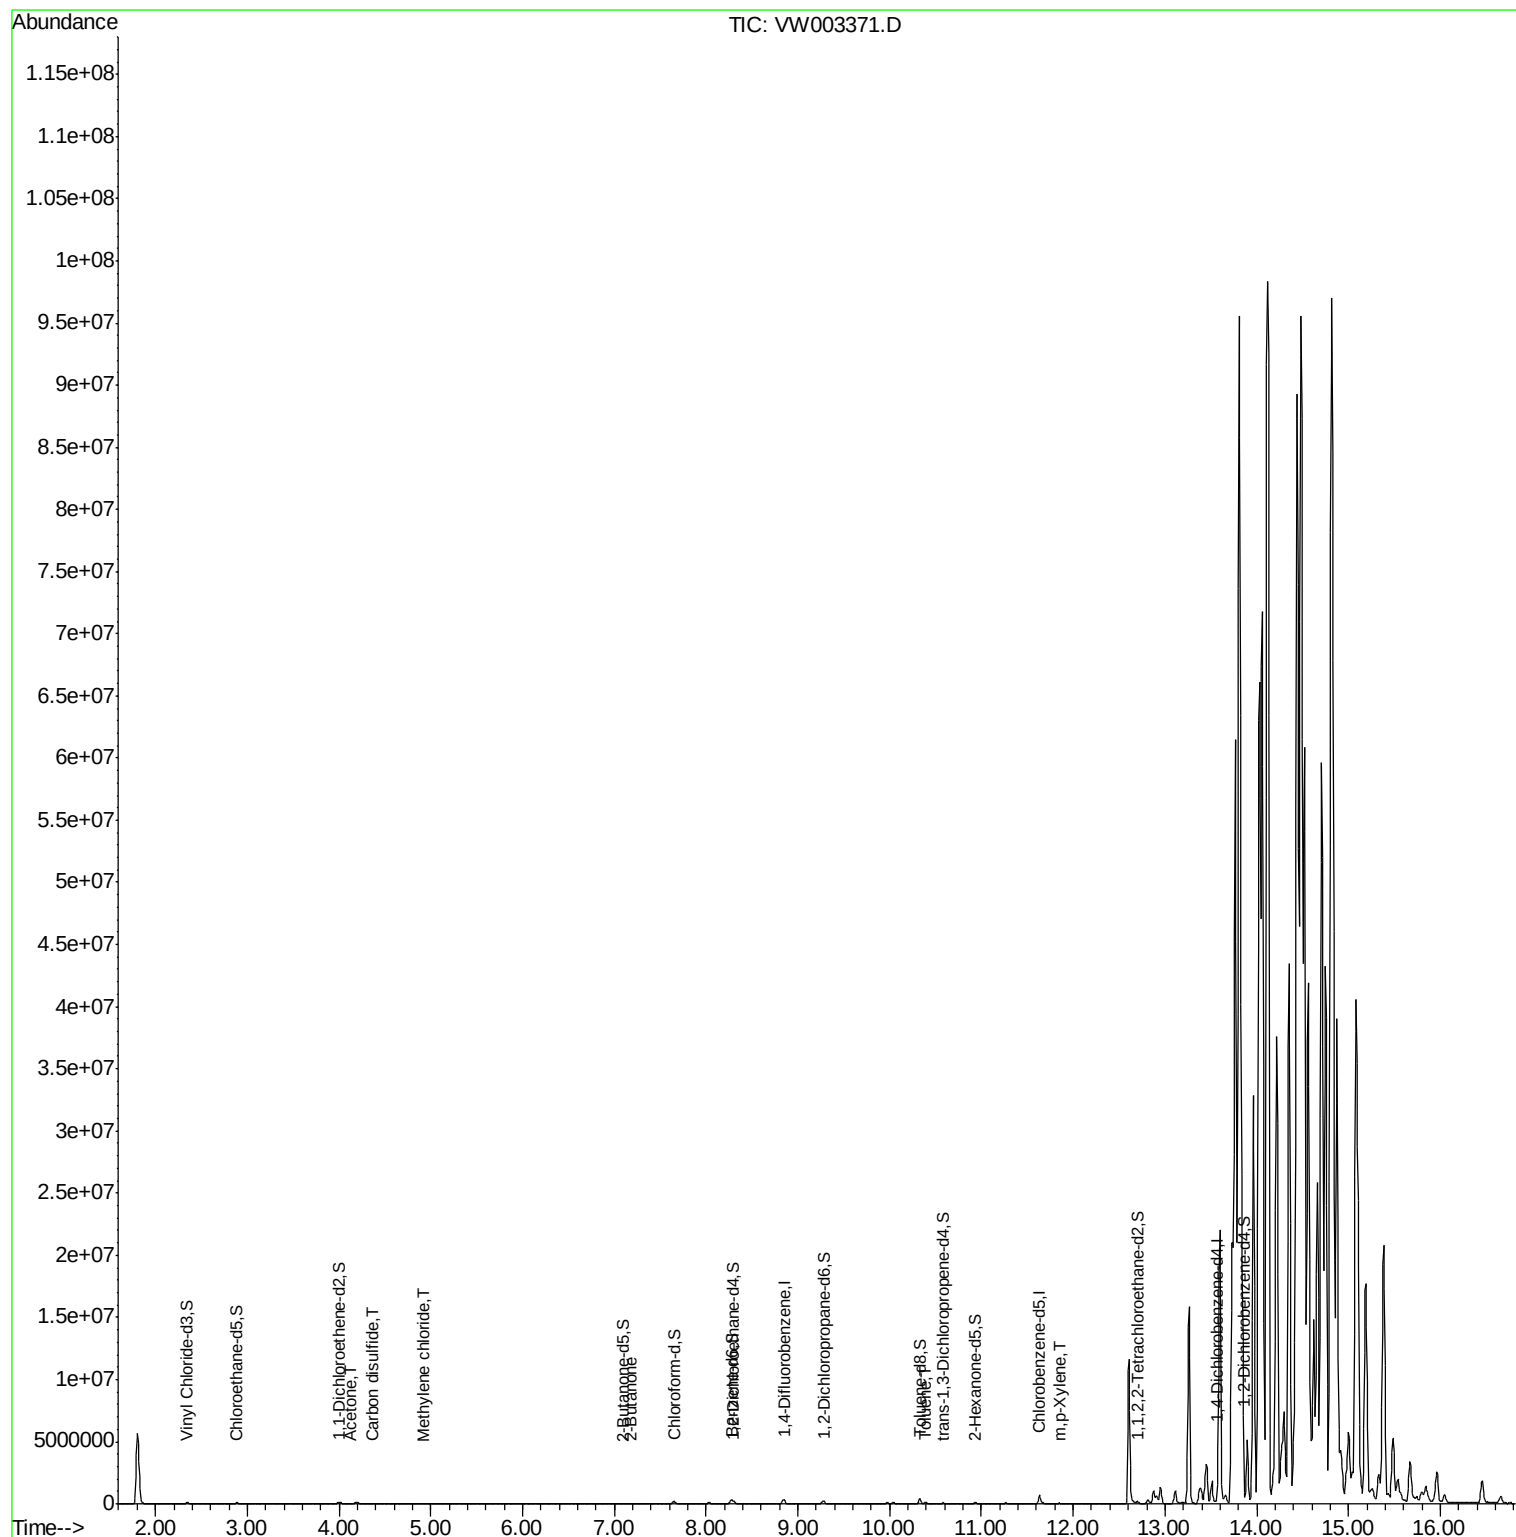

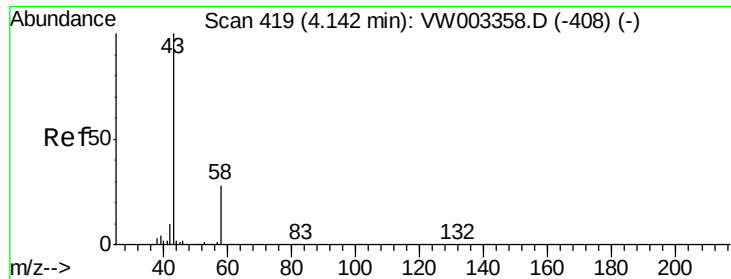





#13
Acetone
Concen: 84.50 ug/L
RT: 4.13 min Scan# 417
Delta R.T. -0.01 min
Lab File: VW003371.D
Acq: 20 Jun 2018 23:38

Instrument :
MSVOA_W
ClientSampleId :
DAXT1

Tot Ion	43	Resp	108033
Ion Ratio	43	100	Lower Upper
	58	21.8	0.0 58.6




Manual Integrations
APPROVED


MMDadoda
6/22/2018 4:56:06 PM

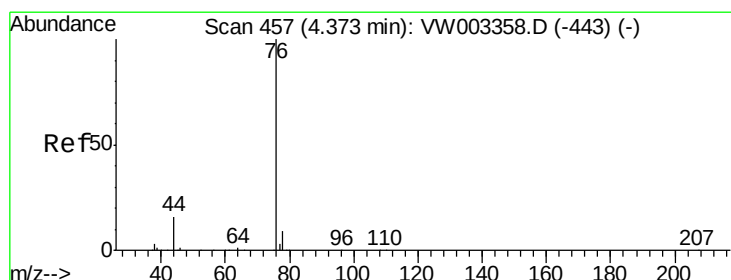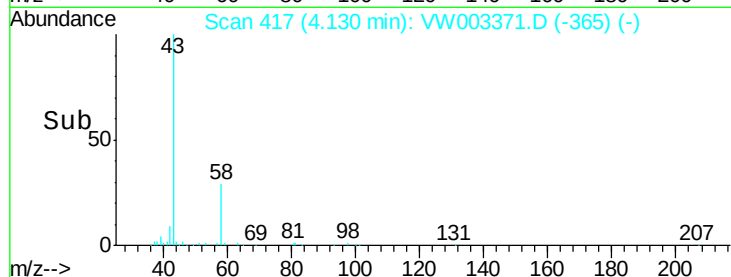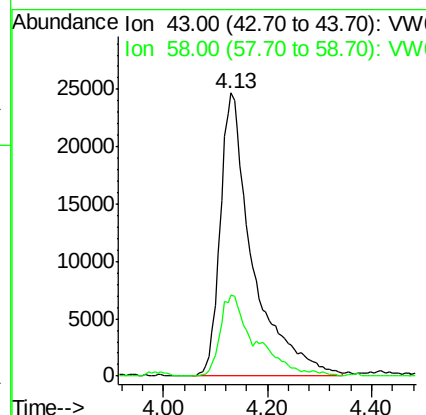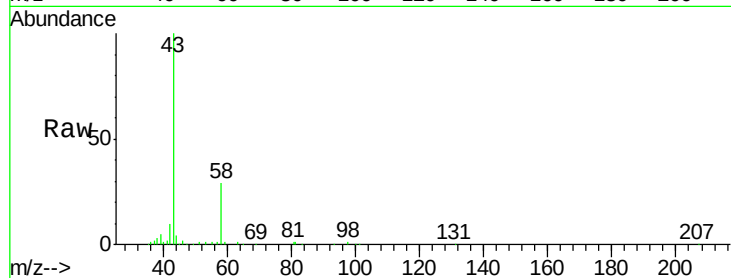

#14
Carbon disulfide
Concen: 7.20 ug/L
RT: 4.36 min Scan# 455
Delta R.T. -0.01 min
Lab File: VW003371.D
Acq: 20 Jun 2018 23:38

Tgt Ion	76	Resp	81465
Ion Ratio	76	100	Lower Upper
	78	8.8	7.3 10.9

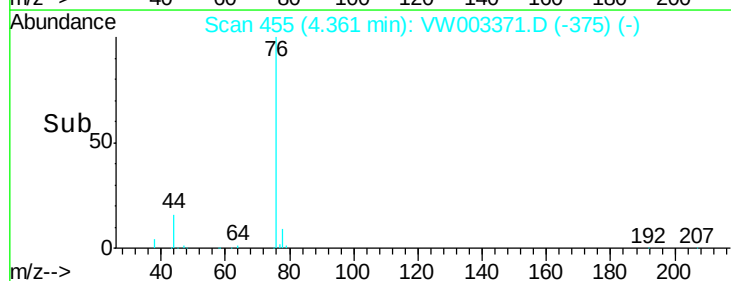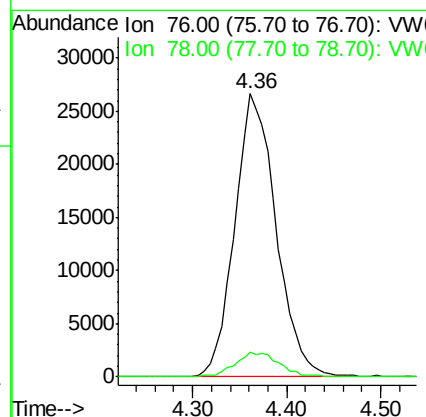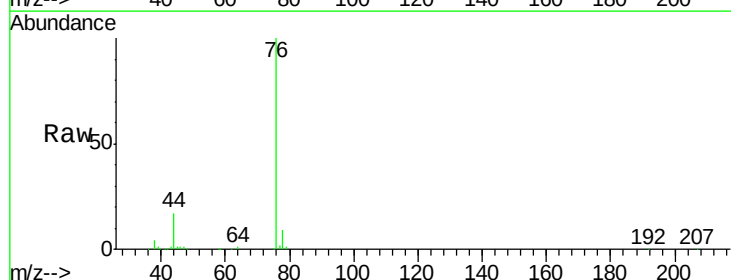

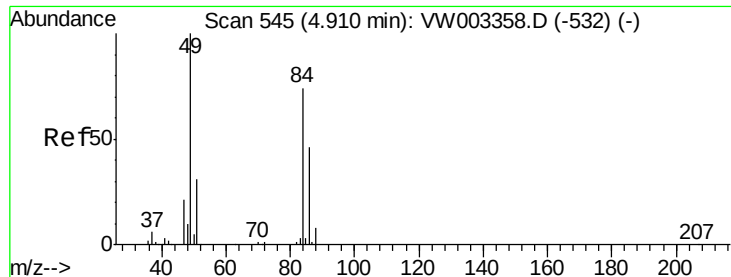





#16
Methylene chloride
Concen: 3.48 ug/L m
RT: 4.91 min Scan# 545
Delta R.T. -0.00 min
Lab File: VW003371.D
Acq: 20 Jun 2018 23:38

Instrument :
MSVOA_W
ClientSampled :
DAXT1

Tot Ion	84	Resp	13455
Ion Ratio	Lower	Upper	
84	100		
49	108.3	88.7	164.7
86	54.7	44.2	82.0




Manual Integrations
APPROVED


MMDadoda
6/22/2018 4:56:06 PM

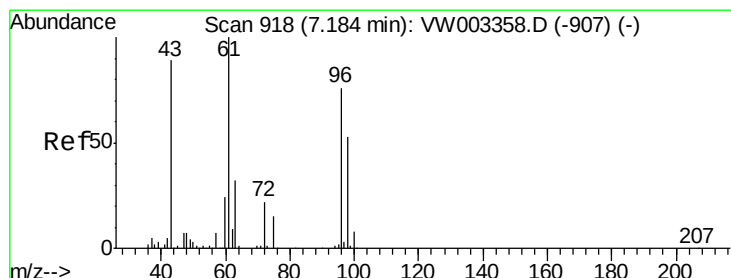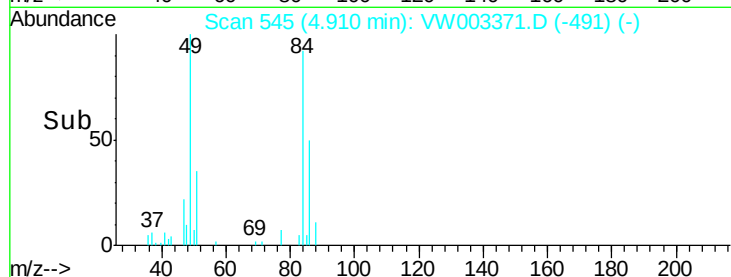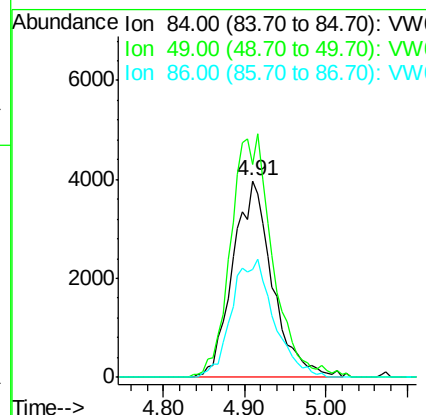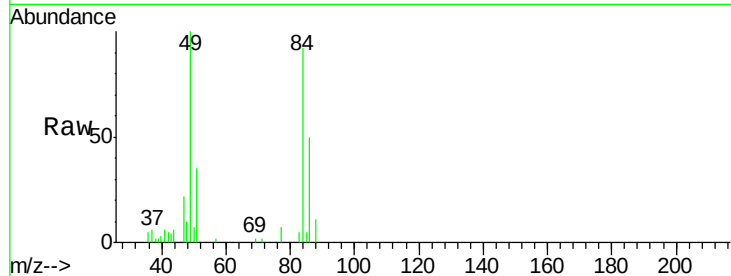

#21
2-Butanone
Concen: 37.76 ug/L
RT: 7.18 min Scan# 918
Delta R.T. -0.00 min
Lab File: VW003371.D
Acq: 20 Jun 2018 23:38

Tgt Ion	43	Resp	56734
Ion Ratio <td>Lower</td> <td>Upper</td> <td></td>	Lower	Upper	
43	100		
72	24.4	12.5	37.5

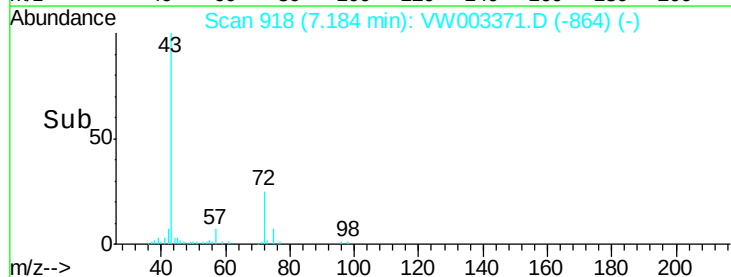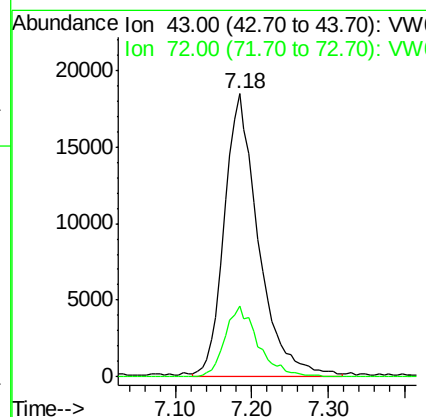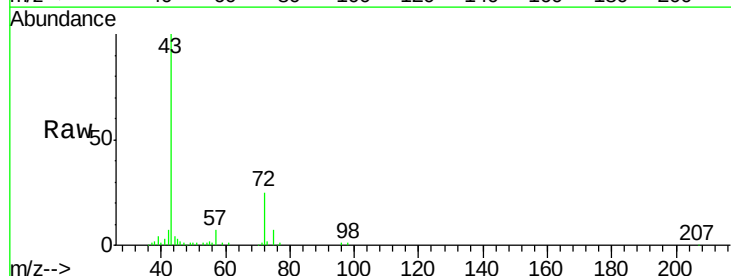

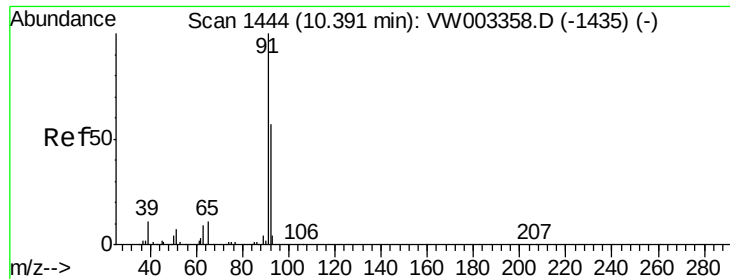

#44

Toluene

Concen: 7.48 ug/L

RT: 10.39 min Scan# 1444

Delta R.T. 0.00 min

Lab File: VW003371.D

Acq: 20 Jun 2018 23:38

Instrument :

MSVOA_W

ClientSampled :

DAXT1

Tot Ion: 91 Resp: 88114





Ion Ratio Lower Upper

91 100

92 59.6 39.5 73.4

Manual Integrations
APPROVED

MMDadoda
6/22/2018 4:56:06 PM

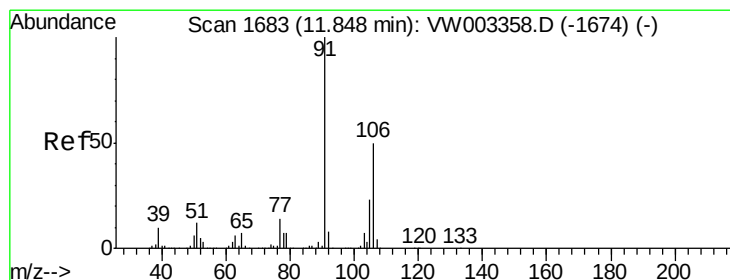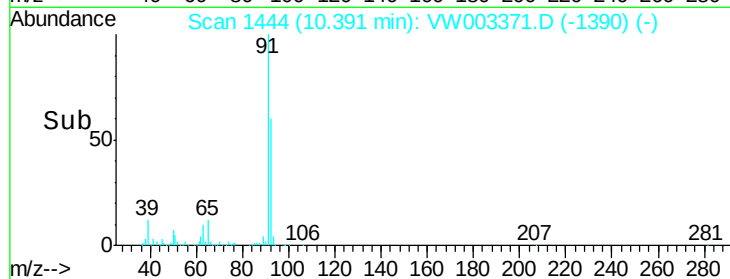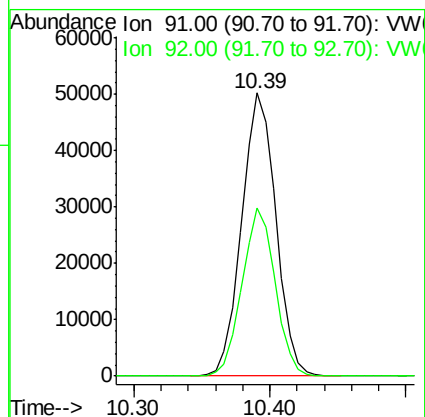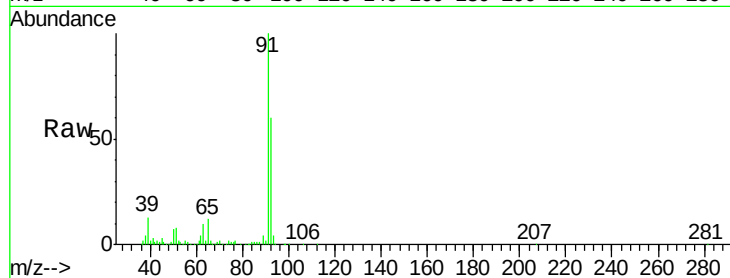

#54

m,p-Xylene

Concen: 2.05 ug/L

RT: 11.84 min Scan# 1682

Delta R.T. -0.01 min

Lab File: VW003371.D

Acq: 20 Jun 2018 23:38

Tgt Ion: 106 Resp: 10052

Ion Ratio Lower Upper

106 100

91 190.4 146.4 271.8

