

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062018\
 Data File : VW003372.D
 Acq On : 21 Jun 2018 00:04
 Operator : SY/AP
 Sample : J3569-19
 Misc : 4.73G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 DAXT2

Quant Time: Jun 21 06:55:52 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Jun 21 05:02:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.85	114	362579	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	261068	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.57	152	69227	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	138618	28.19	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	112.76%
7) Chloroethane-d5	2.89	69	101223	24.67	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.68%
10) 1,1-Dichloroethene-d2	4.00	63	196615	20.14	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	80.56%
20) 2-Butanone-d5	7.09	46	59589	38.46	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	76.92%
24) Chloroform-d	7.65	84	245536	25.74	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	102.96%
26) 1,2-Dichloroethane-d4	8.31	65	154419	27.25	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	109.00%
29) Benzene-d6	8.28	84	471885	34.07	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	136.28%#
33) 1,2-Dichloropropane-d6	9.28	67	155714	35.51	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	142.04%#
37) Toluene-d8	10.33	98	393223	29.69	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	118.76%
38) trans-1,3-Dichloropropene-	10.58	79	30439	14.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	59.16%
39) 2-Hexanone-d5	10.93	63	23415	26.13	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	52.26%
48) 1,1,2,2-Tetrachloroethane-	12.70	84	92802	22.75	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.00%
61) 1,2-Dichlorobenzene-d4	13.86	152	61003	23.33	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.32%


Target Compounds					Ovalue
13) Acetone	4.15	43	12995	7.87 ug/L	79


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW062018\
Data File : VW003372.D
Acq On : 21 Jun 2018 00:04
Operator : SY/AP
Sample : J3569-19
Misc : 4.73G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
DAXT2

Quant Time: Jun 21 06:55:52 2018
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM062018S.M
Quant Title : VOC Analysis
QLast Update : Thu Jun 21 05:02:42 2018
Response via : Initial Calibration

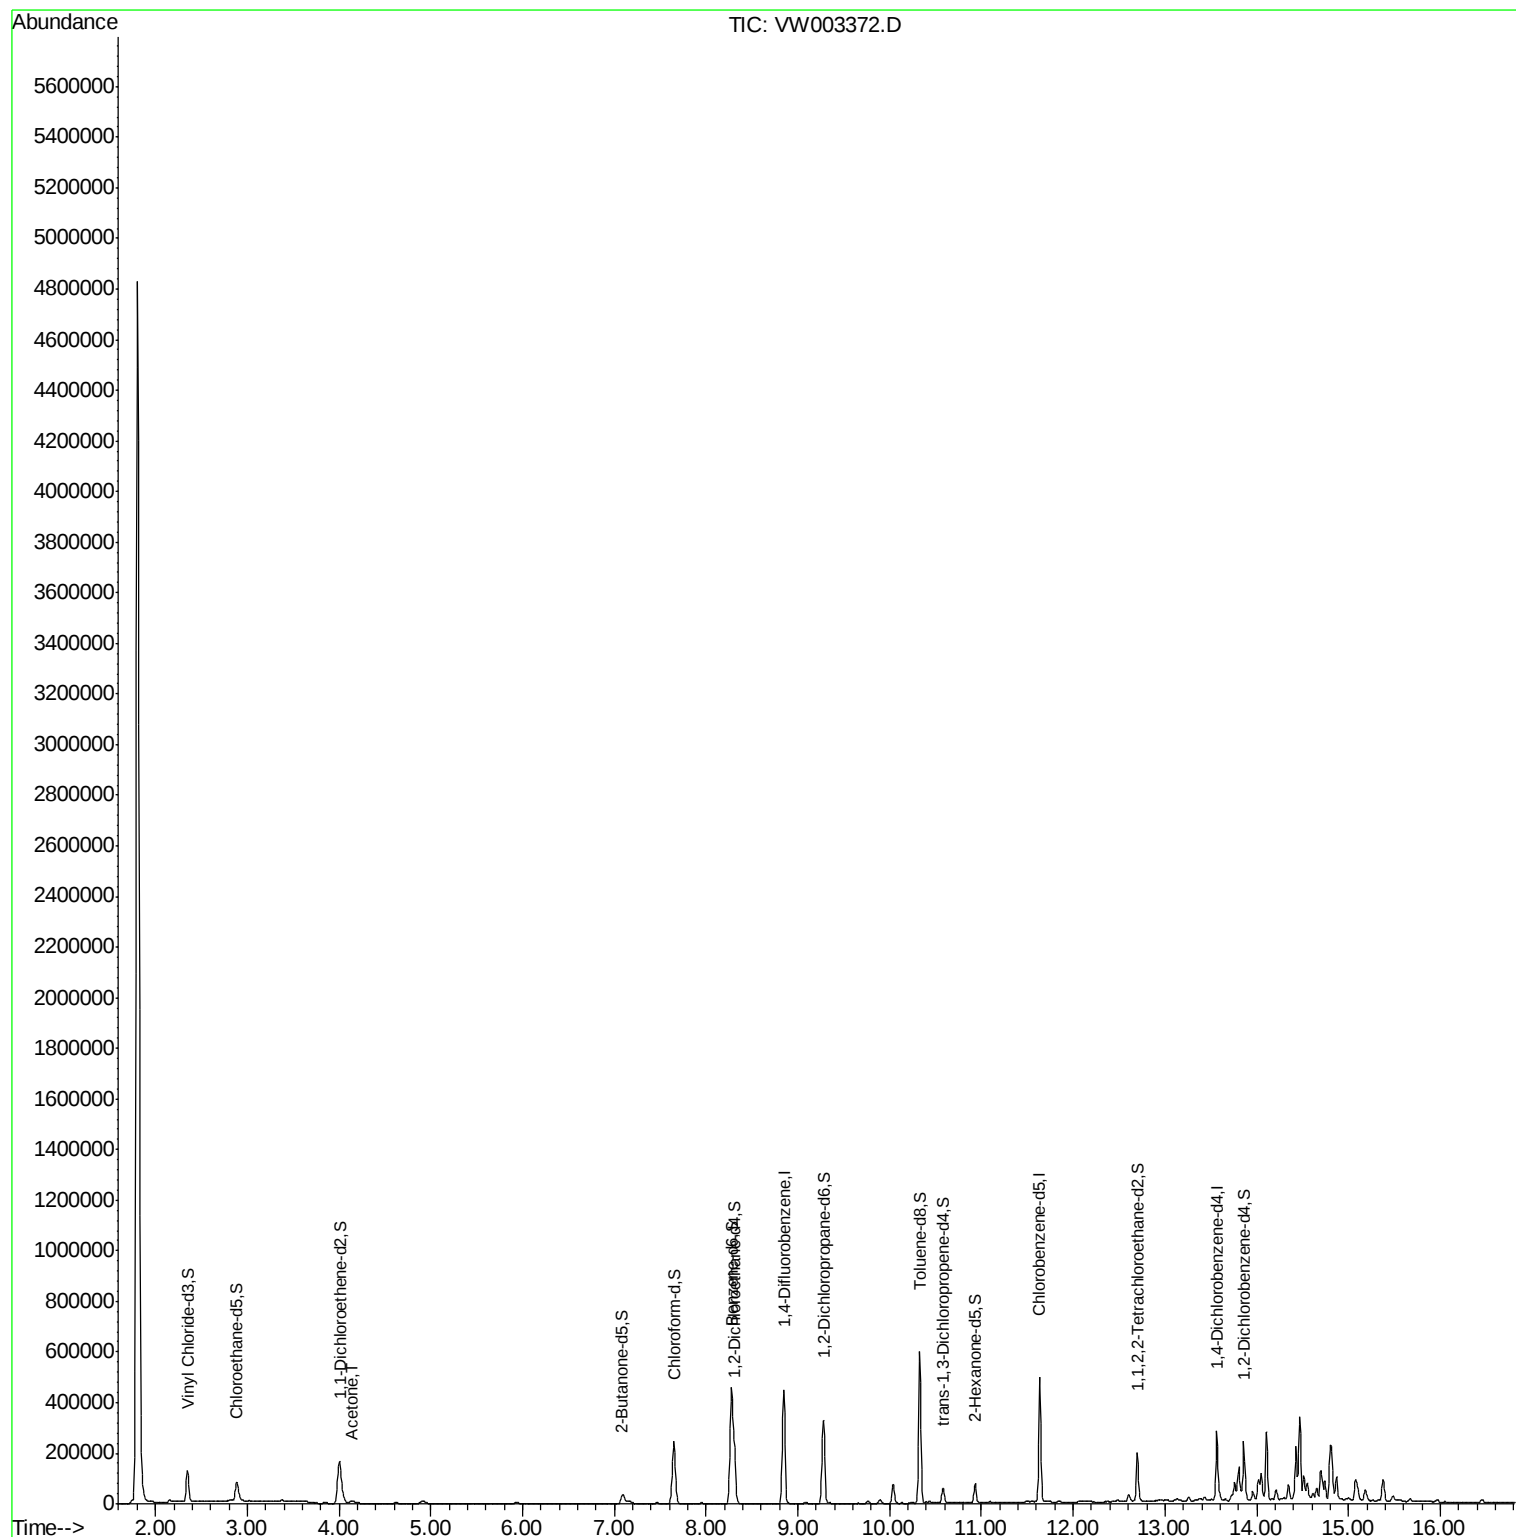

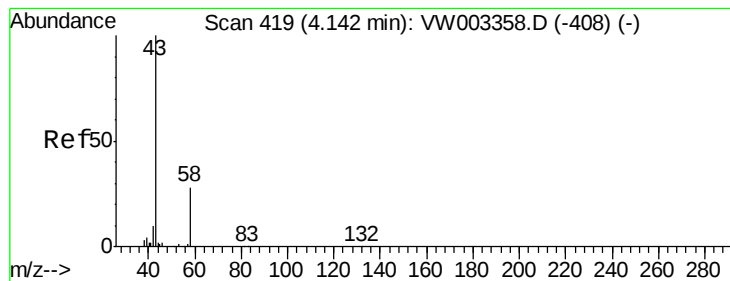

#13

Acetone

Concen: 7.87 ug/L

RT: 4.15 min Scan# 420

Delta R.T. 0.01 min

Lab File: VW003372.D

Acq: 21 Jun 2018 00:04

Instrument :

MSVOA_W

ClientSampleId :

DAXT2

Tot Ion: 43 Resp: 12995

Ion Ratio Lower Upper

43 100

58 18.1 0.0 58.6

