




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062023\
 Data File : VW026263.D
 Acq On : 20 Jun 2023 12:32
 Operator : SY/MD
 Sample : 03334-10
 Misc : 4.31g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YBW14

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/22/2023
 Supervised By :Mahesh Dadoda 06/22/2023

Quant Time: Jun 21 01:11:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 21 01:09:17 2023
 Response via : Initial Calibration

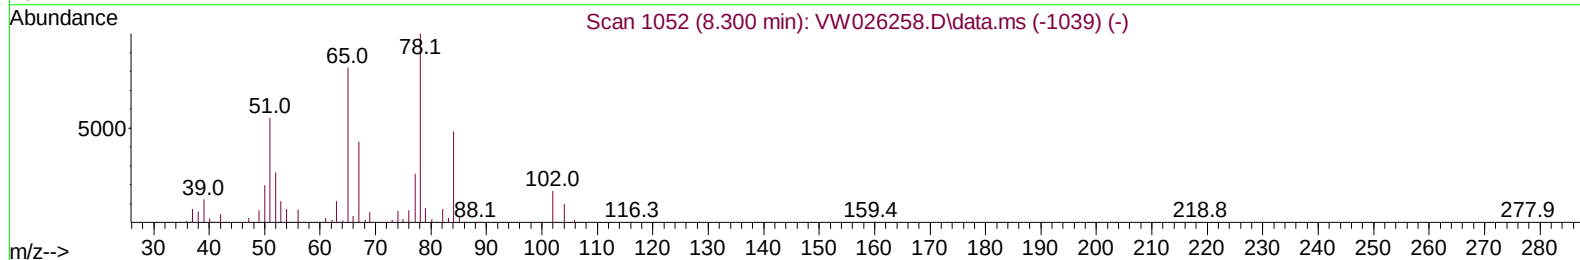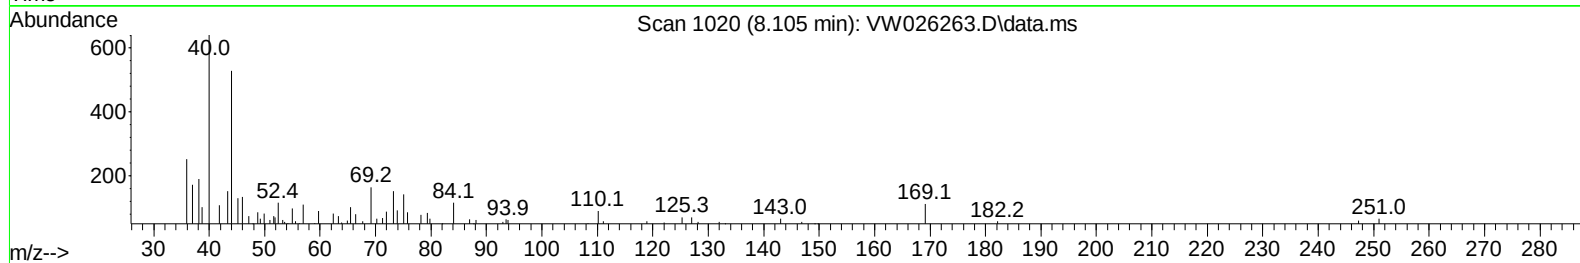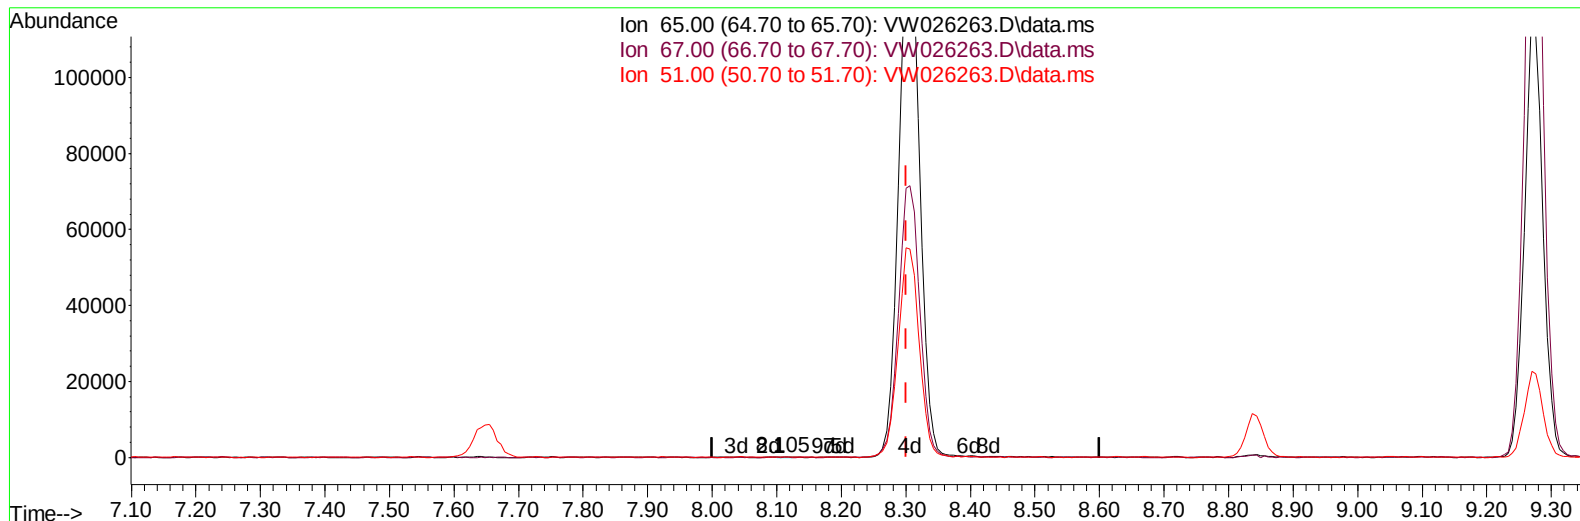

TIC: VW026263.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.105min (-0.195) 0.01 ug/L

response 130

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.70	46.15
51.00	106.50	93.85
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062023\
 Data File : VW026263.D
 Acq On : 20 Jun 2023 12:32
 Operator : SY/MD
 Sample : 03334-10
 Misc : 4.31g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YBW14

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/22/2023
 Supervised By :Mahesh Dadoda 06/22/2023

Quant Time: Jun 21 01:11:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 21 01:09:17 2023
 Response via : Initial Calibration

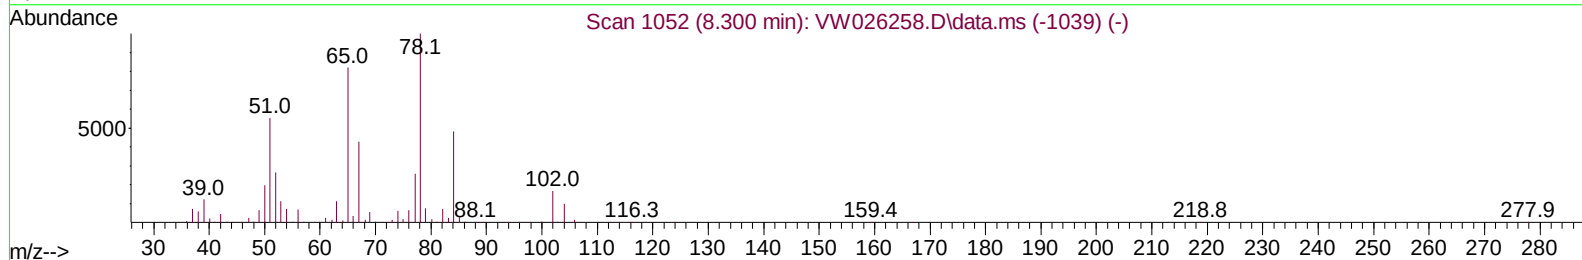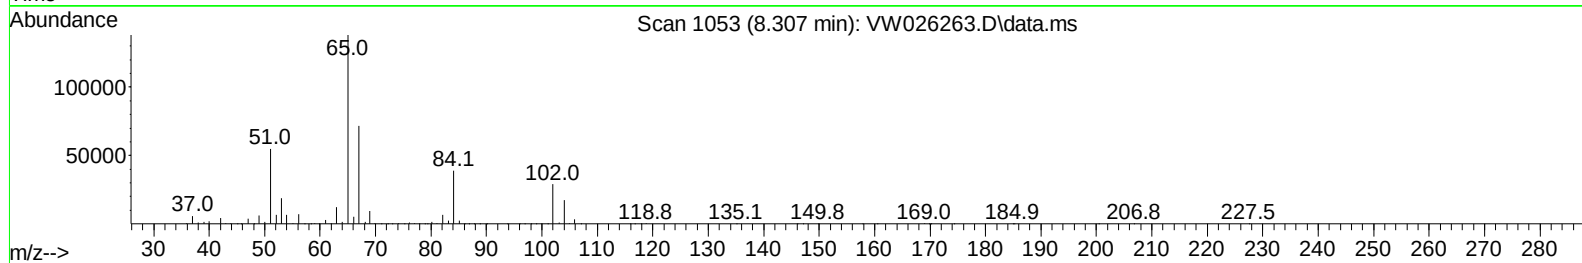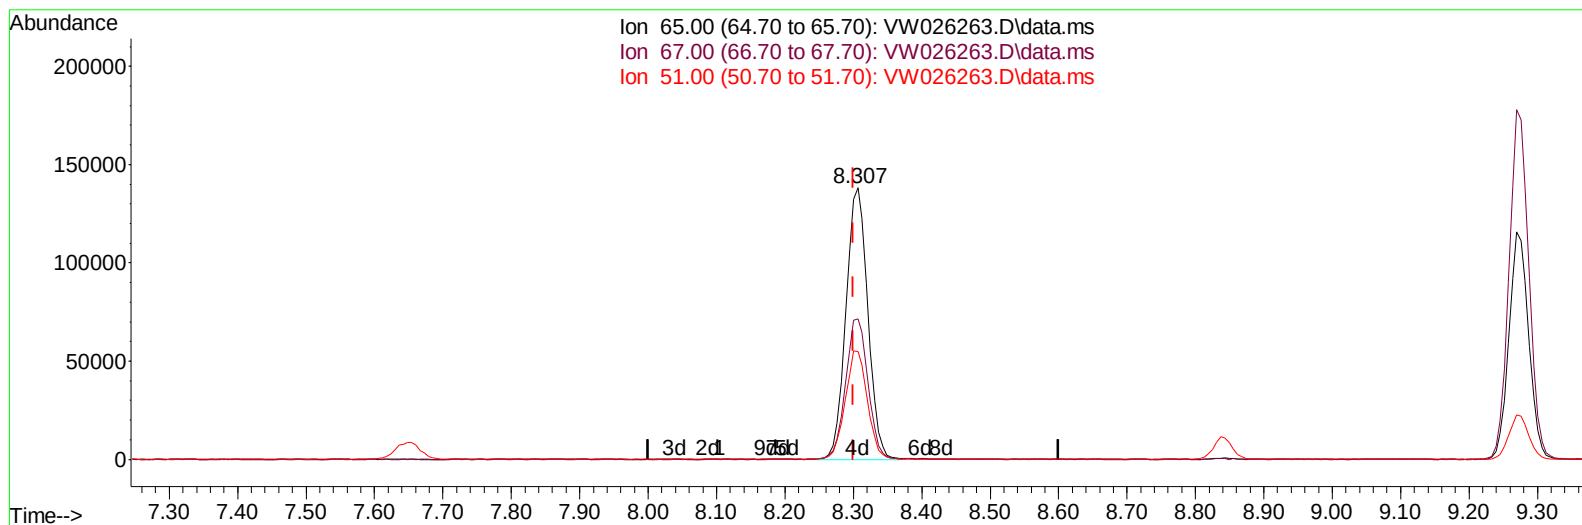

TIC: VW026263.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.006) 20.96 ug/L m

response 307017

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	52.70	0.02#
51.00	106.50	0.04#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062023\
 Data File : VW026263.D
 Acq On : 20 Jun 2023 12:32
 Operator : SY/MD
 Sample : 03334-10
 Misc : 4.31g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YBW14

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/22/2023
 Supervised By :Mahesh Dadoda 06/22/2023

Quant Time: Jun 21 01:11:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 21 01:09:17 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		914894	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		818429	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		368069	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		197779	15.367	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	61.480%		
7) Chloroethane-d5	2.893	69		193944	20.130	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	80.520%		
11) 1,1-Dichloroethene-d2	4.021	65		107141	16.882	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	67.520%		
21) 2-Butanone-d5	7.075	46		191112	51.003	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	102.000%		
24) Chloroform-d	7.648	84		534917	19.966	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	79.880%		
26) 1,2-Dichloroethane-d4	8.307	65		307017m	20.957	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	83.840%		
32) Benzene-d6	8.276	84		1050045	19.067	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	76.280%		
36) 1,2-Dichloropropane-d6	9.270	67		355442	20.373	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	81.480%		
41) Toluene-d8	10.318	98		887773	18.178	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	72.720%		
43) trans-1,3-Dichloroprop...	10.575	79		121363	17.554	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	70.200%		
47) 2-Hexanone-d5	10.922	63		125098	45.473	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	90.940%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		287410	22.638	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	90.560%		
66) 1,2-Dichlorobenzene-d4	13.848	152		283324	20.111	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	80.440%		
Target Compounds							
13) Acetone	4.124	43		7951	2.742	ug/L	Qvalue 78

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062023\
Data File : VW026263.D
Acq On : 20 Jun 2023 12:32
Operator : SY/MD
Sample : 03334-10
Misc : 4.31g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YBW14

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/22/2023
Supervised By :Mahesh Dadoda 06/22/2023

Quant Time: Jun 21 01:11:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 21 01:09:17 2023
Response via : Initial Calibration

