

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062023\
 Data File : VW026262.D
 Acq On : 20 Jun 2023 12:08
 Operator : SY/MD
 Sample : 03334-09
 Misc : 4.69g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YBW13

Quant Time: Jun 21 01:11:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 21 01:09:17 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	738267	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	635936	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	245309	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	167523	16.130	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.520%
7) Chloroethane-d5	2.893	69	163554	21.037	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.160%
11) 1,1-Dichloroethene-d2	4.015	65	90167	17.607	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.440%
21) 2-Butanone-d5	7.075	46	189105	62.541	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	125.080%
24) Chloroform-d	7.648	84	451762	20.896	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.600%
26) 1,2-Dichloroethane-d4	8.307	65	270367	22.870	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.480%
32) Benzene-d6	8.270	84	876593	20.485	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.960%
36) 1,2-Dichloropropane-d6	9.270	67	303864	22.414	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.640%
41) Toluene-d8	10.325	98	718467	18.933	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.720%
43) trans-1,3-Dichloroprop...	10.575	79	104460	19.445	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	77.760%
47) 2-Hexanone-d5	10.922	63	118188	55.290	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	110.580%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	268441	27.211	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	108.840%
66) 1,2-Dichlorobenzene-d4	13.848	152	198740	21.166	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.680%
Target Compounds						
13) Acetone	4.124	43	14843	6.344	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062023\
Data File : VW026262.D
Acq On : 20 Jun 2023 12:08
Operator : SY/MD
Sample : 03334-09
Misc : 4.69g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YBW13

Quant Time: Jun 21 01:11:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 21 01:09:17 2023
Response via : Initial Calibration

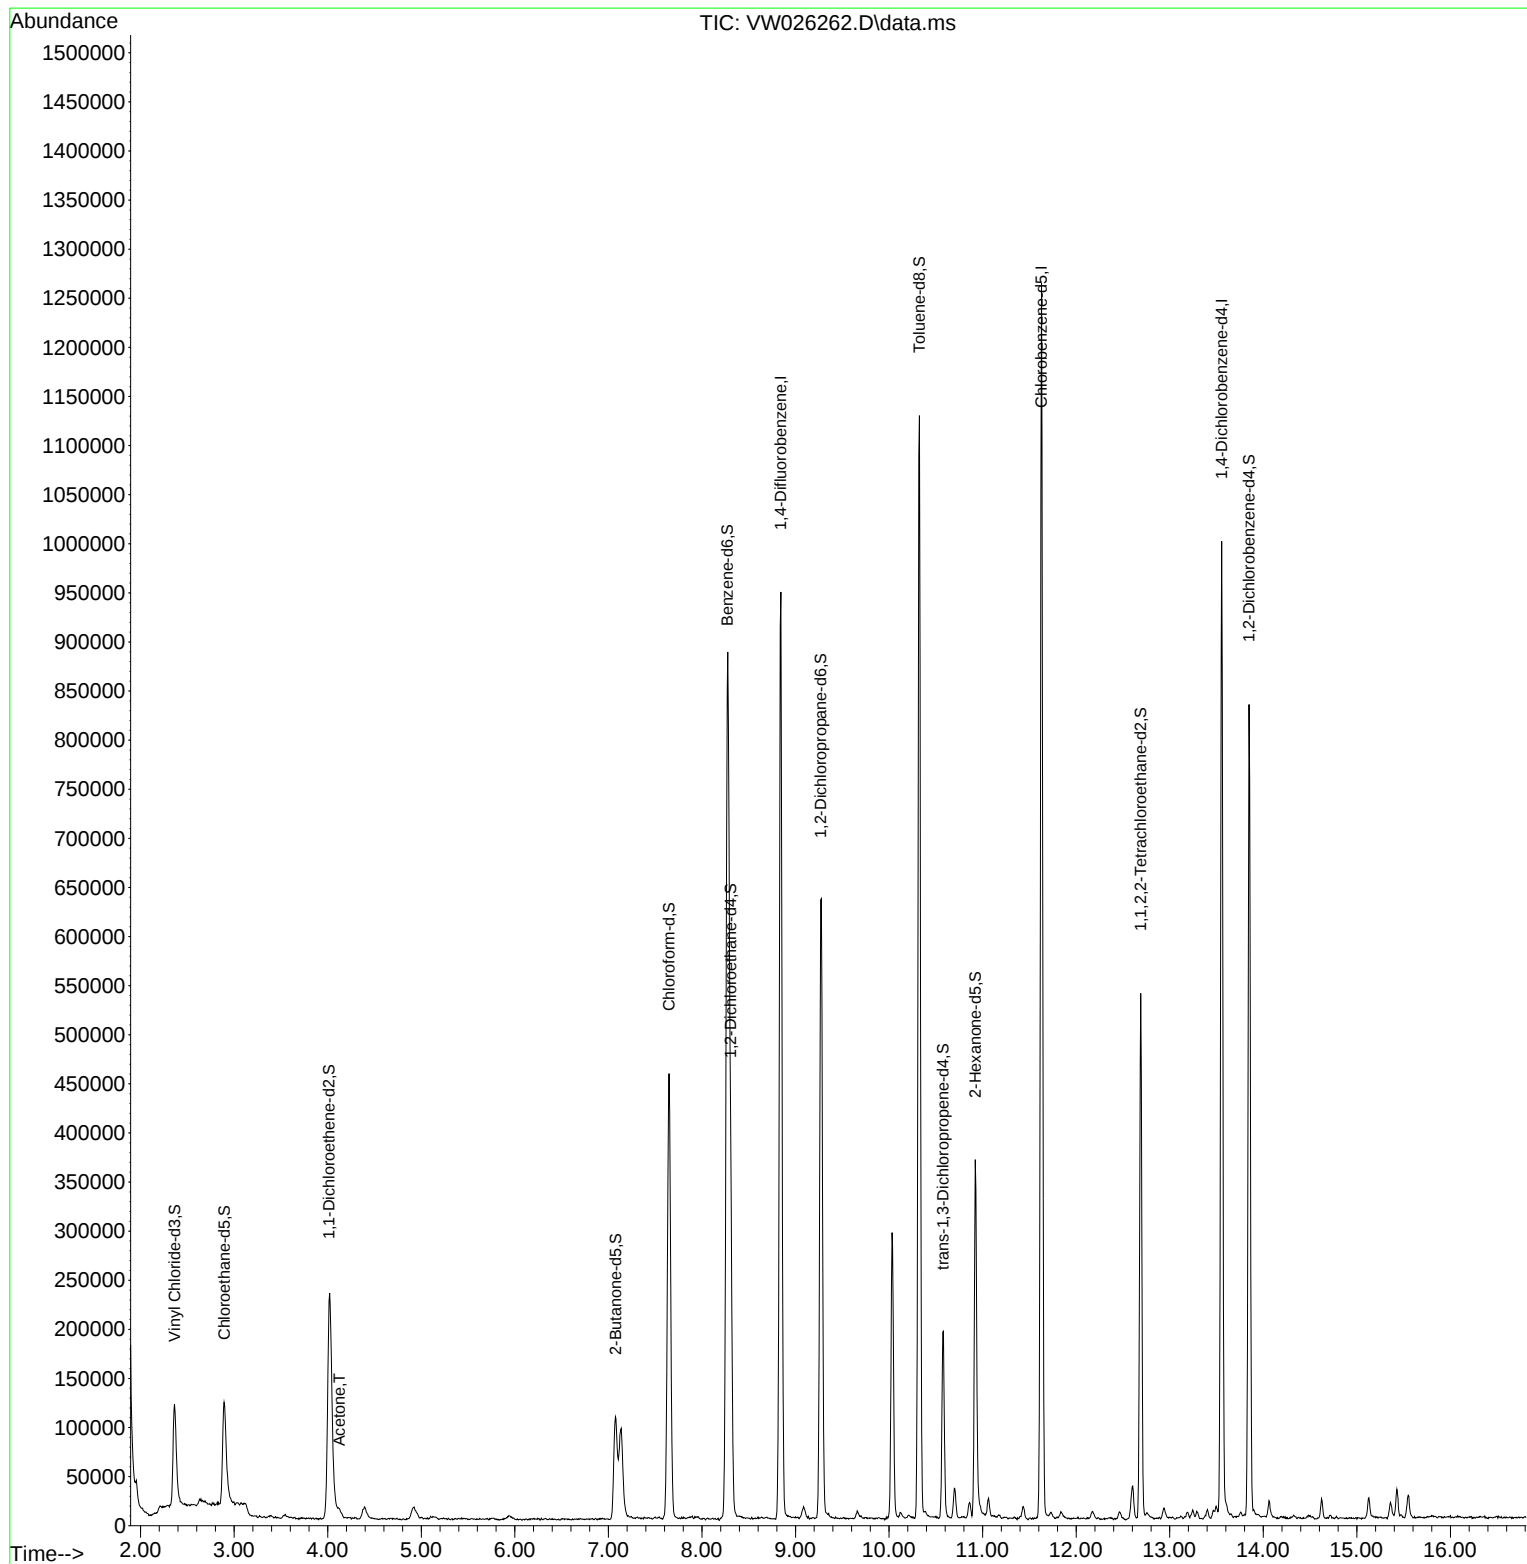

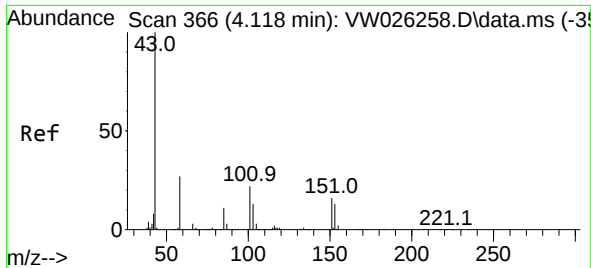

#13

Acetone

Concen: 6.344 ug/L

RT: 4.124 min Scan# 3

Delta R.T. 0.006 min

Lab File: VW026262.D

Acq: 20 Jun 2023 12:08

Instrument :

MSVOA_W

ClientSampleId :

YBW13

Tgt Ion: 43 Resp: 14843

Ion Ratio Lower Upper

43 100

58 28.8 0.0 58.2

