

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062023\
 Data File : VW026263.D
 Acq On : 20 Jun 2023 12:32
 Operator : SY/MD
 Sample : 03334-10
 Misc : 4.31g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YBW14

Manual Integrations
 APPROVED

Reviewed By :Semsettin Yesilyurt 06/22/2023
 Supervised By :Mahesh Dadoda 06/22/2023

Quant Time: Jun 21 01:11:51 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 21 01:09:17 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	914894	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	818429	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	368069	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	197779	15.367	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	61.480%		
7) Chloroethane-d5	2.893	69	193944	20.130	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	80.520%		
11) 1,1-Dichloroethene-d2	4.021	65	107141	16.882	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	67.520%		
21) 2-Butanone-d5	7.075	46	191112	51.003	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	102.000%		
24) Chloroform-d	7.648	84	534917	19.966	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	79.880%		
26) 1,2-Dichloroethane-d4	8.307	65	307017m	20.957	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	83.840%		
32) Benzene-d6	8.276	84	1050045	19.067	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	76.280%		
36) 1,2-Dichloropropane-d6	9.270	67	355442	20.373	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	81.480%		
41) Toluene-d8	10.318	98	887773	18.178	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	72.720%		
43) trans-1,3-Dichloroprop...	10.575	79	121363	17.554	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	70.200%		
47) 2-Hexanone-d5	10.922	63	125098	45.473	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	90.940%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	287410	22.638	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	90.560%		
66) 1,2-Dichlorobenzene-d4	13.848	152	283324	20.111	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	80.440%		
Target Compounds					Qvalue	
13) Acetone	4.124	43	7951	2.742	ug/L	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062023\
Data File : VW026263.D
Acq On : 20 Jun 2023 12:32
Operator : SY/MD
Sample : 03334-10
Misc : 4.31g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
YBW14

Quant Time: Jun 21 01:11:51 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 21 01:09:17 2023
Response via : Initial Calibration

Manual Integrations
APPROVED

Reviewed By :Semsettin Yesilyurt 06/22/2023
Supervised By :Mahesh Dadoda 06/22/2023

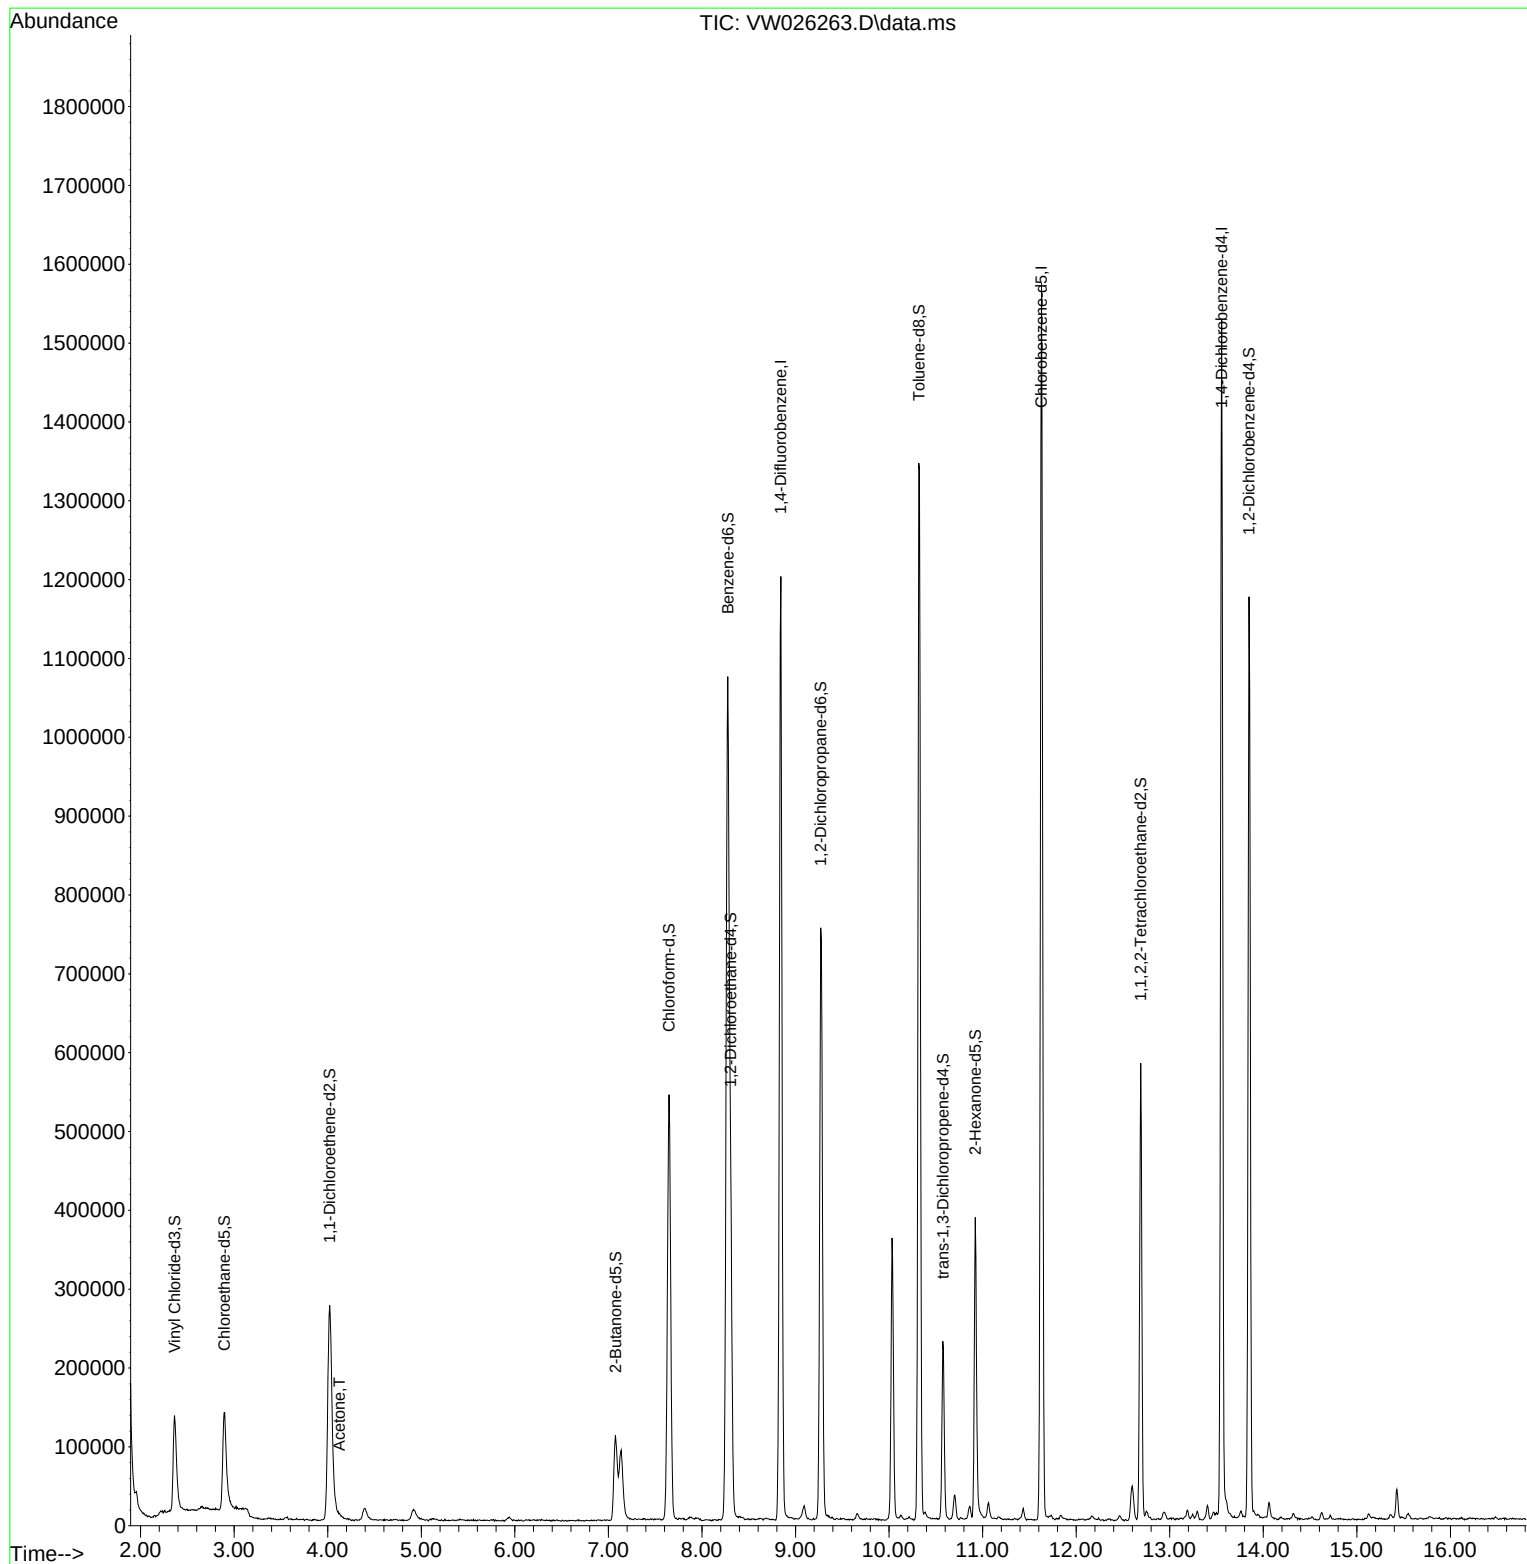

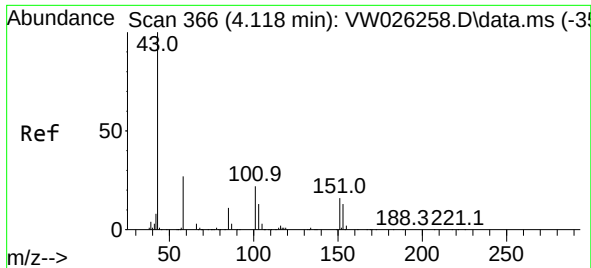

#13

Acetone

Concen: 2.742 ug/L

RT: 4.124 min Scan# 30

Delta R.T. 0.006 min

Lab File: VW026263.D

Acq: 20 Jun 2023 12:32

Instrument :

MSVOA_W

ClientSampleId :

YBW14

Tgt Ion: 43 Resp: 795

Ion Ratio Lower Upper

43 100

58 17.2 0.0 58.2

Manual Integrations

APPROVED

Reviewed By :Semsettin Yesilyurt 06/22/2023

Supervised By :Mahesh Dadoda 06/22/2023

