

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062023\
 Data File : VW026265.D
 Acq On : 20 Jun 2023 13:20
 Operator : SY/MD
 Sample : 03334-17
 Misc : 4.59g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 YBW21

Quant Time: Jun 21 01:12:16 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 21 01:09:17 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	774850	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	644401	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	248139	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	168648	15.472	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.880%
7) Chloroethane-d5	2.893	69	168442	20.643	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.560%
11) 1,1-Dichloroethene-d2	4.021	65	89163	16.589	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	66.360%
21) 2-Butanone-d5	7.075	46	194559	61.307	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	122.620%
24) Chloroform-d	7.648	84	471063	20.760	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.040%
26) 1,2-Dichloroethane-d4	8.307	65	271710	21.899	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	87.600%
32) Benzene-d6	8.276	84	898095	20.712	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	82.840%
36) 1,2-Dichloropropane-d6	9.270	67	308281	22.441	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.760%
41) Toluene-d8	10.325	98	708892	18.435	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	73.720%
43) trans-1,3-Dichloroprop...	10.581	79	92235	16.944	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	67.760%
47) 2-Hexanone-d5	10.922	63	116413	53.744	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.480%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	258967	25.906	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	103.640%
66) 1,2-Dichlorobenzene-d4	13.848	152	189635	19.966	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	79.880%
Target Compounds					Qvalue	
13) Acetone	4.118	43	42142	17.162	ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062023\
Data File : VW026265.D
Acq On : 20 Jun 2023 13:20
Operator : SY/MD
Sample : 03334-17
Misc : 4.59g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
YBW21

Quant Time: Jun 21 01:12:16 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 21 01:09:17 2023
Response via : Initial Calibration

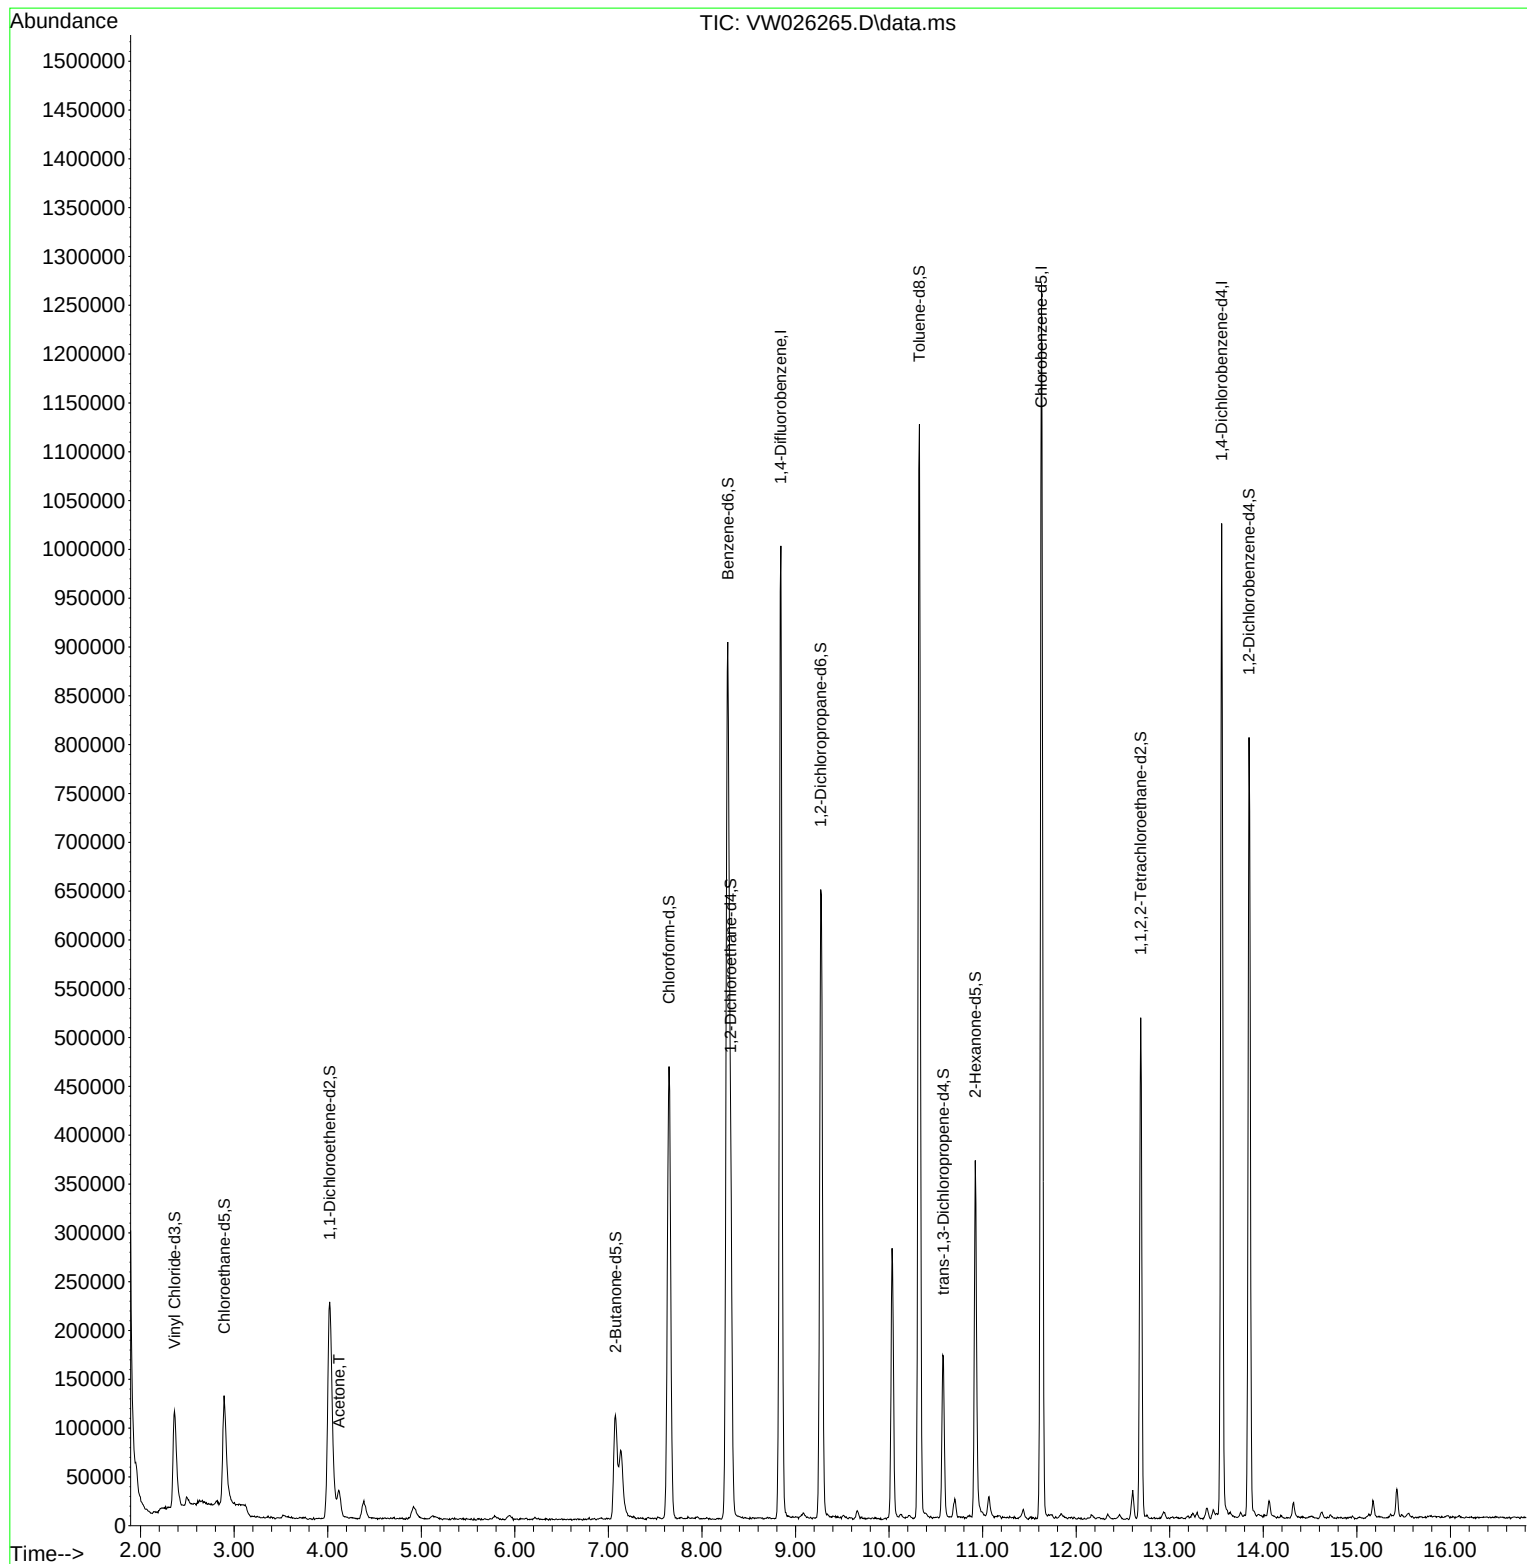

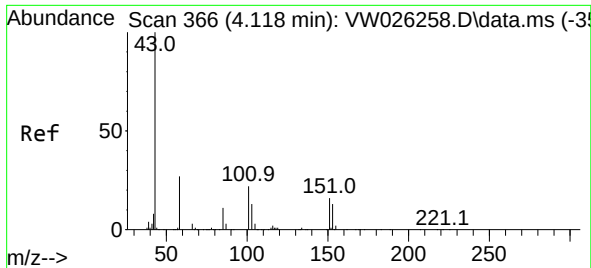

#13
 Acetone
 Concen: 17.162 ug/L
 RT: 4.118 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW026265.D
 Acq: 20 Jun 2023 13:20

Instrument :
 MSVOA_W
 ClientSampleId :
 YBW21

Tgt Ion: 43 Resp: 42142
 Ion Ratio Lower Upper
 43 100
 58 29.3 0.0 58.2

