
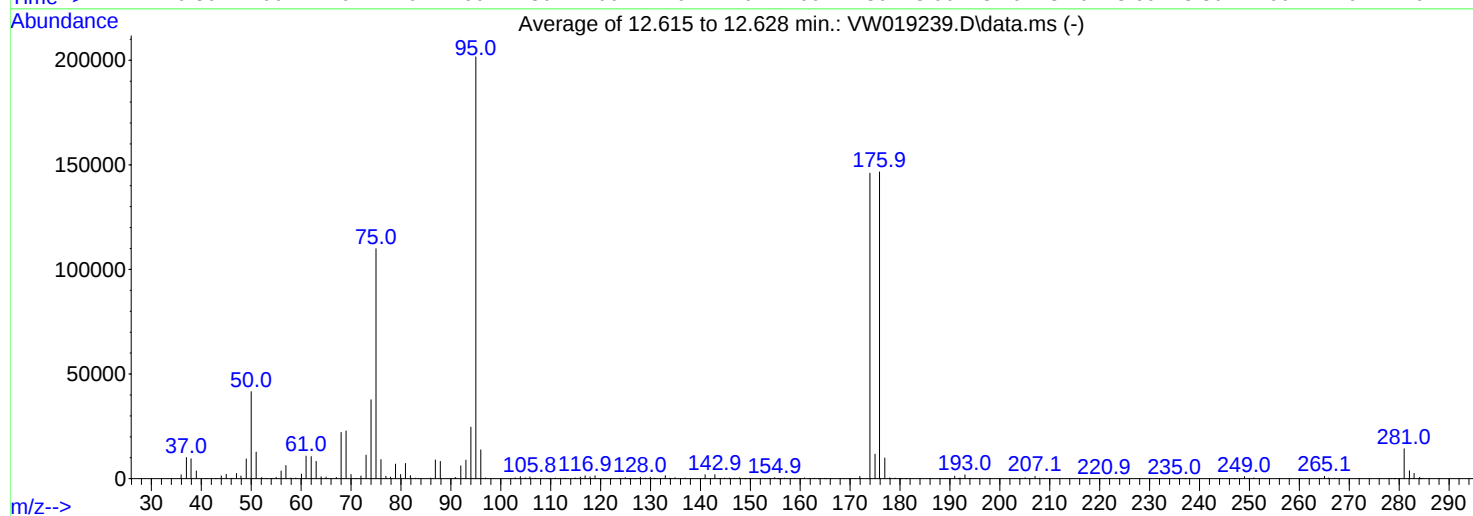


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062121\
Data File : VW019239.D
Acq On : 21 Jun 2021 08:46
Operator : SY/VA
Sample : BFB
Misc : 5.00G/5ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\82W062121S.M
Title : SW846 8260
Last Update : Mon Jun 21 12:12:47 2021

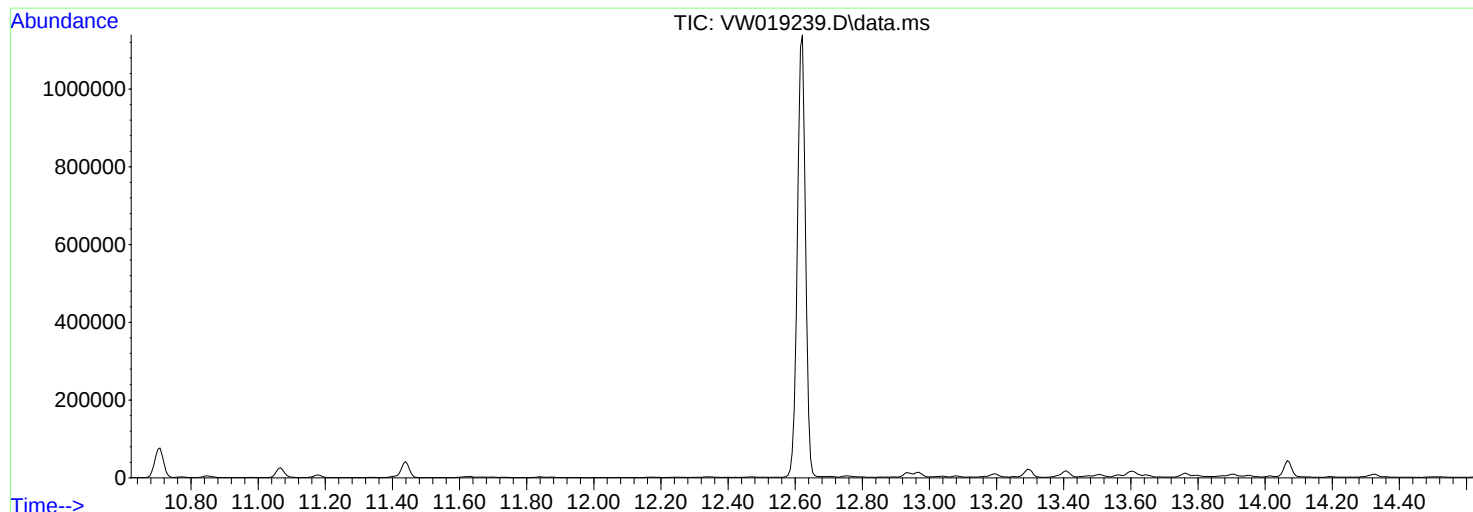

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.6	41595	PASS
75	95	30	60	54.5	109877	PASS
95	95	100	100	100.0	201600	PASS
96	95	5	9	6.8	13789	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	72.4	145984	PASS
175	174	5	9	8.0	11708	PASS
176	174	95	101	100.4	146584	PASS
177	176	5	9	6.7	9841	PASS