
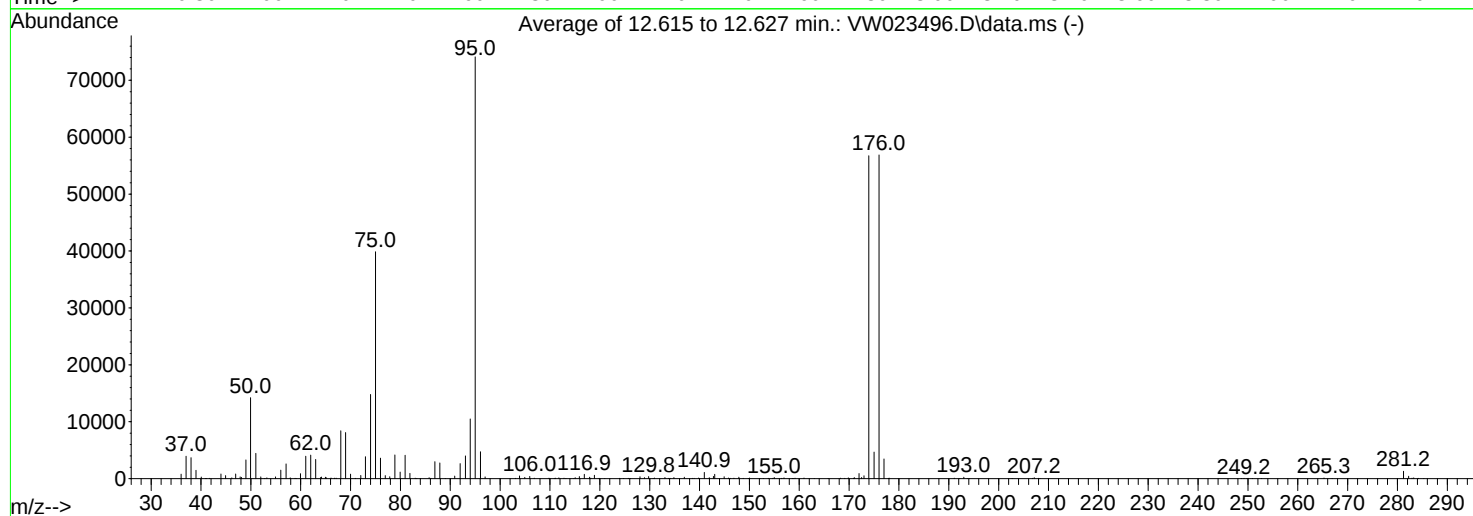


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062122\
 Data File : VW023496.D
 Acq On : 21 Jun 2022 07:40
 Operator : SY/VA
 Sample : BFB574
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB574

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061022SMA.M
 Title : SFAM01.0
 Last Update : Wed Jun 22 01:04:18 2022

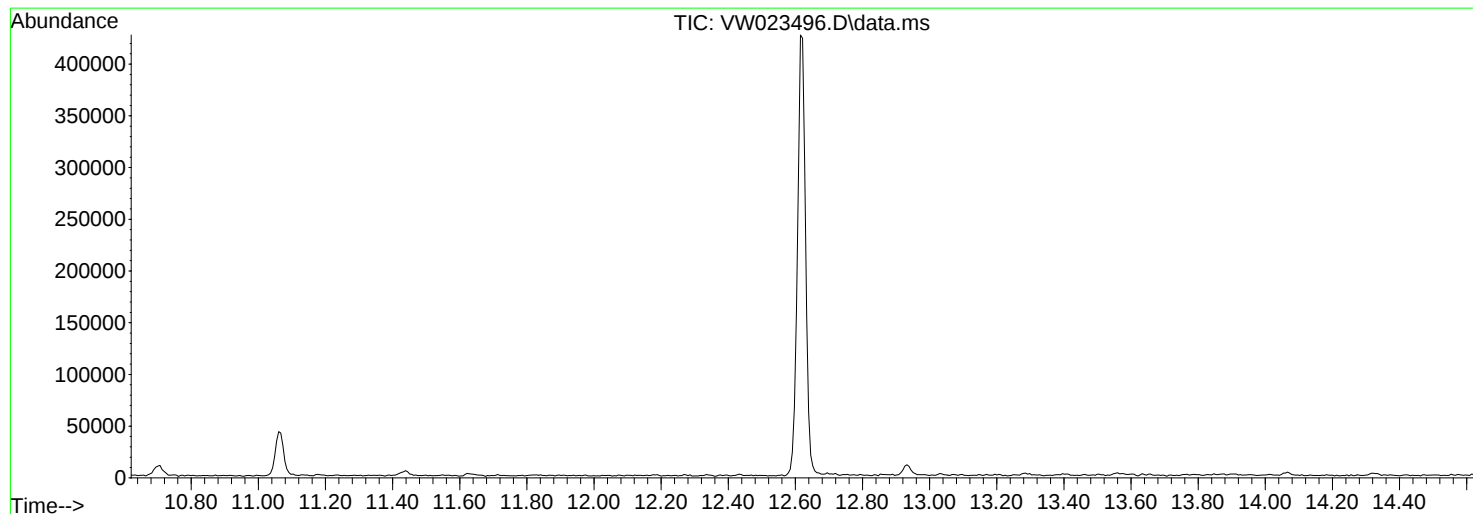

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	14219	PASS
75	95	30	80	53.8	39875	PASS
95	95	100	100	100.0	74125	PASS
96	95	5	9	6.4	4730	PASS
173	174	0.00	2	0.9	515	PASS
174	95	50	120	76.6	56747	PASS
175	174	5	9	8.2	4673	PASS
176	174	95	105	100.2	56869	PASS
177	176	5	10	6.1	3465	PASS

m/z	Abundance
35.40	80.0
37.70	50.0
38.40	89.0
39.00	98.0
39.70	186.0
42.00	53.0
43.00	105.0
44.20	108.0
45.10	70.0
45.60	80.0
46.70	69.0
49.80	116.0
51.60	58.0
54.50	65.0
55.70	106.0
59.70	65.0
73.00	58.0
83.00	88.0
86.60	59.0
125.80	66.0
139.20	78.0
179.00	71.0
201.50	76.0

Instrument :
MSVOA_W
ClientSampleId :
BFB574

m/z	Abundance
35.90	992.0
37.00	4323.0
38.00	3942.0
39.10	1956.0
40.00	249.0
41.80	86.0
43.10	143.0
44.00	1017.0
45.00	660.0
46.20	153.0
46.90	774.0
47.80	597.0
49.00	3817.0
50.00	16456.0
51.00	4598.0
52.00	412.0
53.20	164.0
55.00	359.0
56.00	1832.0
57.00	2990.0
57.90	247.0
58.90	81.0
59.90	905.0
61.00	4823.0
62.00	4495.0
63.00	3977.0
64.00	565.0
64.90	500.0
66.00	86.0
67.10	269.0
68.00	9320.0
69.00	9325.0
70.00	908.0
71.00	109.0
72.00	594.0
73.00	4688.0
74.00	16456.0
75.00	44360.0
76.00	4522.0
77.00	590.0
78.90	4598.0
79.90	1306.0
81.00	4050.0
81.90	1125.0
82.90	215.0
85.80	103.0
86.90	3583.0
87.90	3418.0
89.00	84.0
90.90	463.0
92.00	2957.0
93.10	4303.0
94.00	11939.0
95.00	82800.0
96.10	5450.0
97.00	391.0
103.90	661.0
105.00	267.0
105.90	452.0
106.90	82.0
109.90	66.0
110.80	86.0
111.80	168.0
112.80	116.0
114.80	127.0
115.00	128.0
115.90	341.0
116.90	1011.0
118.00	316.0
118.90	801.0
123.90	56.0
124.80	81.0
125.60	112.0
126.10	95.0
128.20	247.0
129.00	165.0
129.90	381.0
130.90	199.0
133.00	301.0
133.80	57.0
134.10	54.0
134.80	186.0
136.90	271.0
138.50	87.0
139.80	133.0
141.00	1199.0
141.90	175.0
142.80	1218.0
145.00	528.0
145.80	365.0
147.00	89.0
148.00	480.0

Instrument :
MSVOA_W
ClientSampleId :
BFB574

148.80	109.0
150.10	172.0
152.10	102.0
153.80	70.0
154.70	144.0
155.10	274.0
156.50	68.0
156.90	105.0
158.60	87.0
159.20	105.0
161.00	180.0
163.00	68.0
168.30	121.0
169.10	99.0
170.00	149.0
170.90	273.0
172.00	1172.0
173.00	1545.0
174.00	59320.0
175.00	4636.0
176.00	60288.0
177.10	3195.0
177.90	143.0
178.90	107.0
191.10	280.0
192.20	82.0
193.00	467.0
194.10	68.0
206.80	184.0
207.20	187.0
208.00	58.0
248.70	84.0
249.20	63.0
249.80	100.0
250.90	72.0
252.70	86.0
265.30	240.0
266.90	113.0
281.20	2082.0
282.20	713.0
283.20	317.0
284.20	125.0
285.30	53.0

Instrument :
MSVOA_W
ClientSampleId :
BFB574

m/z	Abundance
35.20	53.0
36.00	865.0
37.00	5031.0
38.00	4178.0
39.00	1423.0
40.10	306.0
40.90	106.0
42.00	129.0
44.00	1012.0
45.00	677.0
46.20	116.0
47.00	848.0
48.10	695.0
49.00	3606.0
50.00	15539.0
51.00	5584.0
52.10	228.0
53.20	192.0
54.90	305.0
56.00	1452.0
57.10	2753.0
57.90	219.0
59.10	89.0
59.90	978.0
61.00	4257.0
62.00	5018.0
63.00	3751.0
64.20	507.0
65.20	423.0
66.10	154.0
66.80	272.0
68.00	9479.0
69.00	9512.0
70.00	1052.0
70.90	52.0
72.10	542.0
73.00	4066.0
74.00	16116.0
75.00	45544.0
76.00	3701.0
76.90	546.0
77.80	530.0
78.90	4603.0
79.90	1284.0
80.90	4991.0
81.90	1016.0
82.90	178.0
83.30	86.0
85.80	223.0
86.90	2990.0
87.90	2916.0
90.90	535.0
92.00	2932.0
93.00	4860.0
94.00	11244.0
95.00	84344.0
96.10	5177.0
97.00	262.0
103.10	81.0
103.90	457.0
104.90	203.0
105.90	380.0
106.70	80.0
109.70	99.0
111.10	236.0
111.80	189.0
112.80	157.0
115.00	193.0
116.00	493.0
116.90	736.0
117.90	468.0
118.90	612.0
119.90	90.0
121.00	51.0
124.00	88.0
125.70	140.0
128.00	454.0
128.90	167.0
129.80	468.0
131.00	123.0
133.10	161.0
133.80	80.0
134.10	81.0
134.90	269.0
137.00	241.0
138.60	70.0
138.90	69.0
139.90	85.0
140.90	1027.0
142.00	176.0
143.00	1312.0
144.90	261.0

Instrument :
MSVOA_W
ClientSampleId :
BFB574

146.10	91.0
147.00	58.0
147.80	141.0
148.70	87.0
150.00	205.0
152.80	109.0
153.80	73.0
154.90	168.0
156.50	99.0
157.00	130.0
159.10	111.0
161.00	135.0
168.40	59.0
169.20	93.0
169.80	152.0
171.10	273.0
172.10	853.0
173.90	60112.0
175.00	4818.0
176.00	61136.0
176.90	3807.0
178.10	113.0
193.00	161.0
193.70	101.0
207.10	202.0
208.00	133.0
249.20	78.0
250.00	137.0
265.10	102.0
281.20	1255.0
282.30	371.0
282.90	222.0
284.20	61.0

Instrument :
MSVOA_W
ClientSampleId :
BFB574

m/z	Abundance
36.10	477.0
37.00	2498.0
38.00	2930.0
39.10	1348.0
40.00	259.0
41.10	66.0
41.60	54.0
43.10	153.0
44.00	772.0
44.90	517.0
46.20	157.0
46.90	814.0
47.90	360.0
49.00	2468.0
50.00	11011.0
51.10	3186.0
51.90	299.0
52.80	120.0
53.10	81.0
54.90	299.0
56.00	1159.0
57.00	2015.0
58.80	55.0
60.00	732.0
61.00	2736.0
62.00	2937.0
63.10	2410.0
64.10	332.0
65.00	291.0
66.20	134.0
68.10	6437.0
69.00	5449.0
70.00	415.0
72.00	553.0
73.00	2965.0
74.00	11780.0
75.00	29720.0
76.00	2597.0
77.00	497.0
77.90	481.0
78.90	3282.0
80.00	905.0
80.90	3250.0
81.80	624.0
83.00	148.0
84.00	68.0
85.70	168.0
86.10	143.0
86.90	2402.0
87.90	1948.0
90.90	357.0
92.00	2014.0
93.00	2815.0
94.00	8306.0
95.00	55232.0
96.00	3562.0
97.00	258.0
103.10	54.0
103.80	342.0
105.00	204.0
106.00	366.0
106.90	68.0
109.80	89.0
110.90	103.0
111.80	97.0
113.20	51.0
115.10	148.0
115.80	256.0
116.90	505.0
118.20	265.0
118.90	360.0
119.80	61.0
125.80	140.0
128.00	299.0
129.00	193.0
129.70	264.0
130.70	112.0
133.00	164.0
134.90	179.0
137.00	213.0
138.90	73.0
139.90	84.0
140.90	1081.0
141.90	140.0
143.10	949.0
145.00	210.0
146.20	65.0
146.80	103.0
147.80	161.0
149.80	91.0
155.00	162.0
157.00	153.0

Instrument :
MSVOA_W
ClientSampleId :
BFB574

158.80	58.0
160.80	66.0
165.80	83.0
168.20	82.0
169.70	86.0
171.10	261.0
171.90	679.0
172.50	596.0
174.00	50808.0
175.00	4565.0
176.00	49184.0
177.00	3392.0
178.00	103.0
193.00	96.0
202.70	63.0
207.10	116.0
208.30	66.0
281.20	532.0
282.30	161.0
283.30	142.0

Instrument :
MSVOA_W
ClientSampleId :
BFB574