




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062123\
 Data File : VW026288.D
 Acq On : 21 Jun 2023 16:47
 Operator : SY/MD
 Sample : 03234-21
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Quant Time: Jun 22 01:36:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 22 01:33:30 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 06/22/2023
 Supervised By :Mahesh Dadoda 06/22/2023

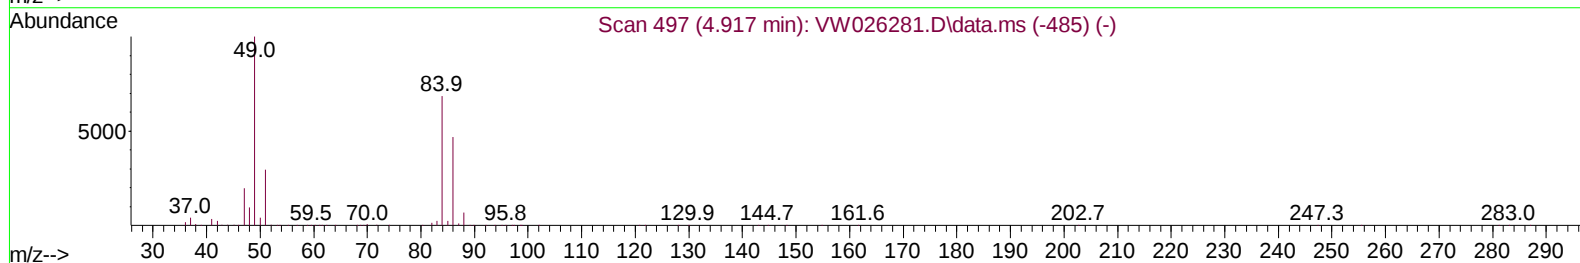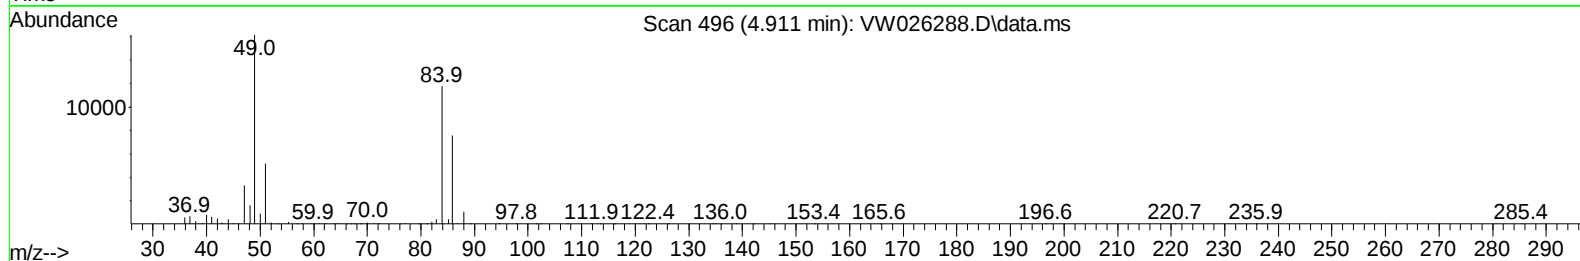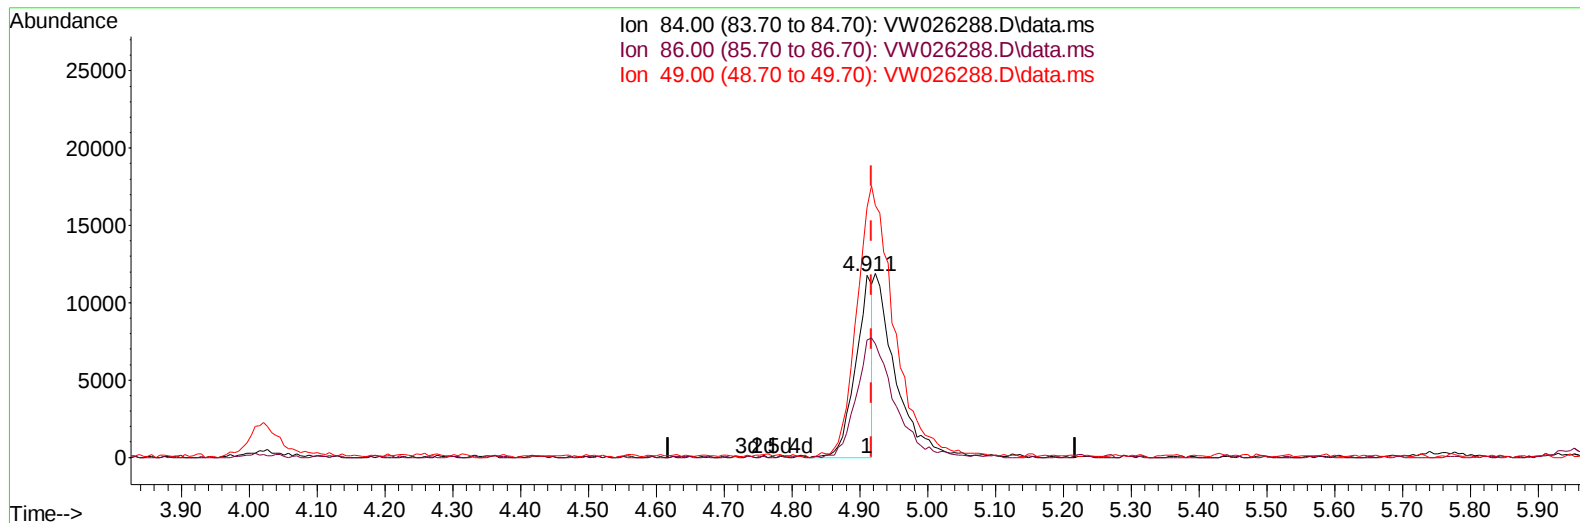

TIC: VW026288.D\data.ms

(16) Methylene chloride (T)

4.911min (-0.006) 2.07 ug/L

response 20307

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.10	64.58
49.00	141.20	137.30
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062123\
 Data File : VW026288.D
 Acq On : 21 Jun 2023 16:47
 Operator : SY/MD
 Sample : 03234-21
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/22/2023
 Supervised By :Mahesh Dadoda 06/22/2023

Quant Time: Jun 22 01:36:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 22 01:33:30 2023
 Response via : Initial Calibration

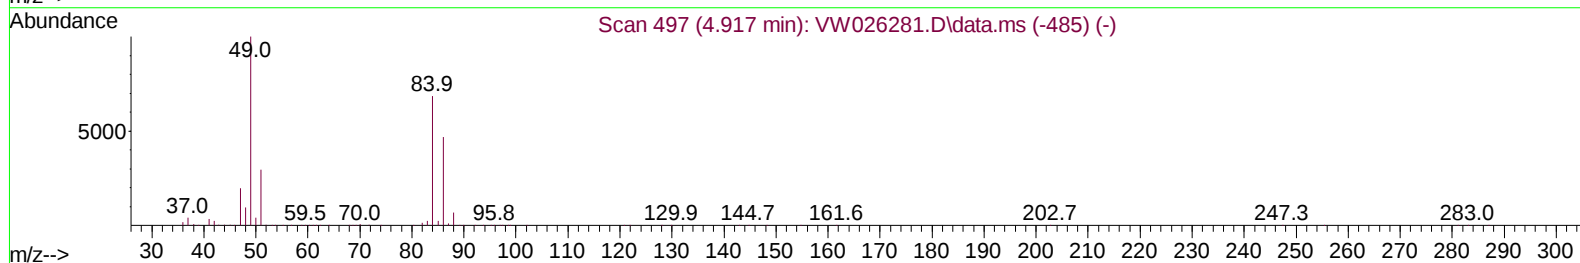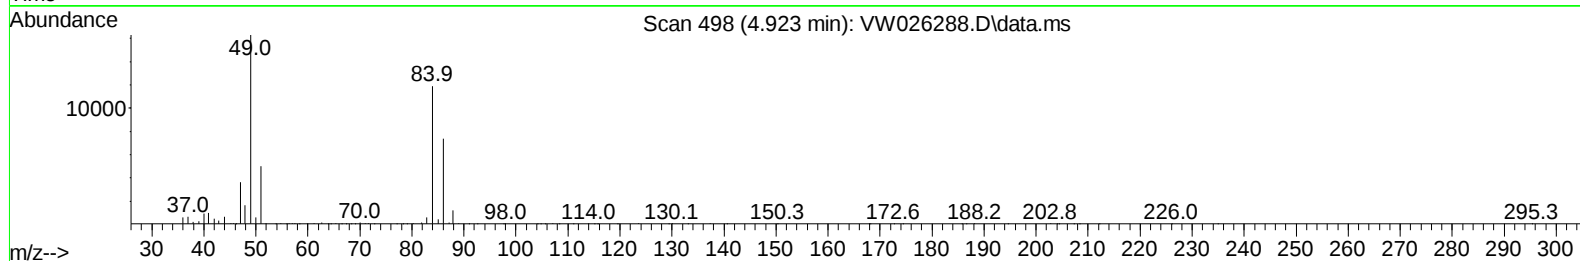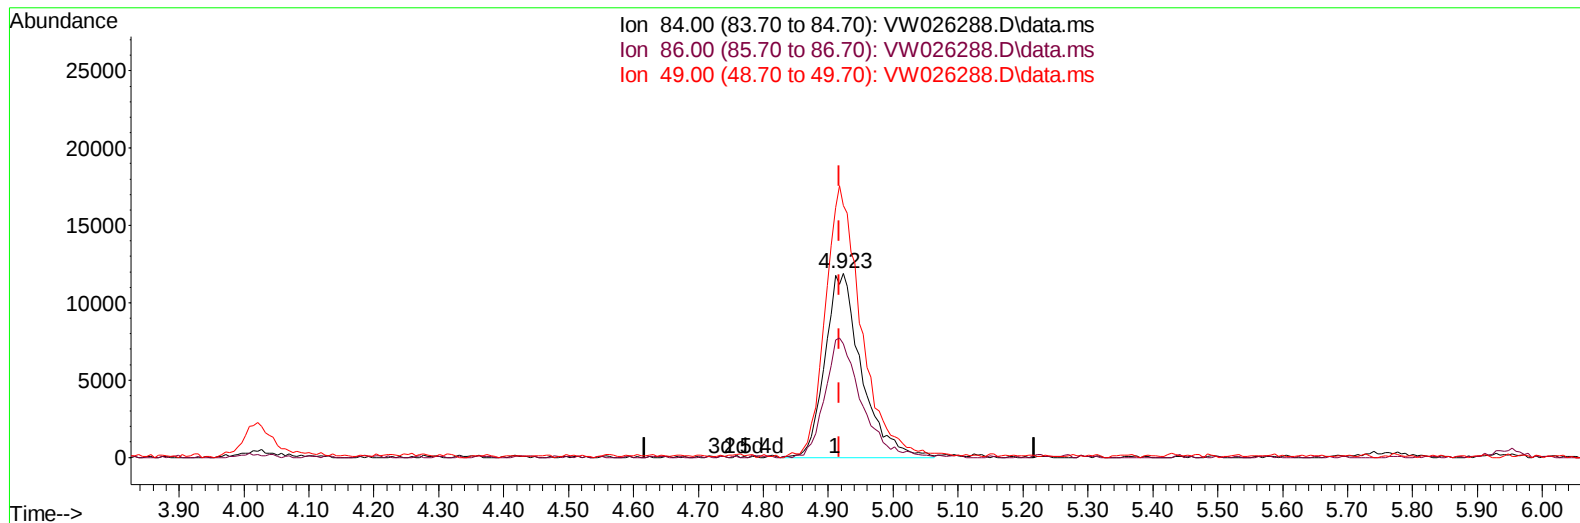

TIC: VW026288.D\data.ms

(16) Methylene chloride (T)

4.923min (+ 0.006) 4.75 ug/L m

response 46615

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	63.10	61.75
49.00	141.20	136.89
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062123\
 Data File : VW026288.D
 Acq On : 21 Jun 2023 16:47
 Operator : SY/MD
 Sample : 03234-21
 Misc : 5.01g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/22/2023
 Supervised By :Mahesh Dadoda 06/22/2023

Quant Time: Jun 22 01:36:12 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Jun 22 01:33:30 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	614745	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	564608	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	259227	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	141521	16.364	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	65.440%	
7) Chloroethane-d5	2.893	69	137083	21.175	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	84.680%	
11) 1,1-Dichloroethene-d2	4.021	65	75685	17.748	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	71.000%	
21) 2-Butanone-d5	7.075	46	146233	58.080	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	116.160%	
24) Chloroform-d	7.648	84	372638	20.700	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	82.800%	
26) 1,2-Dichloroethane-d4	8.301	65	220068	22.356	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	89.440%	
32) Benzene-d6	8.276	84	720047	18.953	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	75.800%	
36) 1,2-Dichloropropane-d6	9.270	67	250043	20.774	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	83.080%	
41) Toluene-d8	10.325	98	583448	17.317	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	69.280%	
43) trans-1,3-Dichloroprop...	10.581	79	85126	17.848	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	71.400%	
47) 2-Hexanone-d5	10.922	63	95508	50.324	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	100.640%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	217278	24.807	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	99.240%	
66) 1,2-Dichlorobenzene-d4	13.848	152	206815	20.844	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	83.360%	
Target Compounds						
16) Methylene chloride	4.923	84	46615m	4.751	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062123\
Data File : VW026288.D
Acq On : 21 Jun 2023 16:47
Operator : SY/MD
Sample : 03234-21
Misc : 5.01g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VHBLK001

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 06/22/2023
Supervised By :Mahesh Dadoda 06/22/2023

Quant Time: Jun 22 01:36:12 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM053023SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Jun 22 01:33:30 2023
Response via : Initial Calibration

