

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062124\
 Data File : VW029307.D
 Acq On : 21 Jun 2024 17:10
 Operator : SY/MD
 Sample : P2982-08
 Misc : 5.27g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Jun 21 22:57:52 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 21 22:53:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	467499	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	389181	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	130177	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	121276	18.742	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.960%
7) Chloroethane-d5	2.899	69	110718	20.262	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.040%
11) 1,1-Dichloroethene-d2	4.021	65	60094	19.235	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	76.920%
21) 2-Butanone-d5	7.075	46	83703	43.237	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.480%
24) Chloroform-d	7.648	84	298600	21.412	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	85.640%
26) 1,2-Dichloroethane-d4	8.307	65	167585	20.930	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	83.720%
32) Benzene-d6	8.276	84	561213	23.741	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.960%
36) 1,2-Dichloropropane-d6	9.270	67	186860	24.867	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.480%
41) Toluene-d8	10.325	98	465568	22.261	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.040%
43) trans-1,3-Dichloroprop...	10.575	79	59098	19.517	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.080%
47) 2-Hexanone-d5	10.922	63	52092	44.222	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.440%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	130858	21.881	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	87.520%
66) 1,2-Dichlorobenzene-d4	13.848	152	108920	24.105	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.440%
Target Compounds						Qvalue
39) cis-1,3-Dichloropropene	10.032	75	4501	0.485	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062124\
Data File : VW029307.D
Acq On : 21 Jun 2024 17:10
Operator : SY/MD
Sample : P2982-08
Misc : 5.27g/10mL/MSVOA_W/SOIL/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Jun 21 22:57:52 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 21 22:53:01 2024
Response via : Initial Calibration

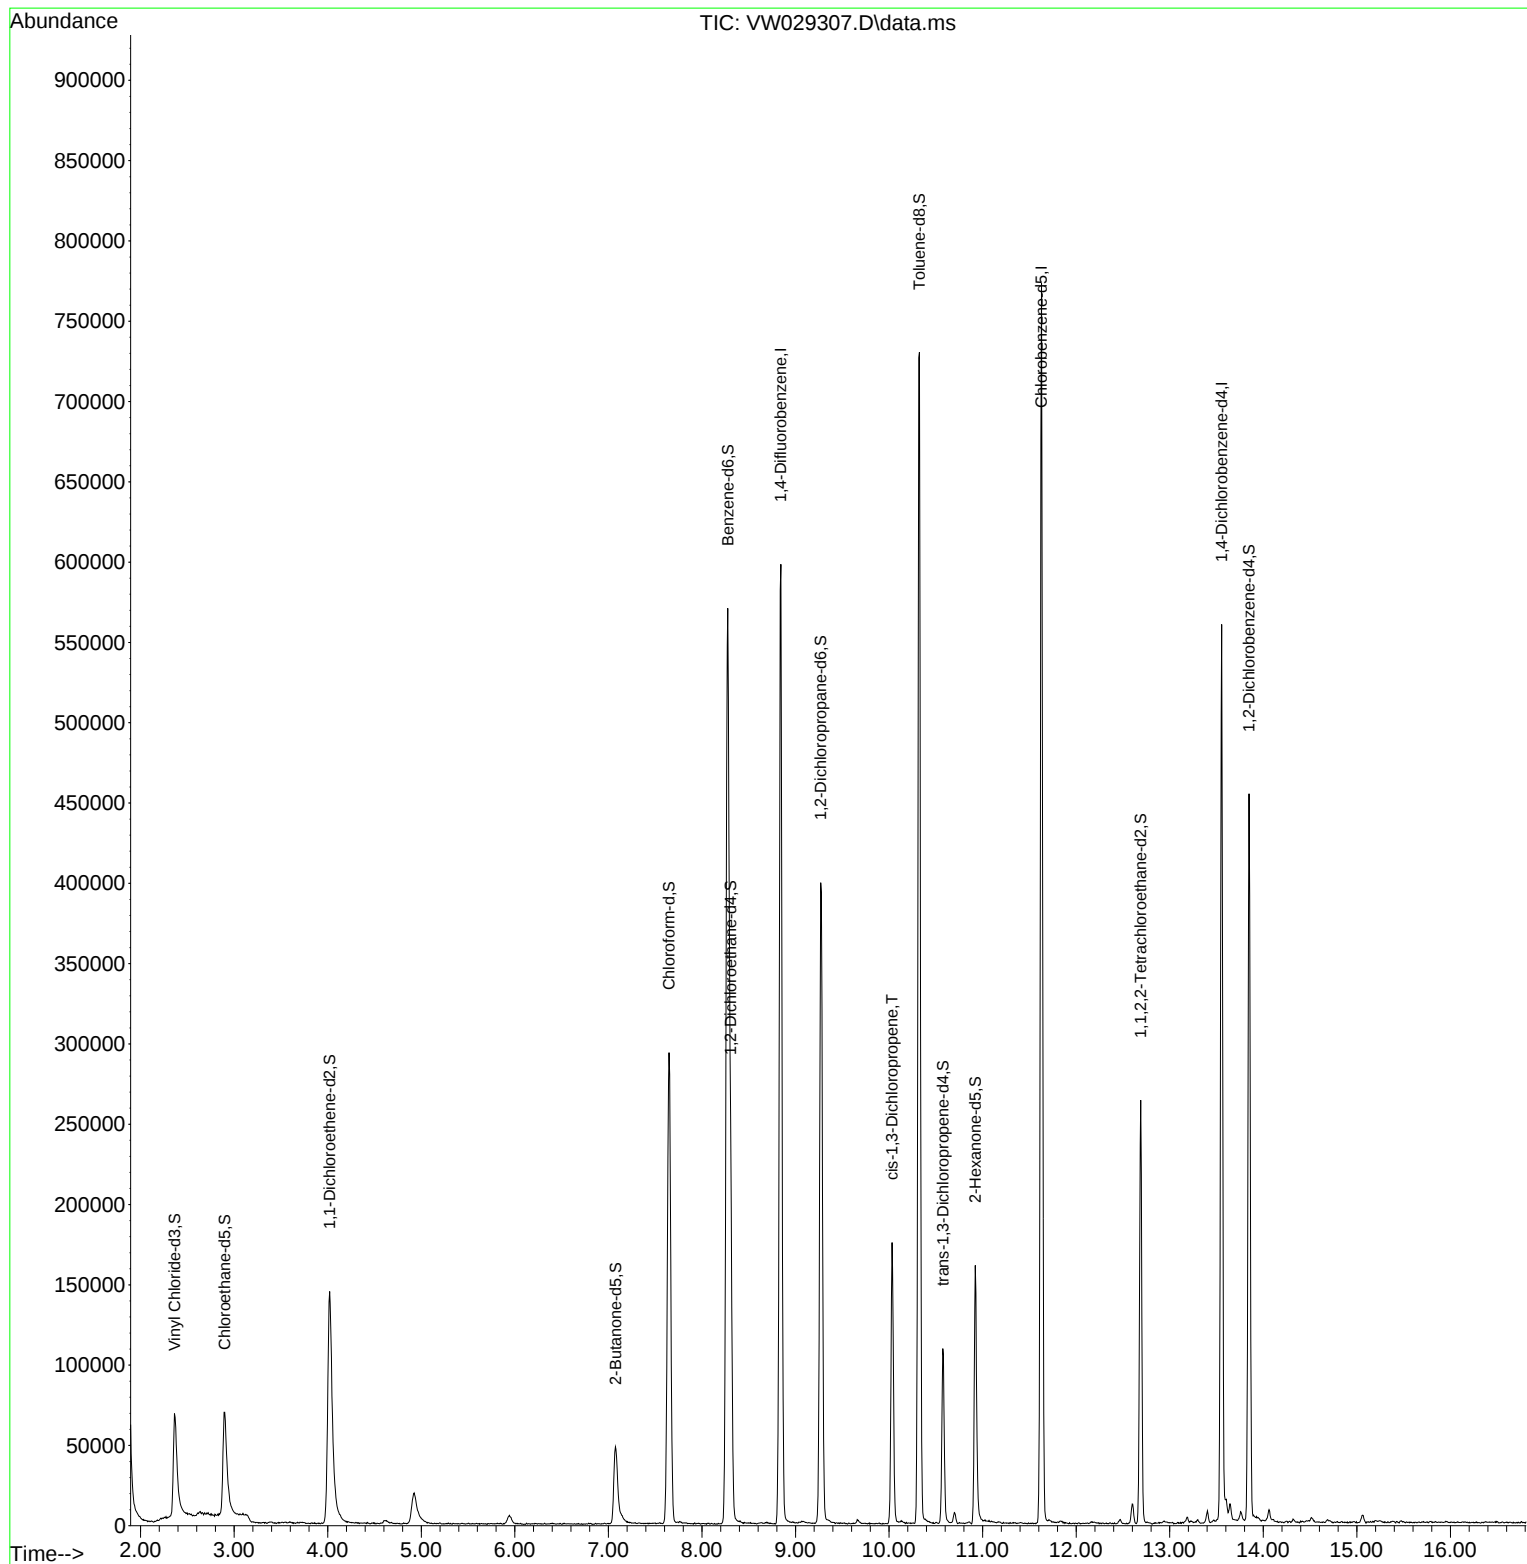

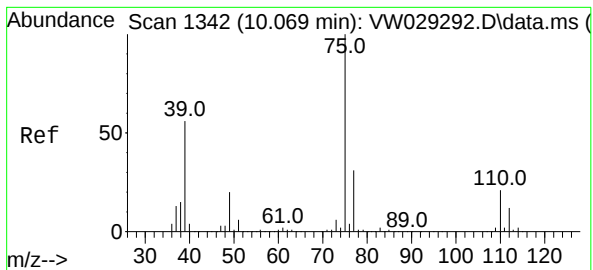

#39
 cis-1,3-Dichloropropene
 Concen: 0.485 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.037 min
 Lab File: VW029307.D
 Acq: 21 Jun 2024 17:10

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion:	75	Resp:	4501
Ion Ratio	Lower	Upper	
75	100		
77	40.7	22.7	42.1

