

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062124\
 Data File : VW029303.D
 Acq On : 21 Jun 2024 15:34
 Operator : SY/MD
 Sample : VIBLK473
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK473

Quant Time: Jun 21 22:56:57 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 21 22:53:01 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	294714	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	275268	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	120450	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	90013	22.066	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	88.280%		
7) Chloroethane-d5	2.899	69	69878	20.285	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	81.160%		
11) 1,1-Dichloroethene-d2	4.021	65	43803	22.240	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	88.960%		
21) 2-Butanone-d5	7.075	46	59176	48.488	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	96.980%		
24) Chloroform-d	7.648	84	184162	20.948	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	83.800%		
26) 1,2-Dichloroethane-d4	8.301	65	111510	22.092	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	88.360%		
32) Benzene-d6	8.276	84	380289	22.745	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	90.960%		
36) 1,2-Dichloropropane-d6	9.270	67	121335	22.829	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	91.320%		
41) Toluene-d8	10.319	98	338591	22.889	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	91.560%		
43) trans-1,3-Dichloroprop...	10.575	79	47284	22.077	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	88.320%		
47) 2-Hexanone-d5	10.922	63	40891	49.079	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	98.160%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	96059	22.709	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	90.840%		
66) 1,2-Dichlorobenzene-d4	13.848	152	106551	25.485	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	101.960%		
Target Compounds						Qvalue
16) Methylene chloride	4.923	84	21215	4.094	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW062124\
Data File : VW029303.D
Acq On : 21 Jun 2024 15:34
Operator : SY/MD
Sample : VIBLK473
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK473

Quant Time: Jun 21 22:56:57 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM061824SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 21 22:53:01 2024
Response via : Initial Calibration

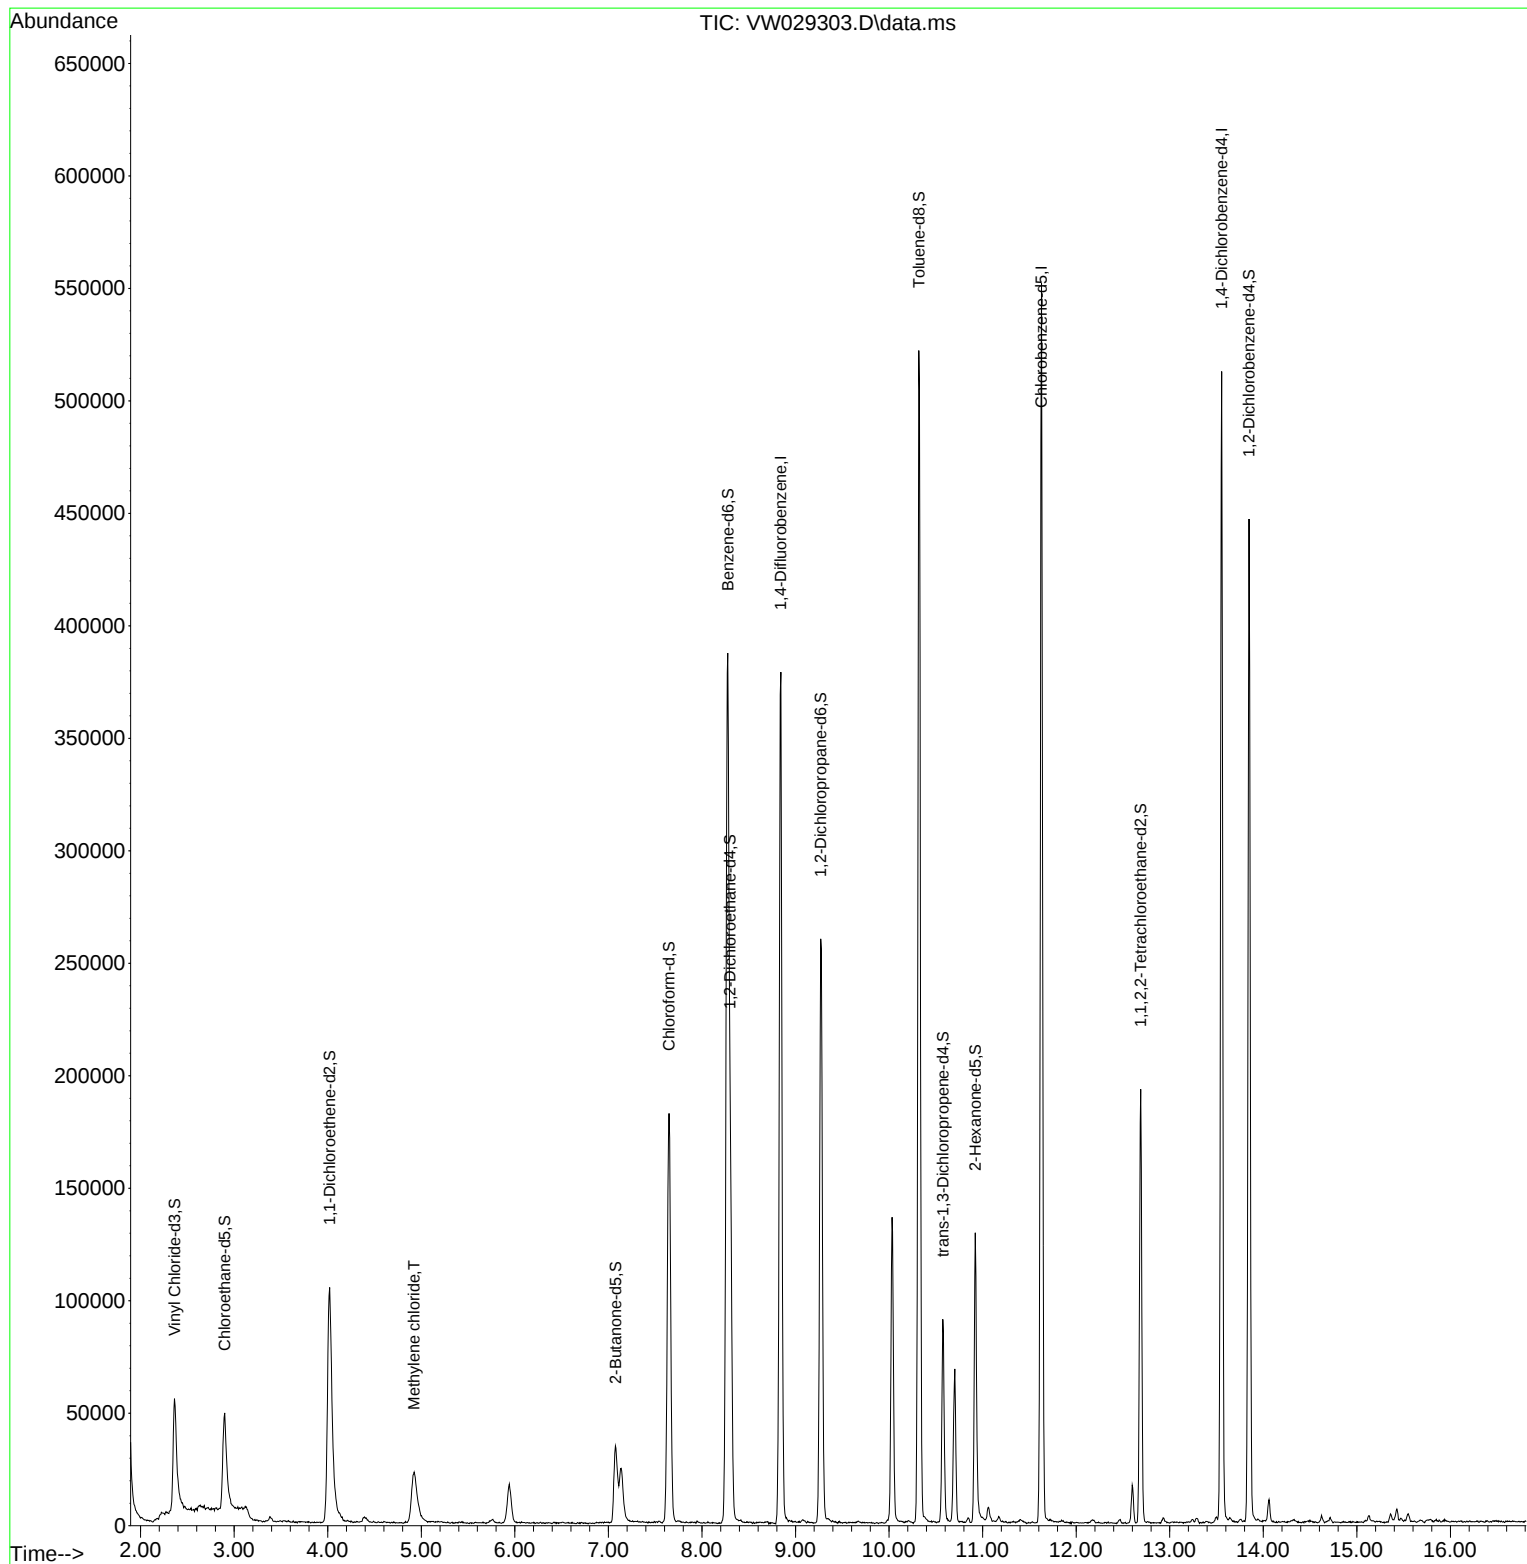

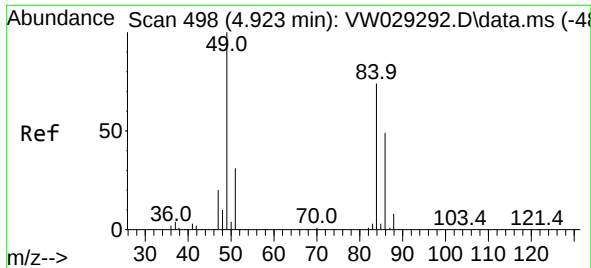

#16
Methylene chloride
Concen: 4.094 ug/L
RT: 4.923 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW029303.D
Acq: 21 Jun 2024 15:34

Instrument :
MSVOA_W
ClientSampleId :
VIBLK473

Tgt Ion: 84 Resp: 21215
Ion Ratio Lower Upper
84 100
86 59.4 41.4 77.0
49 132.7 95.7 177.7

