


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW062220\
 Data File : VW015642.D
 Acq On : 22 Jun 2020 10:22
 Operator : SY/VA
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W060220S.M
 Title : SW846 8260
 Last Update : Tue Jun 02 13:57:56 2020

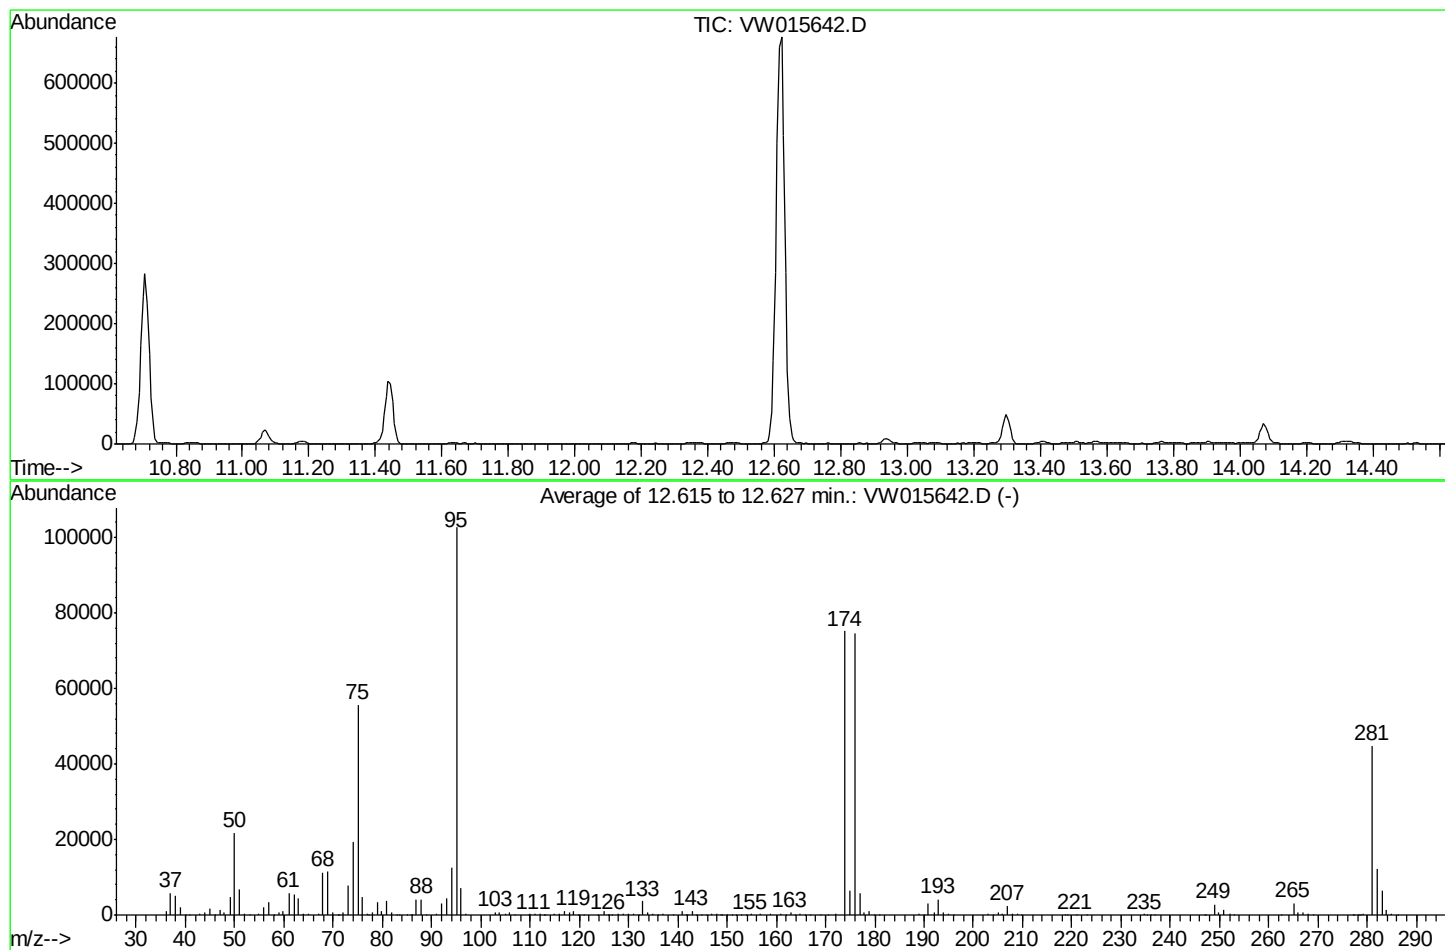

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1748

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	21768	PASS
75	95	30	60	54.2	55666	PASS
95	95	100	100	100.0	102669	PASS
96	95	5	9	6.9	7091	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	73.2	75138	PASS
175	174	5	9	8.4	6296	PASS
176	174	95	101	99.3	74629	PASS
177	176	5	9	7.8	5791	PASS

m/z	Abundance
36.00	1435.0
37.00	6248.0
38.00	6039.0
39.00	2428.0
39.90	254.0
43.00	324.0
44.00	985.0
45.00	1934.0
46.00	178.0
47.00	1630.0
47.90	655.0
49.00	5204.0
50.00	22984.0
51.00	6898.0
52.00	357.0
53.00	90.0
54.90	420.0
56.00	2052.0
57.00	3527.0
57.90	188.0
58.90	915.0
59.90	1225.0
61.00	6092.0
62.00	5741.0
63.00	4696.0
63.90	417.0
65.00	374.0
66.90	331.0
67.90	11564.0
69.00	12195.0
70.00	774.0
71.00	106.0
72.00	687.0
73.00	10224.0
74.00	20104.0
75.00	56896.0
76.00	4798.0
76.80	578.0
77.90	462.0
78.90	3719.0
79.90	1030.0
80.90	4122.0
81.80	886.0
83.00	140.0
83.50	125.0
85.10	129.0
85.80	137.0
86.90	3983.0
87.90	4127.0
88.80	354.0
90.90	468.0
92.00	2987.0
93.00	4549.0
94.00	12615.0
95.00	100960.0
96.00	7599.0
96.90	316.0
102.90	1114.0
103.80	858.0
105.00	323.0
105.90	581.0
106.90	123.0
110.10	400.0
110.90	407.0
111.90	320.0
112.80	166.0
114.90	519.0
115.90	547.0
116.90	1020.0
117.90	893.0
118.90	1595.0
120.00	208.0
121.00	214.0
123.70	63.0
125.00	1457.0
125.90	515.0
126.70	85.0
127.90	365.0
128.90	206.0
129.80	345.0
131.00	224.0
132.00	187.0
132.90	5675.0
133.80	1314.0
134.90	519.0
135.90	88.0
136.90	155.0
139.10	61.0
140.90	878.0
142.00	170.0
142.90	1114.0
143.80	90.0

Instrument :
MSVOA_W
ClientSampleId :
BFB

144.80	232.0
145.90	166.0
146.90	796.0
147.80	376.0
148.80	395.0
149.90	164.0
151.00	89.0
152.90	54.0
153.70	61.0
155.00	247.0
156.90	211.0
158.90	224.0
160.90	490.0
161.90	179.0
162.90	926.0
163.90	199.0
164.90	708.0
165.90	120.0
166.80	73.0
168.90	80.0
170.50	51.0
171.90	426.0
173.90	67664.0
174.90	6065.0
175.90	66768.0
177.00	6165.0
177.90	804.0
178.90	1540.0
179.90	230.0
180.90	142.0
189.00	551.0
189.90	230.0
190.90	4540.0
192.00	1035.0
193.00	6838.0
193.90	1331.0
195.00	779.0
195.90	103.0
203.00	499.0
203.90	181.0
205.00	1257.0
206.00	383.0
207.00	4017.0
208.10	594.0
208.90	452.0
209.80	85.0
219.00	119.0
220.90	246.0
222.90	97.0
234.80	665.0
236.00	187.0
236.90	197.0
247.00	138.0
248.90	4214.0
249.90	1194.0
250.90	1915.0
252.00	437.0
253.00	231.0
262.60	66.0
265.00	4412.0
265.90	1219.0
266.90	1037.0
268.00	280.0
269.10	113.0
277.10	103.0
278.10	136.0
279.20	445.0
281.00	62032.0
282.00	18384.0
283.00	8357.0
284.00	2158.0
285.00	729.0
286.00	110.0

Instrument :
MSVOA_W
ClientSampleId :
BFB

m/z	Abundance
35.10	70.0
36.00	1410.0
37.00	6666.0
38.00	5738.0
39.00	2379.0
40.00	223.0
40.80	63.0
43.00	237.0
44.00	1134.0
45.00	1664.0
45.90	129.0
47.00	1310.0
47.90	796.0
49.00	5288.0
50.00	23616.0
51.00	7368.0
52.00	310.0
53.00	99.0
54.80	315.0
56.00	2331.0
57.00	3645.0
58.00	158.0
59.00	623.0
59.90	1258.0
61.00	6493.0
62.00	6169.0
63.00	4942.0
64.00	388.0
65.00	309.0
67.00	321.0
68.00	12622.0
69.00	12965.0
70.00	972.0
71.00	118.0
71.90	689.0
73.00	8287.0
74.00	21200.0
75.00	62688.0
76.00	5194.0
76.90	657.0
77.80	372.0
78.00	370.0
78.90	3780.0
79.90	1194.0
80.90	4120.0
81.80	894.0
83.10	104.0
85.10	72.0
86.00	139.0
86.90	4277.0
87.90	4393.0
90.90	556.0
92.00	3213.0
92.90	4941.0
94.00	13976.0
95.00	114176.0
96.00	7668.0
96.90	299.0
103.00	479.0
103.80	758.0
104.80	312.0
105.90	554.0
106.90	157.0
110.00	251.0
110.90	292.0
111.90	181.0
113.00	142.0
115.00	270.0
115.90	469.0
116.90	823.0
117.90	799.0
118.90	1218.0
119.90	105.0
120.80	145.0
124.90	766.0
127.90	358.0
128.90	209.0
129.90	434.0
130.80	212.0
131.90	120.0
132.90	3549.0
133.90	729.0
134.90	518.0
135.80	76.0
136.90	223.0
139.10	59.0
140.80	1122.0
141.70	170.0
142.90	1126.0
143.80	95.0
144.90	163.0
145.70	202.0

Instrument :
MSVOA_W
ClientSampleId :
BFB

146.90	514.0
147.80	376.0
149.00	209.0
149.80	143.0
151.80	63.0
152.90	111.0
153.80	74.0
154.80	343.0
156.90	220.0
158.80	244.0
160.90	356.0
161.70	89.0
162.90	572.0
163.70	119.0
164.90	449.0
165.90	70.0
166.80	59.0
170.60	58.0
172.00	521.0
173.90	81152.0
175.00	7408.0
175.90	85944.0
176.90	6035.0
177.90	565.0
178.90	828.0
180.00	151.0
180.90	124.0
189.00	441.0
190.90	2838.0
192.00	642.0
192.90	3869.0
193.90	802.0
194.90	481.0
196.00	75.0
203.00	371.0
204.00	78.0
204.90	794.0
206.00	237.0
207.00	2362.0
207.90	475.0
208.90	338.0
219.00	142.0
220.80	176.0
235.10	438.0
235.80	88.0
236.70	88.0
247.20	93.0
248.90	3001.0
249.90	613.0
250.80	1248.0
252.00	303.0
253.00	167.0
265.00	3470.0
265.90	821.0
267.00	905.0
267.90	218.0
277.00	96.0
277.90	115.0
281.00	50152.0
282.00	12621.0
283.00	7040.0
283.90	1348.0
285.00	519.0
286.10	63.0

Instrument :
MSVOA_W
ClientSampleId :
BFB

m/z	Abundance
36.00	1105.0
37.00	4831.0
38.00	4069.0
39.00	1675.0
39.90	230.0
40.90	80.0
43.00	149.0
44.00	824.0
45.00	1160.0
45.90	85.0
47.00	1094.0
47.90	653.0
49.00	3988.0
50.00	18704.0
51.00	5609.0
52.00	258.0
54.90	332.0
55.90	1509.0
57.00	2731.0
57.90	125.0
59.10	236.0
59.90	1048.0
61.00	4809.0
62.00	4692.0
63.00	3466.0
64.00	405.0
64.90	185.0
67.00	274.0
68.00	9784.0
69.00	9846.0
70.00	721.0
71.20	52.0
71.90	564.0
73.00	5221.0
74.00	16808.0
75.00	47416.0
76.00	4064.0
77.10	523.0
77.90	475.0
78.90	3151.0
79.90	1005.0
80.90	3361.0
81.90	763.0
82.90	95.0
85.80	127.0
86.90	3699.0
87.90	4044.0
90.80	451.0
92.00	2974.0
93.00	4219.0
94.00	11098.0
95.00	92872.0
96.00	6006.0
97.00	213.0
102.90	473.0
103.80	413.0
104.90	235.0
105.80	492.0
106.90	118.0
109.80	87.0
110.80	192.0
112.00	161.0
113.00	88.0
115.00	159.0
115.90	392.0
116.90	751.0
117.80	466.0
118.90	727.0
119.70	86.0
124.90	429.0
126.10	91.0
127.90	355.0
128.90	174.0
129.90	368.0
131.00	161.0
132.10	118.0
132.90	1500.0
133.90	197.0
135.00	276.0
135.90	66.0
136.90	239.0
140.90	943.0
142.00	92.0
142.90	1046.0
143.70	53.0
144.80	137.0
145.70	147.0
146.80	193.0
147.90	284.0
149.00	120.0
149.90	104.0
152.80	98.0

Instrument :
MSVOA_W
ClientSampleId :
BFB

154.80	163.0
156.80	190.0
158.70	94.0
160.80	209.0
162.80	293.0
164.90	294.0
170.70	59.0
172.00	322.0
173.90	76600.0
175.00	5416.0
175.90	71176.0
176.90	5174.0
178.00	352.0
178.80	386.0
179.80	62.0
181.00	60.0
188.80	176.0
190.00	68.0
190.90	1394.0
191.90	335.0
193.00	1947.0
193.90	353.0
194.90	203.0
203.00	167.0
204.90	343.0
205.80	90.0
206.90	1182.0
207.80	263.0
208.90	102.0
218.70	55.0
221.00	58.0
234.80	130.0
248.90	1383.0
249.90	301.0
250.90	507.0
252.00	139.0
265.00	1597.0
265.90	446.0
266.90	356.0
268.10	75.0
277.40	55.0
278.30	83.0
278.70	106.0
279.30	159.0
280.90	22424.0
281.90	5816.0
283.00	4105.0
284.00	554.0
284.80	248.0
286.10	62.0

Instrument :
MSVOA_W
ClientSampleId :
BFB

Scan 1748 (12.560 min): VW015642.D
BFB

m/z	Abundance
35.20	72.0
36.00	181.0
37.80	106.0
39.90	149.0
41.10	90.0
42.10	98.0
43.90	219.0
55.00	72.0
68.80	52.0

Instrument :
MSVOA_W
ClientSampleId :
BFB